


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052424\
Data File : VU058963.D
Acq On : 24 May 2024 10:12
Operator : MD/SY
Sample : BFB052
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB052

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis
Last Update : Fri May 24 22:25:41 2024

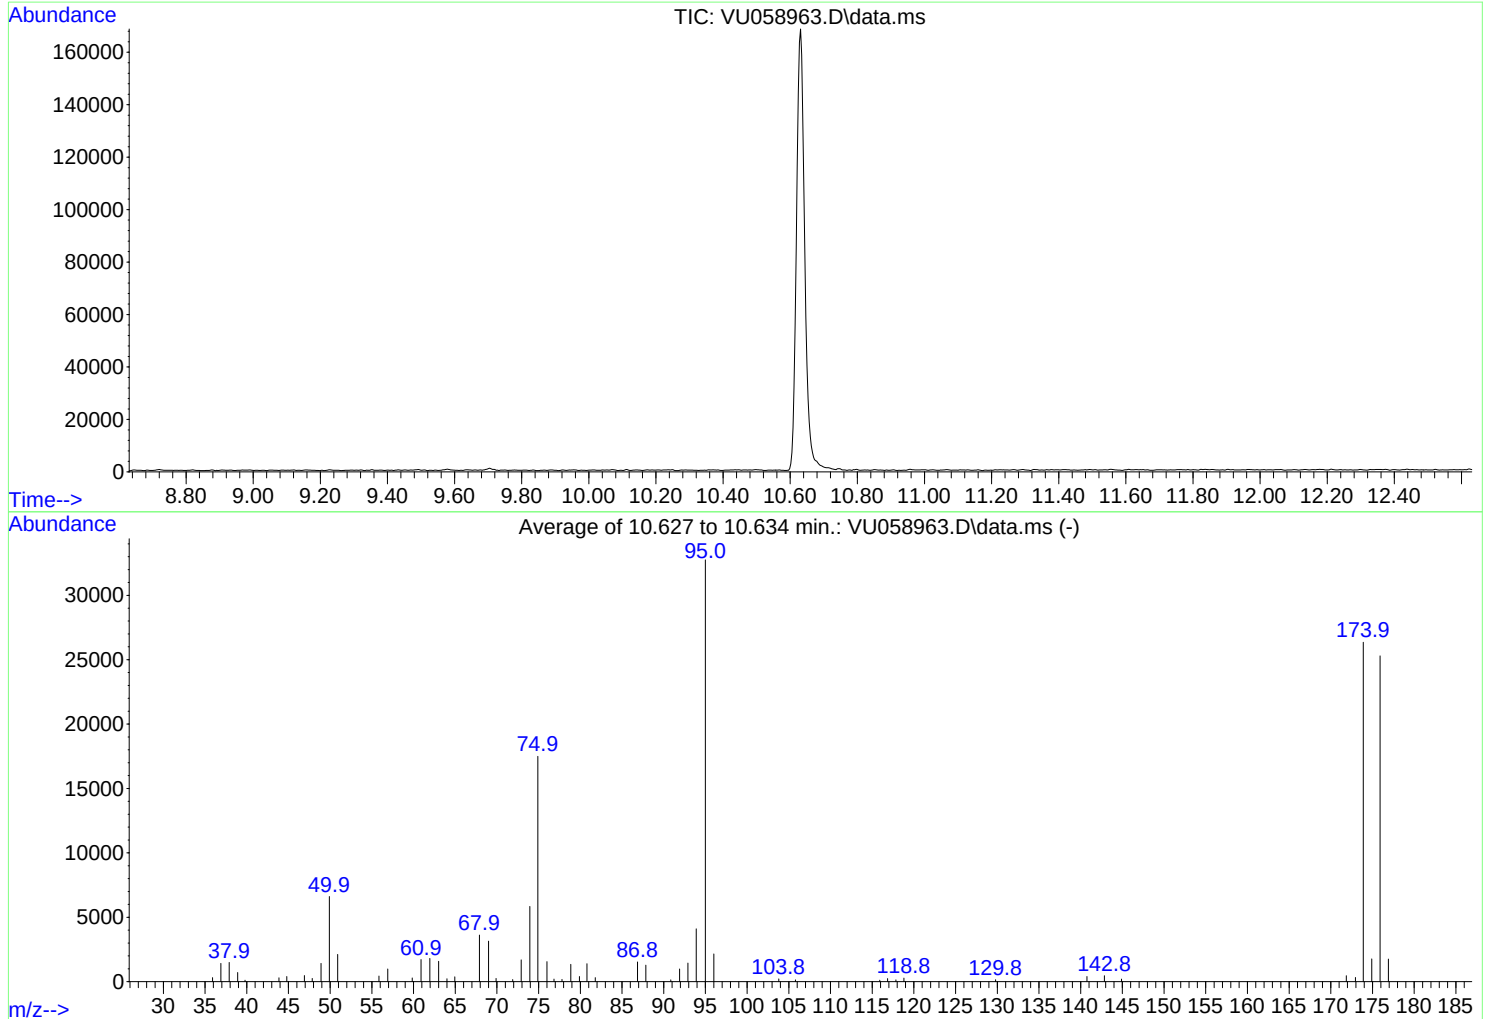

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	6613	PASS
75	95	30	80	53.4	17499	PASS
95	95	100	100	100.0	32755	PASS
96	95	5	9	6.6	2152	PASS
173	174	0.00	2	1.2	319	PASS
174	95	50	120	80.5	26355	PASS
175	174	5	9	6.7	1760	PASS
176	174	95	101	96.0	25299	PASS
177	176	5	9	6.9	1757	PASS

m/z	Abundance
39.80	274.0
43.90	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	357.0
36.90	1478.0
37.90	1660.0
38.90	784.0
39.80	351.0
43.80	665.0
44.80	406.0
46.90	465.0
47.90	253.0
48.90	1500.0
49.90	6334.0
50.90	2116.0
55.80	400.0
56.90	1021.0
59.90	288.0
60.90	1641.0
61.90	1814.0
63.00	1439.0
64.00	247.0
65.00	404.0
67.90	3599.0
69.00	3058.0
69.90	335.0
71.90	135.0
72.90	1683.0
74.00	5845.0
74.90	17832.0
76.00	1581.0
76.90	268.0
77.80	173.0
78.80	1424.0
79.90	425.0
80.80	1357.0
81.80	330.0
86.90	1401.0
87.90	1347.0
90.80	158.0
91.90	1070.0
92.90	1402.0
93.90	4218.0
95.00	33336.0
96.00	2178.0
103.80	176.0
105.80	119.0
115.90	116.0
116.90	229.0
117.80	143.0
118.80	282.0
129.80	143.0
140.80	376.0
142.90	448.0
144.90	224.0
171.90	482.0
173.00	331.0
173.90	25720.0
174.90	1779.0
175.90	24576.0
176.90	1760.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	323.0
36.90	1447.0
37.90	1536.0
38.90	737.0
39.80	386.0
43.90	612.0
44.80	424.0
46.90	461.0
47.80	244.0
48.90	1448.0
49.90	6822.0
50.90	2150.0
55.80	418.0
56.90	1025.0
59.80	297.0
60.90	1762.0
62.00	1868.0
63.00	1660.0
64.00	220.0
65.00	368.0
67.90	3751.0
69.00	3218.0
69.90	252.0
71.90	165.0
72.90	1771.0
73.90	5965.0
74.90	18144.0
76.00	1574.0
76.90	188.0
77.80	200.0
78.80	1400.0
79.90	440.0
80.80	1460.0
81.80	319.0
86.80	1592.0
87.90	1279.0
90.90	146.0
91.90	1018.0
92.90	1453.0
93.90	4211.0
95.00	33760.0
96.00	2204.0
103.80	225.0
105.80	137.0
115.90	129.0
116.90	244.0
117.80	146.0
118.80	306.0
129.80	152.0
140.80	398.0
142.90	481.0
144.90	215.0
171.90	480.0
172.90	329.0
173.90	27120.0
174.90	1768.0
175.90	26176.0
176.90	1806.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	272.0
36.90	1315.0
37.90	1264.0
38.90	624.0
39.80	407.0
43.90	574.0
44.80	371.0
46.90	482.0
47.80	239.0
48.90	1320.0
49.90	6682.0
50.90	2086.0
55.90	484.0
56.90	916.0
59.80	291.0
60.90	1740.0
61.90	1745.0
63.00	1630.0
64.00	188.0
64.90	348.0
67.90	3517.0
69.00	3146.0
69.90	162.0
71.90	175.0
72.90	1610.0
73.90	5707.0
74.90	16520.0
76.00	1523.0
76.80	154.0
77.80	166.0
78.90	1223.0
79.90	347.0
80.80	1371.0
81.80	268.0
86.80	1591.0
87.80	1232.0
90.90	113.0
91.90	853.0
92.90	1471.0
93.90	3859.0
95.00	31168.0
96.00	2074.0
103.80	234.0
105.80	151.0
115.90	105.0
116.80	252.0
117.90	140.0
118.80	245.0
129.80	143.0
140.70	405.0
142.80	455.0
144.90	159.0
171.80	408.0
172.90	297.0
173.90	26224.0
174.90	1733.0
175.90	25144.0
176.90	1704.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052