


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052521\
 Data File : VU043965.D
 Acq On : 25 May 2021 16:10
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB135

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052521.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed May 26 16:45:31 2021

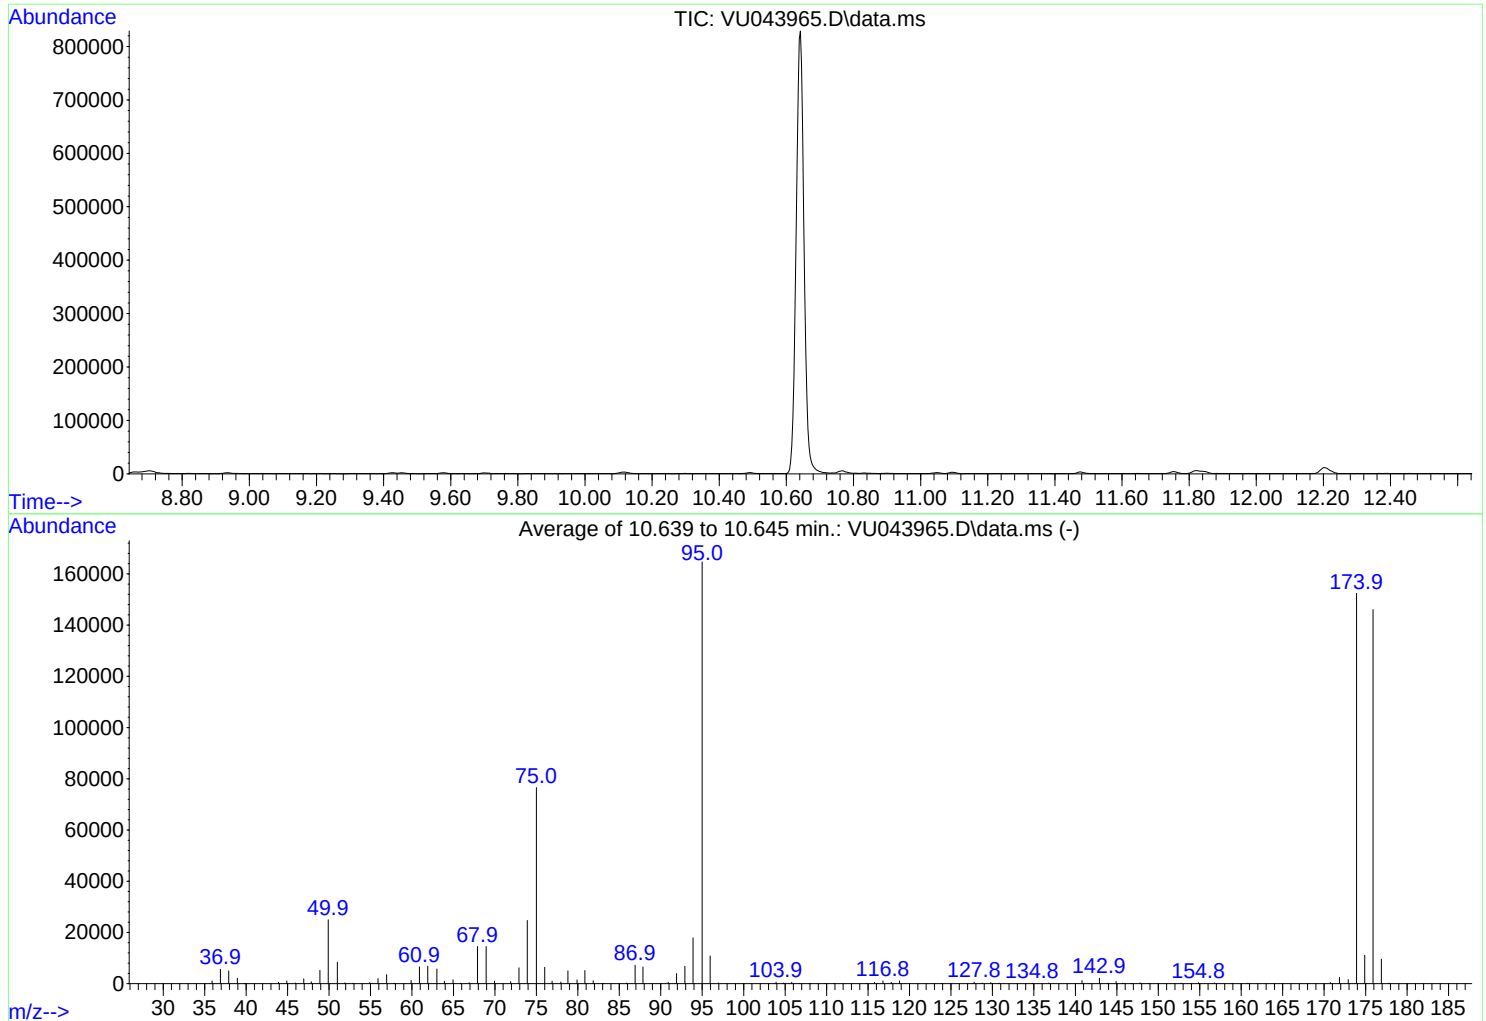

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	24925	PASS
75	95	30	80	46.5	76515	PASS
95	95	100	100	100.0	164715	PASS
96	95	5	9	6.6	10806	PASS
173	174	0.00	2	1.0	1540	PASS
174	95	50	120	92.5	152363	PASS
175	174	5	9	7.3	11047	PASS
176	174	95	101	95.9	146069	PASS
177	176	5	9	6.6	9577	PASS

m/z	Abundance
39.90	187.0
43.90	514.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	1108.0
36.90	5836.0
37.90	5089.0
39.00	2153.0
39.80	210.0
43.90	1068.0
44.90	1122.0
45.90	217.0
47.00	1929.0
47.80	765.0
48.90	5418.0
49.90	25632.0
51.00	8791.0
51.90	344.0
52.90	209.0
54.90	347.0
55.90	2171.0
56.90	3511.0
58.00	180.0
59.90	1359.0
60.90	6441.0
61.90	7236.0
63.00	5988.0
63.90	1025.0
64.90	1488.0
66.00	193.0
66.90	428.0
67.90	15178.0
69.00	15010.0
70.00	1072.0
71.90	891.0
72.90	6355.0
73.90	25200.0
75.00	78440.0
76.00	6822.0
76.90	1052.0
78.00	671.0
78.80	5096.0
79.90	1450.0
80.90	5371.0
81.90	1120.0
83.00	103.0
85.80	274.0
86.90	7368.0
87.90	6707.0
90.90	563.0
91.90	3981.0
92.90	7085.0
93.90	18360.0
95.00	168320.0
96.00	11201.0
97.00	344.0
103.90	612.0
104.80	271.0
105.80	576.0
106.70	160.0
110.90	163.0
114.80	161.0
115.80	557.0
116.80	1069.0
117.80	581.0
118.80	1061.0
127.80	612.0
128.70	271.0
129.80	538.0
130.80	200.0
134.80	244.0
136.80	258.0
140.80	1245.0
142.90	2369.0
143.90	182.0
144.90	996.0
145.70	265.0
146.70	100.0
147.80	312.0
148.80	104.0
152.70	143.0
154.80	329.0
156.80	356.0
158.80	154.0
160.80	188.0
170.70	456.0
171.90	2399.0
172.90	1583.0
173.90	151296.0
174.90	11350.0
175.90	144384.0
176.90	9811.0
177.80	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	1133.0
36.90	5862.0
37.90	5092.0
38.90	2226.0
39.80	223.0
43.90	1109.0
44.90	1094.0
45.90	242.0
47.00	1948.0
47.90	791.0
48.90	5368.0
49.90	25800.0
51.00	8756.0
51.90	332.0
52.90	186.0
54.90	403.0
55.90	2078.0
57.00	3607.0
57.80	165.0
59.90	1315.0
60.90	6728.0
61.90	6942.0
63.00	5851.0
63.90	991.0
65.00	1593.0
65.80	155.0
66.90	384.0
67.90	14953.0
68.90	14903.0
70.00	1085.0
71.90	837.0
72.90	6413.0
73.90	25544.0
75.00	78840.0
76.00	6576.0
76.90	1078.0
78.00	664.0
78.80	5157.0
79.90	1485.0
80.90	5354.0
81.90	1142.0
85.80	228.0
86.90	7389.0
87.80	6675.0
90.90	572.0
91.90	4038.0
92.90	7080.0
93.90	18528.0
95.00	170176.0
95.90	11104.0
97.00	286.0
103.90	676.0
104.80	278.0
105.80	629.0
106.70	155.0
109.80	105.0
110.90	155.0
114.80	149.0
115.80	519.0
116.80	1113.0
117.80	493.0
118.80	1093.0
123.90	122.0
127.80	600.0
128.80	280.0
129.80	456.0
130.80	214.0
134.80	211.0
136.80	258.0
140.80	1254.0
141.70	129.0
142.90	2206.0
143.90	197.0
144.90	906.0
145.70	287.0
147.80	360.0
148.80	131.0
152.80	159.0
153.90	100.0
154.80	390.0
156.80	351.0
158.90	163.0
160.80	203.0
170.70	479.0
171.80	2524.0
172.90	1553.0
173.90	156992.0
174.90	11437.0
175.90	150912.0
176.90	9923.0
177.80	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	1027.0
36.90	5226.0
37.90	4624.0
39.00	2084.0
39.80	235.0
43.90	1080.0
44.90	934.0
46.00	219.0
46.90	1751.0
47.90	744.0
48.90	4792.0
49.90	23344.0
51.00	7507.0
51.90	320.0
52.90	155.0
54.90	361.0
55.90	1793.0
57.00	3382.0
57.80	141.0
59.90	1161.0
60.90	6499.0
61.90	6176.0
63.00	5230.0
63.90	891.0
65.00	1483.0
65.80	147.0
66.90	300.0
67.90	13408.0
68.90	13537.0
69.90	936.0
71.90	770.0
72.90	5896.0
73.90	23352.0
75.00	72264.0
76.00	5740.0
76.90	977.0
77.90	607.0
78.80	4712.0
79.90	1390.0
80.80	4699.0
81.80	1129.0
85.90	212.0
86.90	6830.0
87.80	6040.0
90.90	482.0
91.90	3840.0
92.90	6328.0
93.90	16736.0
95.00	155648.0
95.90	10112.0
96.90	249.0
103.90	642.0
104.80	231.0
105.80	576.0
106.70	140.0
107.90	103.0
109.80	101.0
110.90	149.0
114.80	128.0
115.80	441.0
116.80	1067.0
117.80	431.0
118.80	998.0
123.80	117.0
127.80	512.0
128.80	278.0
129.80	388.0
130.80	206.0
134.80	179.0
136.80	237.0
140.80	1137.0
141.70	143.0
142.90	1876.0
143.90	153.0
144.90	781.0
145.90	303.0
147.80	348.0
148.80	127.0
150.00	120.0
152.80	181.0
153.90	109.0
154.90	407.0
156.80	270.0
159.00	154.0
160.80	190.0
170.80	412.0
171.80	2443.0
172.90	1485.0
173.90	148800.0
174.90	10355.0
175.90	142912.0
176.90	8996.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

177.80

167.0

Instrument :

MSVOA_U

ClientSampleId :

BFB135