

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048662.D
 Acq On : 25 May 2022 11:36
 Operator : SY/MD
 Sample : VU0525MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M

Title : VOC Analysis

Signal : TIC: VU048662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	60180	66032	9.02%	1.067%
2	1.771	130	134	138	rVB4	1872	1604	0.22%	0.026%
3	1.793	138	141	146	rBV2	492	576	0.08%	0.009%
4	1.912	169	178	191	rBV	51702	68039	9.29%	1.099%
5	2.009	205	208	214	rVB2	492	472	0.06%	0.008%
6	2.147	241	251	256	rBV	2532	2877	0.39%	0.046%
7	2.176	256	260	261	rBV	533	379	0.05%	0.006%
8	2.256	282	285	286	rBV	358	180	0.02%	0.003%
9	2.340	304	311	313	rBV	4167	3817	0.52%	0.062%
10	2.491	351	358	361	rBV	451	570	0.08%	0.009%
11	2.568	371	382	398	rVB	139828	225334	30.77%	3.641%
12	2.761	437	442	444	rBV2	583	545	0.07%	0.009%
13	2.784	445	449	452	rBV	689	666	0.09%	0.011%
14	2.909	485	488	489	rBV	322	181	0.02%	0.003%
15	3.182	562	573	576	rBV2	1585	2448	0.33%	0.040%
16	3.301	608	610	612	rBV	491	227	0.03%	0.004%
17	3.350	620	625	627	rBV2	399	394	0.05%	0.006%
18	3.385	633	636	638	rBV	376	211	0.03%	0.003%
19	3.475	661	664	668	rBV	659	500	0.07%	0.008%
20	3.549	684	687	690	rBV2	468	252	0.03%	0.004%
21	3.610	703	706	708	rBV	535	413	0.06%	0.007%
22	3.745	745	748	749	rBV	330	196	0.03%	0.003%
23	3.983	819	822	826	rBV	298	188	0.03%	0.003%
24	4.006	826	829	832	rBV	414	274	0.04%	0.004%
25	4.121	863	865	870	rVB	473	335	0.05%	0.005%
26	4.289	915	917	921	rVB	613	337	0.05%	0.005%
27	4.314	922	925	929	rBV	310	224	0.03%	0.004%
28	4.620	1007	1020	1047	rBV	83156	203481	27.79%	3.288%
29	4.893	1102	1105	1107	rBV	368	267	0.04%	0.004%
30	4.986	1130	1134	1137	rBV2	485	393	0.05%	0.006%
31	5.002	1137	1139	1142	rVV	383	271	0.04%	0.004%
32	5.063	1143	1158	1183	rVB	150843	334804	45.72%	5.410%
33	5.356	1244	1249	1251	rBV2	599	540	0.07%	0.009%
34	5.504	1292	1295	1299	rBV	451	309	0.04%	0.005%
35	5.726	1342	1364	1386	rBV2	259281	732267	100.00%	11.833%
36	5.932	1426	1428	1432	rVB	753	485	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048662.D
 Acq On : 25 May 2022 11:36
 Operator : SY/MD
 Sample : VU0525MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	5.951	1432	1434	1436	rBV	350	196	0.03%	0.003%
38	6.009	1449	1452	1453	rBV2	364	176	0.02%	0.003%
39	6.038	1458	1461	1463	rBV2	572	308	0.04%	0.005%
40	6.060	1464	1468	1472	rBV	437	382	0.05%	0.006%
41	6.108	1479	1483	1485	rBV	372	290	0.04%	0.005%
42	6.179	1499	1505	1508	rBV	454	582	0.08%	0.009%
43	6.250	1513	1527	1549	rBV	250157	473571	64.67%	7.653%
44	6.533	1602	1615	1626	rBV5	5364	10513	1.44%	0.170%
45	6.588	1630	1632	1635	rBV2	505	274	0.04%	0.004%
46	6.690	1651	1664	1687	rBV	170845	330383	45.12%	5.339%
47	6.832	1705	1708	1712	rBV	404	430	0.06%	0.007%
48	6.896	1722	1728	1732	rBV2	442	517	0.07%	0.008%
49	6.973	1749	1752	1756	rBV2	407	360	0.05%	0.006%
50	7.182	1811	1817	1832	rVB3	2301	4390	0.60%	0.071%
51	7.263	1836	1842	1844	rBV	382	344	0.05%	0.006%
52	7.279	1844	1847	1850	rBV	432	350	0.05%	0.006%
53	7.314	1854	1858	1861	rBV	379	373	0.05%	0.006%
54	7.375	1874	1877	1879	rBV	355	223	0.03%	0.004%
55	7.391	1879	1882	1885	rVV	314	245	0.03%	0.004%
56	7.565	1925	1936	1954	rVB2	97550	171509	23.42%	2.772%
57	7.845	2020	2023	2026	rBV	457	293	0.04%	0.005%
58	7.899	2026	2040	2055	rBV	320025	561372	76.66%	9.072%
59	8.134	2111	2113	2116	rBV	439	250	0.03%	0.004%
60	8.179	2116	2127	2146	rBV	74608	126600	17.29%	2.046%
61	8.456	2209	2213	2214	rBV	423	270	0.04%	0.004%
62	8.497	2222	2226	2228	rBV	447	255	0.03%	0.004%
63	8.533	2234	2237	2242	rBV2	447	315	0.04%	0.005%
64	8.632	2256	2268	2303	rBV	242566	454403	62.05%	7.343%
65	8.857	2335	2338	2341	rBV2	504	443	0.06%	0.007%
66	8.973	2370	2374	2382	rVB2	796	869	0.12%	0.014%
67	9.009	2382	2385	2387	rBV	334	237	0.03%	0.004%
68	9.099	2410	2413	2417	rBV	883	661	0.09%	0.011%
69	9.253	2454	2461	2462	rBV	403	493	0.07%	0.008%
70	9.417	2499	2512	2536	rBV	355840	600927	82.06%	9.711%
71	9.568	2555	2559	2560	rBV3	932	612	0.08%	0.010%
72	9.748	2610	2615	2619	rBV2	746	816	0.11%	0.013%
73	9.835	2640	2642	2644	rBV	354	209	0.03%	0.003%
74	9.877	2652	2655	2659	rVB2	751	624	0.09%	0.010%
75	9.922	2664	2669	2672	rBV2	717	685	0.09%	0.011%
76	9.951	2676	2678	2680	rBV2	351	231	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048662.D
 Acq On : 25 May 2022 11:36
 Operator : SY/MD
 Sample : VU0525MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.089	2717	2721	2723	rBV2	809	558	0.08%	0.009%
78	10.452	2832	2834	2839	rVB	567	374	0.05%	0.006%
79	10.507	2849	2851	2853	rBV	389	205	0.03%	0.003%
80	10.523	2853	2856	2861	rVV2	760	726	0.10%	0.012%
81	10.758	2917	2929	2945	rBV	281133	460550	62.89%	7.442%
82	10.909	2970	2976	2979	rBV3	1021	949	0.13%	0.015%
83	10.976	2994	2997	3001	rBV2	460	341	0.05%	0.006%
84	11.092	3028	3033	3035	rBV2	722	792	0.11%	0.013%
85	11.140	3046	3048	3052	rBV	404	347	0.05%	0.006%
86	11.337	3105	3109	3112	rBV	329	289	0.04%	0.005%
87	11.356	3112	3115	3117	rBV	477	329	0.04%	0.005%
88	11.562	3176	3179	3184	rVB	578	375	0.05%	0.006%
89	11.674	3211	3214	3219	rVB	405	393	0.05%	0.006%
90	11.703	3219	3223	3228	rBV2	459	556	0.08%	0.009%
91	11.745	3232	3236	3239	rBV2	1112	1050	0.14%	0.017%
92	11.812	3245	3257	3279	rBV	404482	651981	89.04%	10.536%
93	12.192	3363	3375	3392	rBV	391163	644408	88.00%	10.413%
94	12.446	3451	3454	3458	rVB	714	521	0.07%	0.008%
95	12.880	3586	3589	3592	rBV	450	377	0.05%	0.006%
96	13.488	3775	3778	3781	rBV	766	554	0.08%	0.009%
97	13.799	3872	3875	3876	rBV	619	325	0.04%	0.005%
98	13.844	3885	3889	3899	rVB4	3267	3681	0.50%	0.059%
99	14.092	3959	3966	3982	rVB	10206	17552	2.40%	0.284%
100	14.330	4034	4040	4052	rBV8	2995	4946	0.68%	0.080%




Sum of corrected areas: 6188248

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048662.D
Acq On : 25 May 2022 11:36
Operator : SY/MD
Sample : VU0525MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

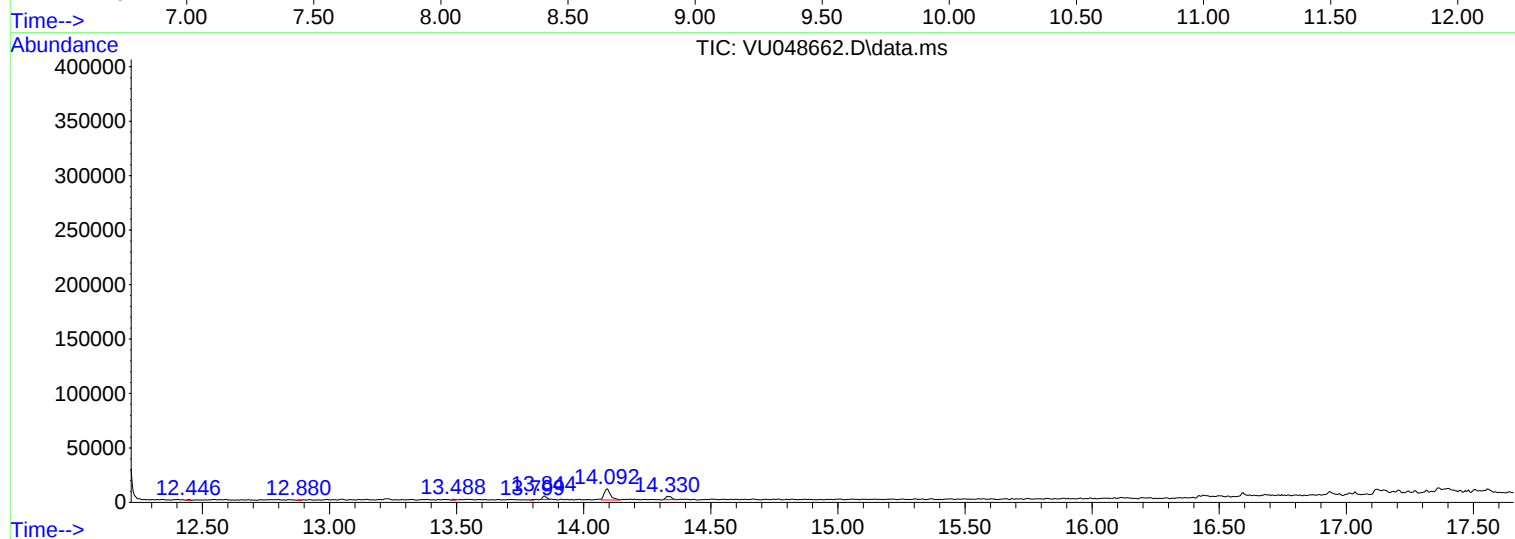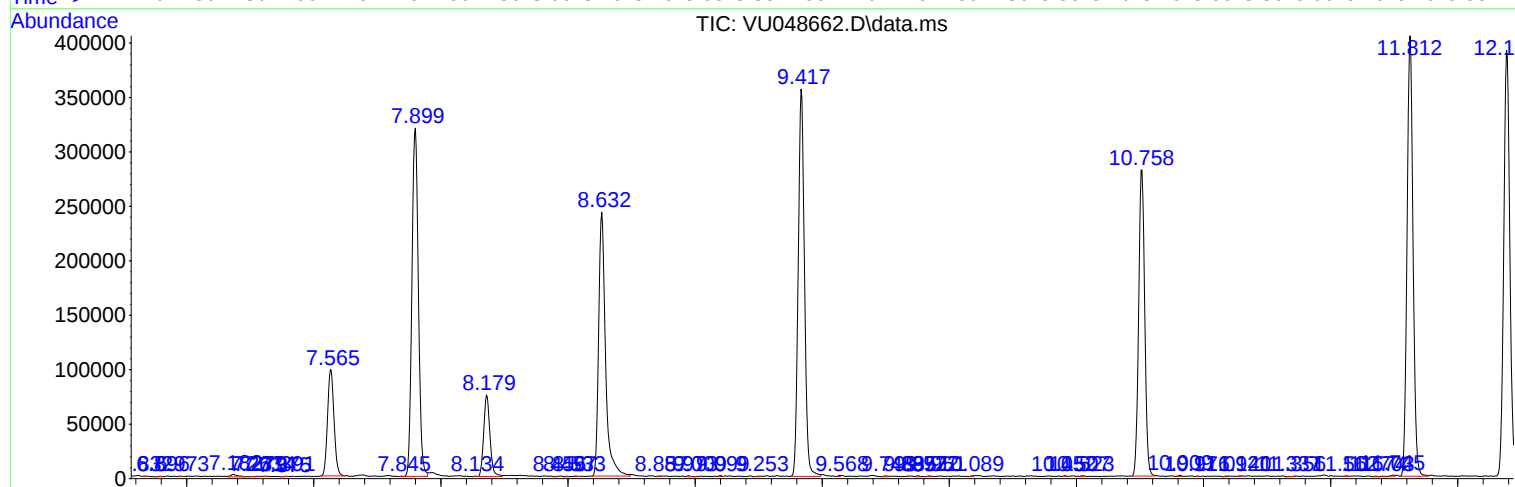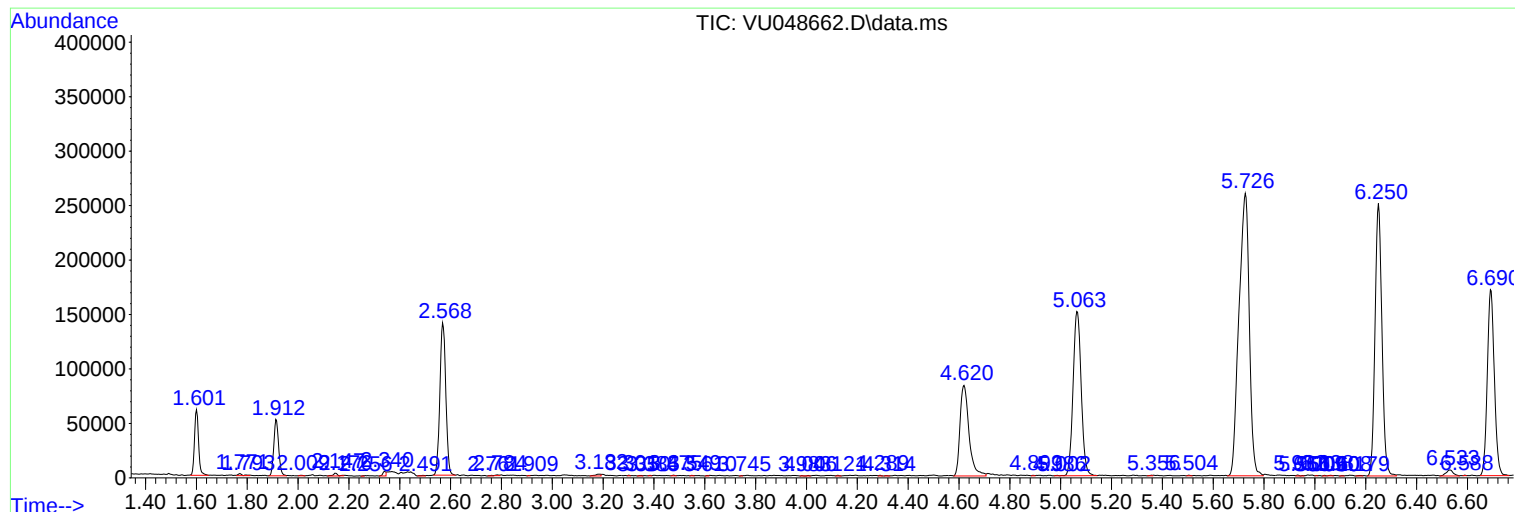

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048662.D
Acq On : 25 May 2022 11:36
Operator : SY/MD
Sample : VU0525MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048662.D
Acq On : 25 May 2022 11:36
Operator : SY/MD
Sample : VU0525MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc