

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048663.D
 Acq On : 25 May 2022 11:59
 Operator : SY/MD
 Sample : VU0525WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M

Title : VOC Analysis

Signal : TIC: VU048663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	73688	85078	11.12%	1.370%
2	1.912	169	178	192	rBV	59115	74720	9.77%	1.203%
3	1.993	198	203	208	rBV2	584	633	0.08%	0.010%
4	2.047	217	220	223	rBV2	447	293	0.04%	0.005%
5	2.089	230	233	234	rBV2	313	187	0.02%	0.003%
6	2.199	265	267	269	rBB	326	122	0.02%	0.002%
7	2.211	269	271	273	rVB	188	85	0.01%	0.001%
8	2.234	276	278	280	rBV2	242	118	0.02%	0.002%
9	2.253	280	284	287	rBV	652	506	0.07%	0.008%
10	2.285	291	294	296	rBV	505	314	0.04%	0.005%
11	2.340	296	311	314	rBV	4876	10257	1.34%	0.165%
12	2.504	357	362	370	rBV	563	736	0.10%	0.012%
13	2.568	370	382	398	rBV	166887	272146	35.57%	4.382%
14	2.707	422	425	426	rBV	257	138	0.02%	0.002%
15	2.726	429	431	433	rVV	303	126	0.02%	0.002%
16	2.858	468	472	473	rBV	289	220	0.03%	0.004%
17	2.916	487	490	492	rBV	345	221	0.03%	0.004%
18	3.047	524	531	543	rBV4	1654	2930	0.38%	0.047%
19	3.321	614	616	618	rBV	274	138	0.02%	0.002%
20	3.343	620	623	627	rBV2	370	335	0.04%	0.005%
21	3.395	636	639	641	rBV2	263	129	0.02%	0.002%
22	3.408	641	643	645	rBV	518	292	0.04%	0.005%
23	3.446	651	655	657	rBV2	417	272	0.04%	0.004%
24	3.507	671	674	677	rBV	499	361	0.05%	0.006%
25	3.527	677	680	682	rBV	404	276	0.04%	0.004%
26	3.559	687	690	691	rBV	168	101	0.01%	0.002%
27	3.633	710	713	717	rVB	573	371	0.05%	0.006%
28	3.652	717	719	721	rBV	298	145	0.02%	0.002%
29	3.713	734	738	741	rBV2	624	499	0.07%	0.008%
30	3.909	796	799	802	rBV	443	369	0.05%	0.006%
31	3.967	814	817	819	rBV	429	290	0.04%	0.005%
32	4.089	853	855	859	rBV	342	235	0.03%	0.004%
33	4.109	859	861	864	rVV	531	294	0.04%	0.005%
34	4.141	868	871	876	rVB2	696	432	0.06%	0.007%
35	4.266	907	910	914	rVB	474	331	0.04%	0.005%
36	4.285	914	916	921	rBV2	476	321	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048663.D
 Acq On : 25 May 2022 11:59
 Operator : SY/MD
 Sample : VU0525WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	4.340	930	933	937	rBV	439	332	0.04%	0.005%
38	4.366	938	941	943	rBV	568	342	0.04%	0.006%
39	4.501	980	983	991	rBV	618	712	0.09%	0.011%
40	4.539	991	995	999	rBV	575	527	0.07%	0.008%
41	4.575	999	1006	1008	rBV2	815	814	0.11%	0.013%
42	4.623	1010	1021	1048	rVV2	69407	178156	23.28%	2.869%
43	4.832	1083	1086	1089	rBV3	552	358	0.05%	0.006%
44	4.941	1116	1120	1123	rBV2	521	505	0.07%	0.008%
45	4.983	1127	1133	1137	rVB3	611	698	0.09%	0.011%
46	5.063	1143	1158	1183	rBV	151354	331274	43.29%	5.334%
47	5.308	1231	1234	1237	rBV	551	388	0.05%	0.006%
48	5.417	1265	1268	1270	rBV	590	406	0.05%	0.007%
49	5.520	1297	1300	1304	rBV	434	273	0.04%	0.004%
50	5.726	1342	1364	1390	rBV2	272684	765177	100.00%	12.321%
51	5.864	1404	1407	1408	rBV	500	290	0.04%	0.005%
52	5.980	1439	1443	1445	rBV2	638	471	0.06%	0.008%
53	6.009	1450	1452	1455	rBV	333	259	0.03%	0.004%
54	6.060	1465	1468	1471	rBV	296	195	0.03%	0.003%
55	6.137	1488	1492	1493	rBV	314	222	0.03%	0.004%
56	6.250	1513	1527	1543	rBV	252898	471471	61.62%	7.592%
57	6.440	1584	1586	1590	rVB	620	365	0.05%	0.006%
58	6.459	1590	1592	1594	rBV	205	112	0.01%	0.002%
59	6.533	1606	1615	1625	rBV6	4046	7701	1.01%	0.124%
60	6.694	1651	1665	1686	rBV2	166688	331257	43.29%	5.334%
61	6.793	1694	1696	1699	rVB2	620	280	0.04%	0.005%
62	6.845	1709	1712	1714	rBV2	392	312	0.04%	0.005%
63	6.896	1724	1728	1731	rBV	853	624	0.08%	0.010%
64	6.941	1739	1742	1744	rBV	610	429	0.06%	0.007%
65	7.038	1769	1772	1774	rBV	343	218	0.03%	0.004%
66	7.186	1812	1818	1826	rVB3	843	1117	0.15%	0.018%
67	7.333	1856	1864	1866	rBV	627	769	0.10%	0.012%
68	7.401	1882	1885	1887	rBV	442	318	0.04%	0.005%
69	7.517	1918	1921	1923	rBV	375	208	0.03%	0.003%
70	7.565	1924	1936	1957	rVV	102496	183953	24.04%	2.962%
71	7.768	1993	1999	2001	rBV2	491	567	0.07%	0.009%
72	7.787	2003	2005	2007	rVV	350	162	0.02%	0.003%
73	7.899	2027	2040	2055	rBV	361708	620484	81.09%	9.991%
74	8.179	2116	2127	2145	rBV2	75854	133711	17.47%	2.153%
75	8.494	2223	2225	2227	rBV2	451	240	0.03%	0.004%
76	8.636	2255	2269	2301	rBV2	205112	383688	50.14%	6.178%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048663.D
 Acq On : 25 May 2022 11:59
 Operator : SY/MD
 Sample : VU0525WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	8.973	2371	2374	2377	rBV2	565	451	0.06%	0.007%
78	8.993	2377	2380	2381	rBV	523	282	0.04%	0.005%
79	9.079	2401	2407	2409	rBV2	638	769	0.10%	0.012%
80	9.417	2500	2512	2533	rBV	357998	597956	78.15%	9.629%
81	9.581	2561	2563	2568	rVB	768	530	0.07%	0.009%
82	9.626	2571	2577	2579	rBV	710	711	0.09%	0.011%
83	9.919	2663	2668	2670	rBV2	334	256	0.03%	0.004%
84	10.121	2726	2731	2737	rBV3	725	851	0.11%	0.014%
85	10.314	2788	2791	2796	rBV	551	487	0.06%	0.008%
86	10.456	2832	2835	2837	rBV2	584	417	0.05%	0.007%
87	10.571	2867	2871	2877	rVB2	578	656	0.09%	0.011%
88	10.758	2916	2929	2946	rBV	251317	411268	53.75%	6.622%
89	10.912	2975	2977	2979	rBV2	471	273	0.04%	0.004%
90	11.253	3081	3083	3085	rBV	250	139	0.02%	0.002%
91	11.446	3140	3143	3147	rBV2	975	945	0.12%	0.015%
92	11.542	3170	3173	3176	rBV	627	508	0.07%	0.008%
93	11.812	3245	3257	3279	rBV	411082	651480	85.14%	10.491%
94	12.192	3363	3375	3400	rVB	399220	656076	85.74%	10.565%
95	12.558	3483	3489	3491	rBV2	584	637	0.08%	0.010%
96	14.095	3959	3967	3978	rBV5	4033	6787	0.89%	0.109%
97	15.616	4434	4440	4443	rBV2	3797	5302	0.69%	0.085%




Sum of corrected areas: 6210187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048663.D
Acq On : 25 May 2022 11:59
Operator : SY/MD
Sample : VU0525WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

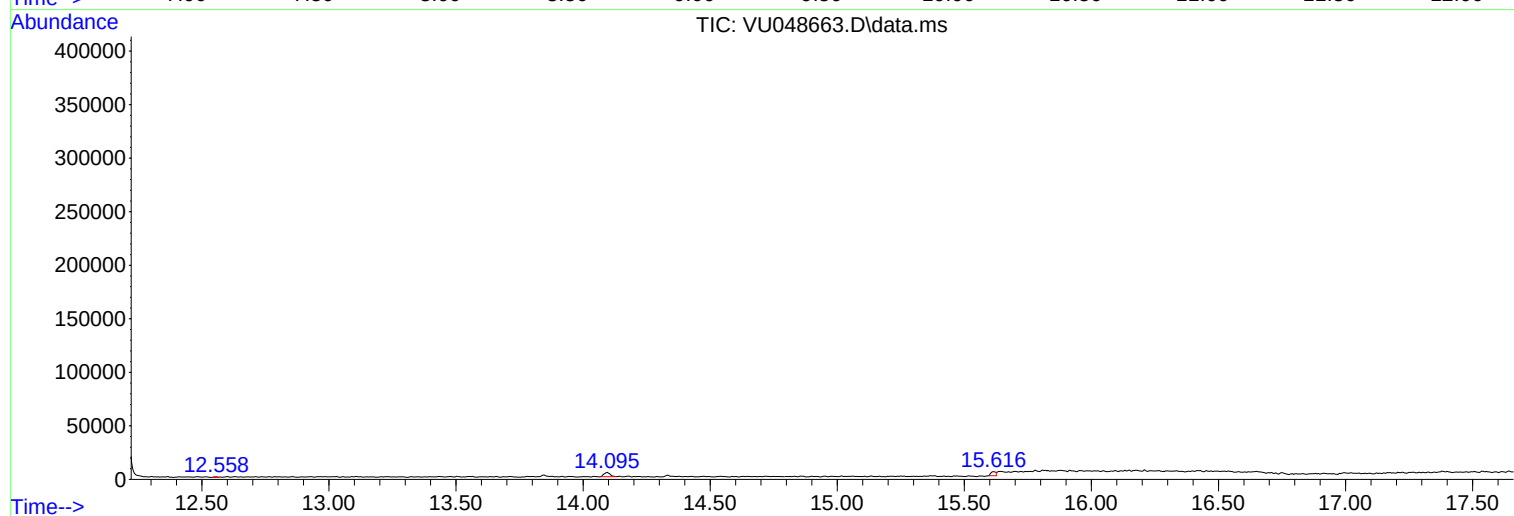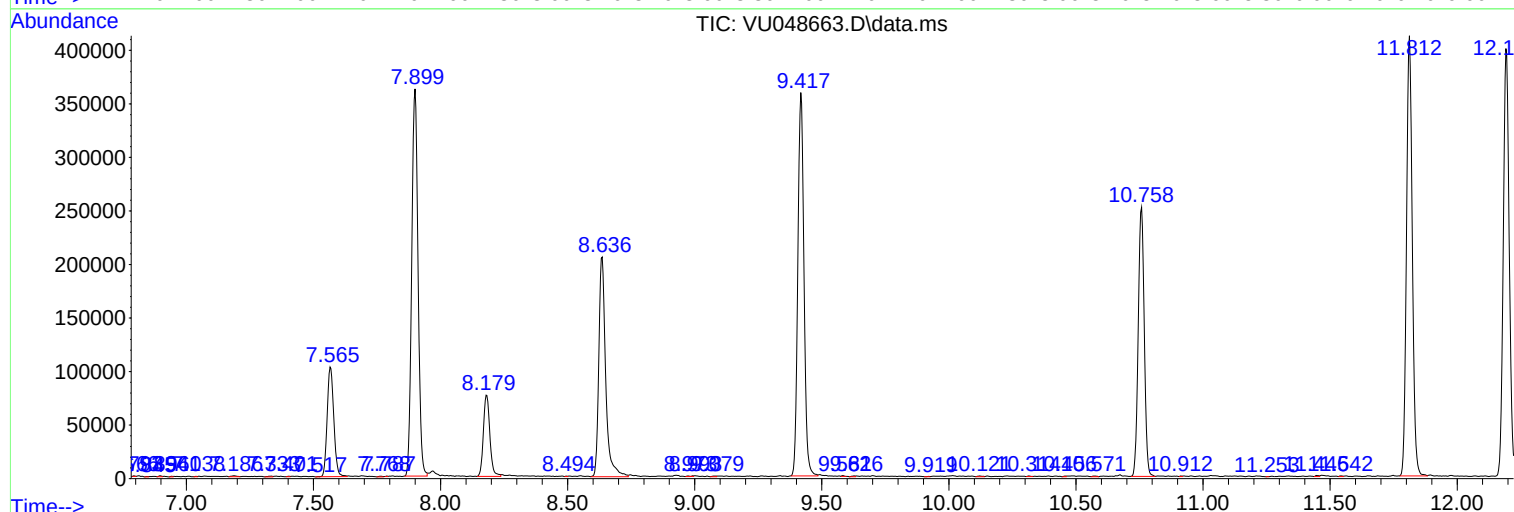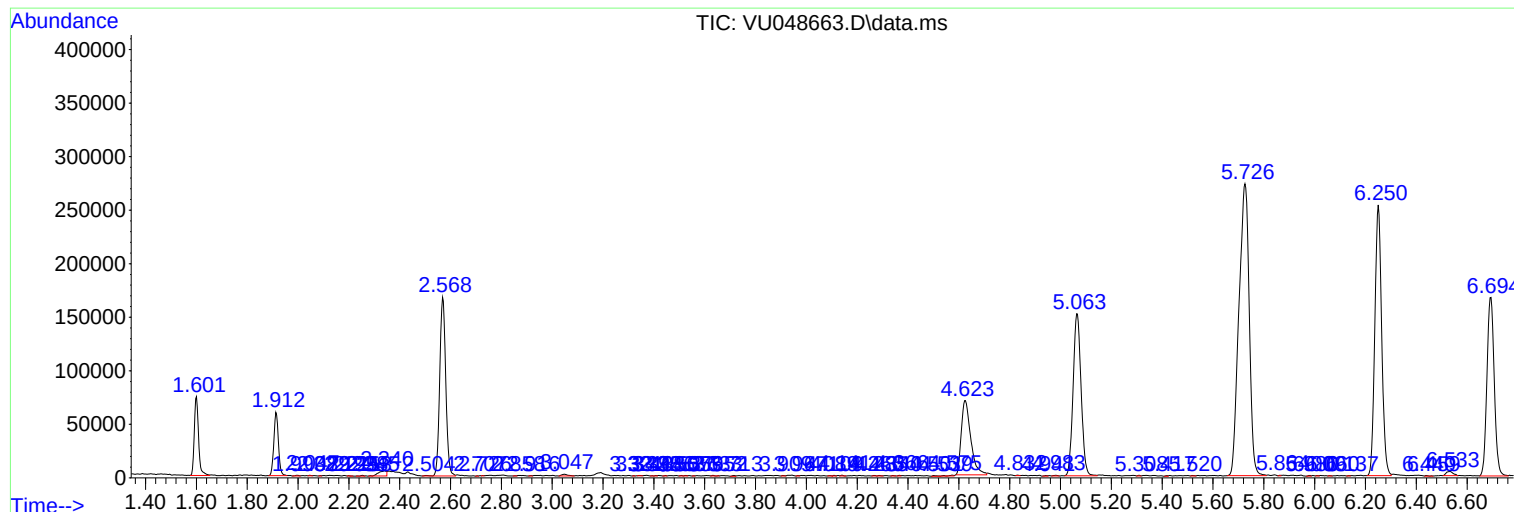

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048663.D
Acq On : 25 May 2022 11:59
Operator : SY/MD
Sample : VU0525WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
Data File : VU048663.D
Acq On : 25 May 2022 11:59
Operator : SY/MD
Sample : VU0525WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------