


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052522\
 Data File : VU048660.D
 Acq On : 25 May 2022 08:44
 Operator : SY/MD
 Sample : BFB093
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB093

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Thu May 26 06:51:07 2022

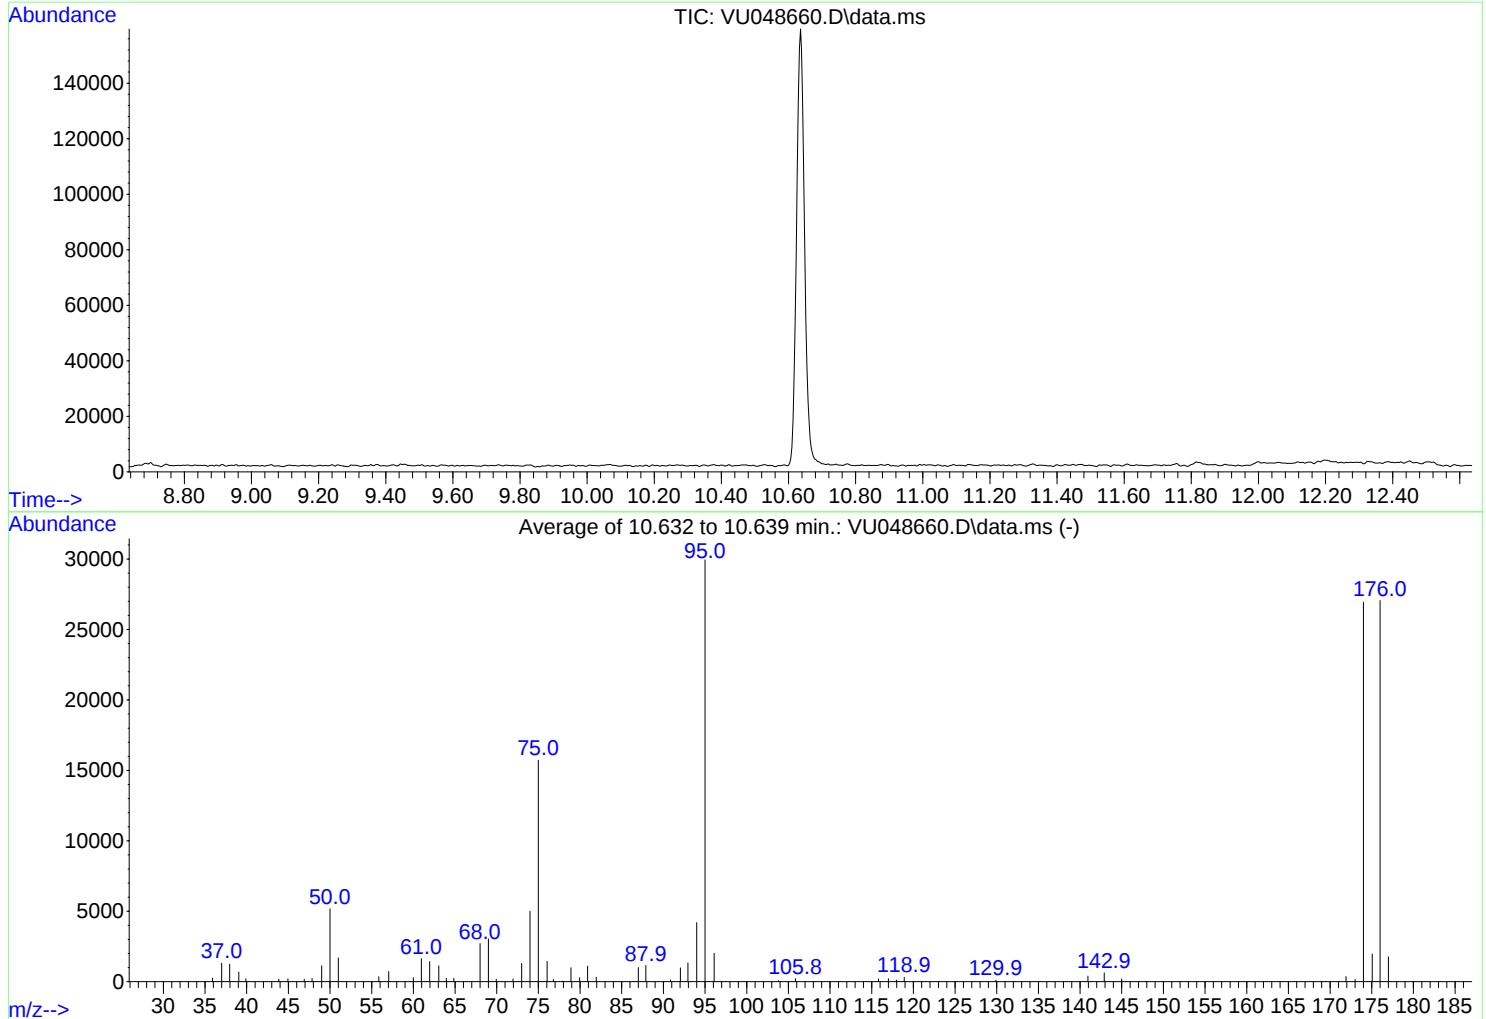

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5182	PASS
75	95	30	80	52.5	15725	PASS
95	95	100	100	100.0	29947	PASS
96	95	5	9	6.7	2010	PASS
173	174	0.00	2	0.6	150	PASS
174	95	50	120	89.9	26933	PASS
175	174	5	9	7.3	1964	PASS
176	174	95	101	100.5	27064	PASS
177	176	5	9	6.5	1766	PASS

m/z	Abundance
39.90	2050.0
44.00	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	276.0
37.00	1204.0
37.90	1276.0
39.00	643.0
39.90	2274.0
43.80	366.0
44.90	198.0
46.90	125.0
47.80	211.0
49.00	1048.0
50.00	5043.0
51.00	1730.0
55.80	332.0
57.10	676.0
60.00	285.0
60.90	1615.0
61.90	1426.0
63.00	1090.0
64.00	231.0
64.80	219.0
68.00	2678.0
69.00	3071.0
70.00	234.0
72.00	156.0
73.00	1334.0
74.00	5052.0
75.00	15533.0
76.00	1505.0
76.80	173.0
78.90	953.0
80.00	240.0
80.90	1132.0
82.00	342.0
87.00	1013.0
87.90	1085.0
90.90	140.0
92.10	911.0
93.00	1273.0
94.00	4060.0
95.00	30040.0
96.10	1971.0
105.80	241.0
115.80	208.0
116.90	191.0
117.90	134.0
118.90	291.0
129.90	193.0
141.00	418.0
142.90	636.0
145.00	180.0
147.90	103.0
171.90	336.0
174.00	26112.0
175.00	1911.0
176.00	26600.0
177.00	1767.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	253.0
37.00	1331.0
38.00	1302.0
39.10	707.0
39.90	2222.0
43.90	352.0
44.90	201.0
46.90	165.0
47.90	224.0
49.00	1168.0
50.00	5276.0
51.00	1759.0
55.90	361.0
57.10	695.0
60.00	291.0
61.00	1692.0
62.00	1405.0
63.10	1124.0
63.90	246.0
64.80	252.0
68.00	2753.0
69.00	3116.0
70.00	156.0
71.90	213.0
73.00	1324.0
74.00	5102.0
75.00	16360.0
76.00	1429.0
76.80	150.0
77.90	102.0
78.90	989.0
80.00	264.0
80.90	1086.0
81.90	319.0
87.00	1065.0
87.90	1217.0
90.80	130.0
92.10	999.0
93.00	1340.0
94.00	4410.0
95.00	30760.0
96.10	2073.0
103.80	115.0
105.90	238.0
115.80	210.0
117.00	194.0
118.00	101.0
118.90	329.0
129.90	151.0
140.90	426.0
142.90	648.0
145.00	213.0
171.90	379.0
173.00	449.0
174.00	27848.0
175.10	2026.0
176.00	27936.0
177.00	1836.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	209.0
37.00	1382.0
38.00	1135.0
39.10	692.0
39.90	2283.0
43.90	321.0
45.00	208.0
46.90	207.0
47.90	237.0
49.00	1166.0
50.00	5226.0
51.00	1571.0
55.90	372.0
57.00	761.0
60.00	293.0
61.00	1597.0
62.00	1414.0
63.00	1173.0
63.90	229.0
64.90	261.0
68.00	2677.0
69.00	2920.0
69.80	120.0
71.90	226.0
73.00	1233.0
74.00	4859.0
75.00	15281.0
76.10	1381.0
76.80	156.0
78.90	1028.0
79.90	300.0
80.90	1092.0
81.90	300.0
87.00	917.0
87.90	1130.0
90.80	107.0
92.00	1036.0
92.90	1358.0
94.00	4122.0
95.00	29040.0
96.10	1986.0
103.80	100.0
105.90	179.0
115.80	172.0
117.10	230.0
118.00	100.0
118.90	309.0
140.90	353.0
142.90	588.0
145.00	204.0
171.90	391.0
174.00	26840.0
175.00	1956.0
176.00	26656.0
177.00	1696.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093