
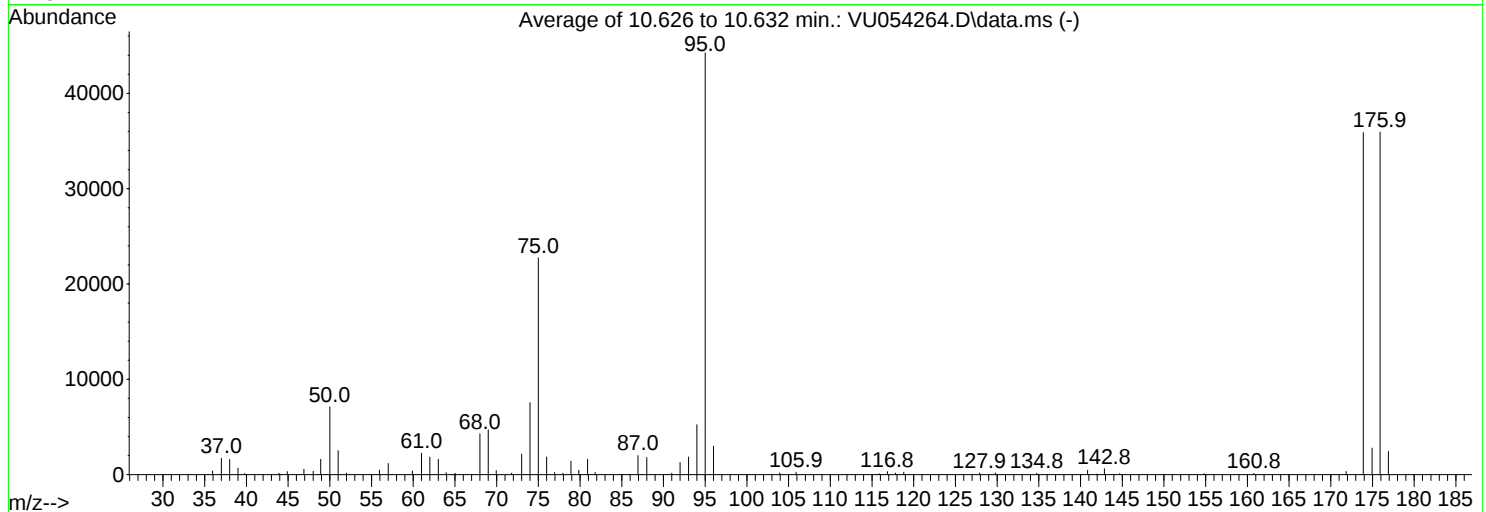


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052523\
Data File : VU054264.D
Acq On : 25 May 2023 13:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
Title : SW846 8260
Last Update : Fri May 26 06:40:51 2023

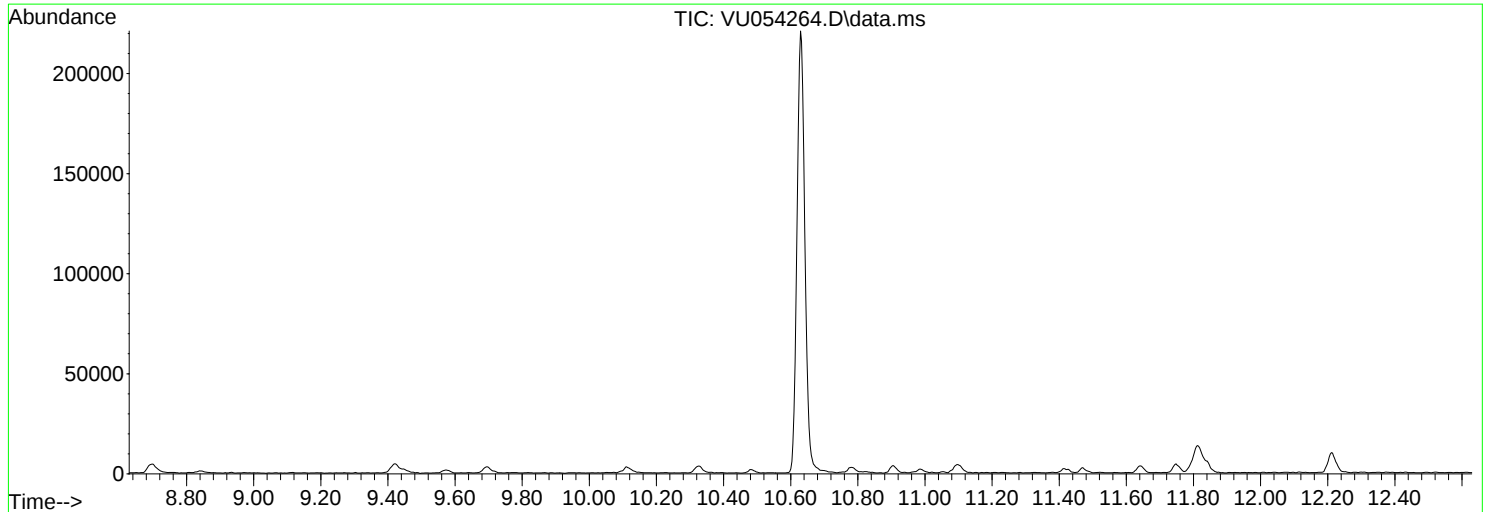

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	7115	PASS
75	95	30	60	51.4	22744	PASS
95	95	100	100	100.0	44248	PASS
96	95	5	9	6.7	2978	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.1	35888	PASS
175	174	5	9	7.8	2786	PASS
176	174	95	101	100.1	35936	PASS
177	176	5	9	6.8	2439	PASS