

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052618\
 Data File : VU024153.D
 Acq On : 26 May 2018 18:23
 Operator : MD/SY
 Sample : J3091-04DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 28 00:59:53 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 00:49:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	276973	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	256369	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	89636	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	83779	39.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.58%
7) Chloroethane-d5	1.68	69	72842	43.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.12%
11) 1,1-Dichloroethene-d2	2.27	63	122533	31.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.56%
21) 2-Butanone-d5	4.18	46	161321	96.37	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.37%
24) Chloroform-d	4.65	84	172181	45.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.26%
26) 1,2-Dichloroethane-d4	5.31	65	112207	46.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.88%
32) Benzene-d6	5.35	84	332207	46.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.64%
36) 1,2-Dichloropropane-d6	6.34	67	119382	49.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.18%
41) Toluene-d8	7.57	98	285594	43.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.86%
43) trans-1,3-Dichloropropene-	7.85	79	42444	43.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.78%
47) 2-Hexanone-d5	8.31	63	112251	96.76	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.76%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	166985	47.07	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.14%
64) 1,2-Dichlorobenzene-d4	11.87	152	104598	53.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.44%


Target Compounds						Qvalue
34) Trichloroethene	6.19	95	77856	32.48	ug/L	99
48) 2-Hexanone	8.31	43	12568	4.91	ug/L #	65
59) 1,2,3-Trichloropropane	11.49	75	10068	3.36	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052618\
Data File : VU024153.D
Acq On : 26 May 2018 18:23
Operator : MD/SY
Sample : J3091-04DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 28 00:59:53 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 00:49:31 2018
Response via : Initial Calibration

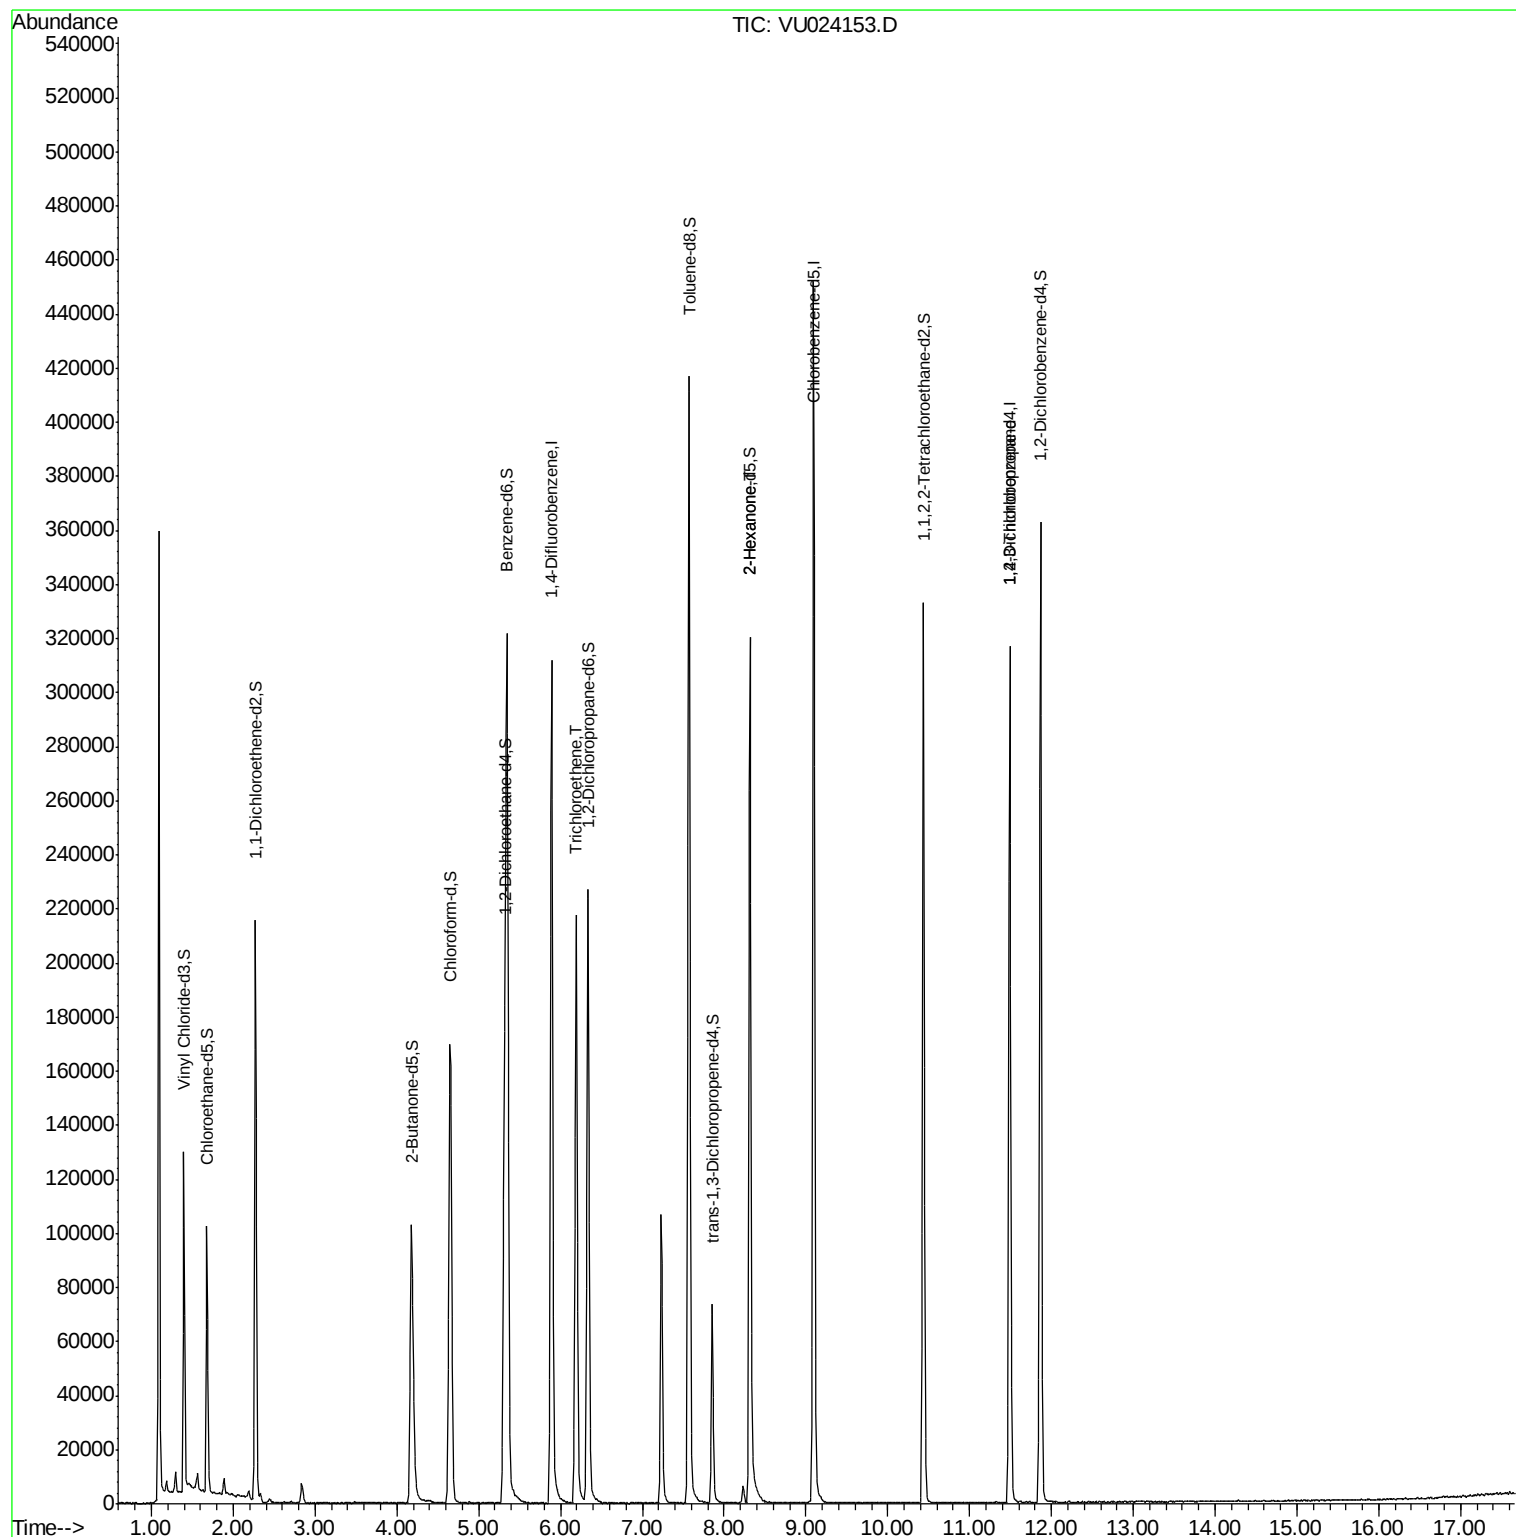

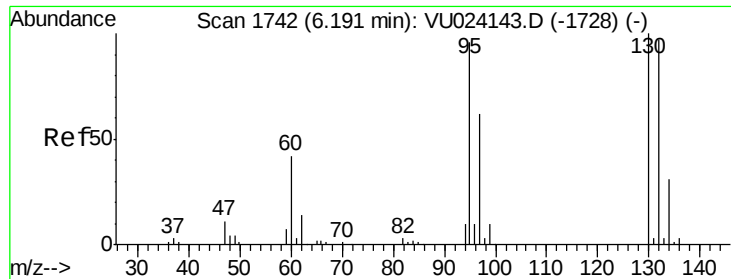

#34

Trichloroethene

Concen: 32.48 ug/L

RT: 6.19 min Scan# 1742

Delta R.T. 0.00 min

Lab File: VU024153.D

Acq: 26 May 2018 18:23

Tgt Ion: 95 Resp: 77856



Ion Ratio Lower Upper

95 100

97 61.7 44.5 82.7

132 97.9 69.0 128.2

130 101.0 70.6 131.0

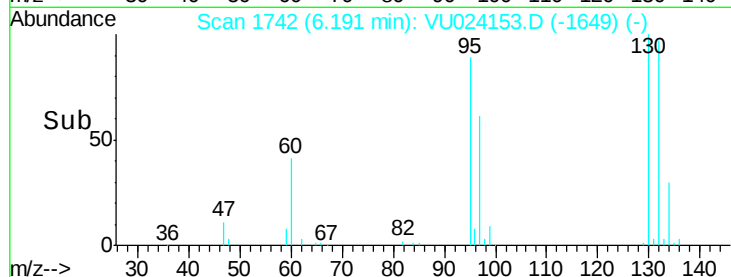
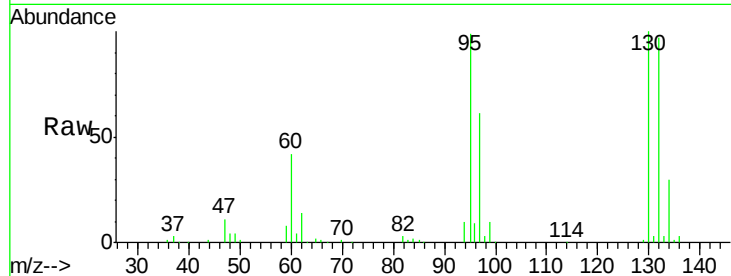


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

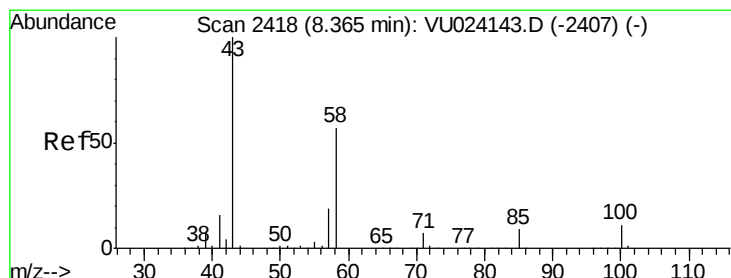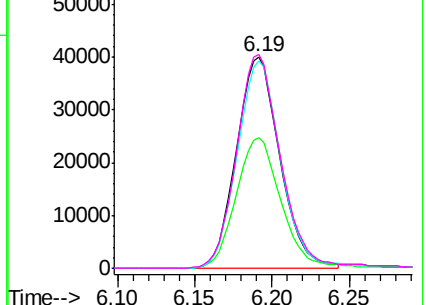

#48

2-Hexanone

Concen: 4.91 ug/L

RT: 8.31 min Scan# 2402

Delta R.T. -0.05 min

Lab File: VU024153.D

Acq: 26 May 2018 18:23

Tgt Ion: 43 Resp: 12568



Ion Ratio Lower Upper

43 100

58 29.5 44.6 67.0#

57 36.0 15.3 22.9#

100 2.8 8.9 13.3#

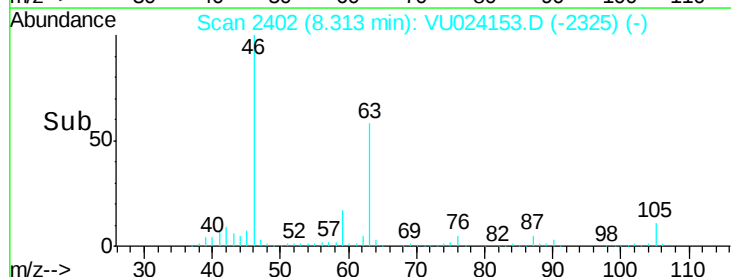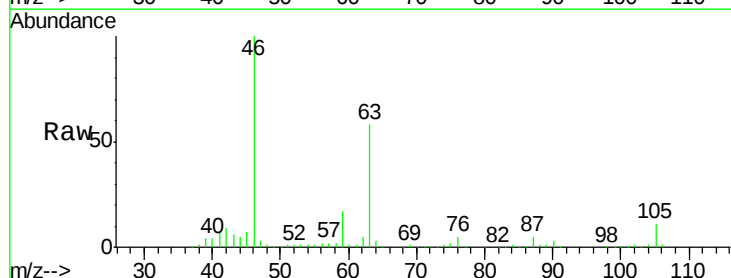



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

Ion 100.00 (99.70 to 100.70): VU0

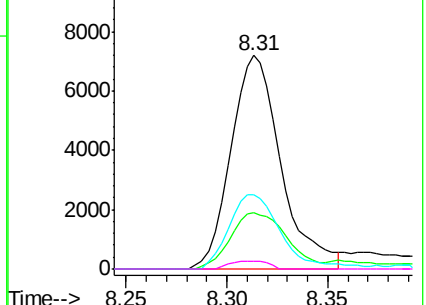

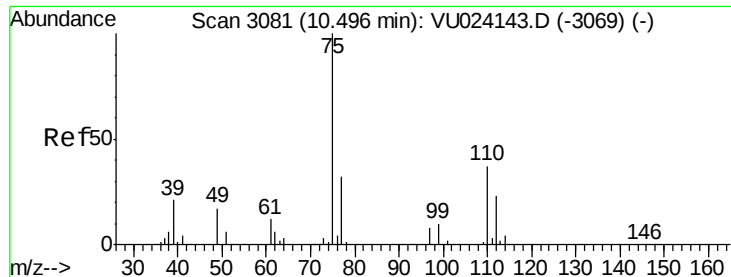

#59

1,2,3-Trichloropropane

Concen: 3.36 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU024153.D


Acq: 26 May 2018 18:23

Tgt Ion: 75 Resp: 10068

Ion Ratio Lower Upper

75 100

77 36.3 25.5 38.3

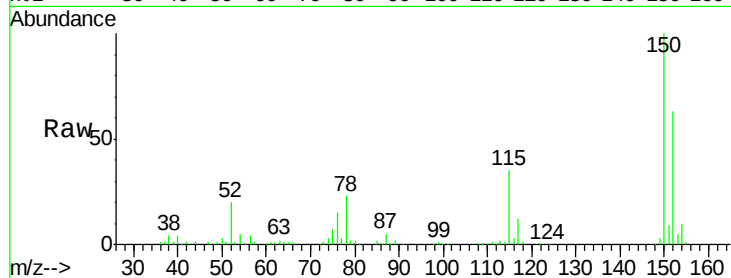

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

