

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052618\
 Data File : VU024163.D
 Acq On : 26 May 2018 22:37
 Operator : MD/SY
 Sample : J3091-18 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 28 01:01:53 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 00:49:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	272857	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	253833	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	84545	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	79387	38.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.54%
7) Chloroethane-d5	1.68	69	71221	43.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.48%
11) 1,1-Dichloroethene-d2	2.27	63	114799	29.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.50%#
21) 2-Butanone-d5	4.18	46	170421	103.34	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.34%
24) Chloroform-d	4.65	84	171094	46.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.06%
26) 1,2-Dichloroethane-d4	5.31	65	114390	48.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.16%
32) Benzene-d6	5.35	84	335000	47.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.38%
36) 1,2-Dichloropropane-d6	6.34	67	117709	48.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.78%
41) Toluene-d8	7.57	98	271200	41.66	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.32%
43) trans-1,3-Dichloropropene-	7.85	79	41826	43.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.38%
47) 2-Hexanone-d5	8.31	63	117704	102.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.47%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	169479	48.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.50%
64) 1,2-Dichlorobenzene-d4	11.87	152	98965	53.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.78%


Target Compounds


						Qvalue
34) Trichloroethene	6.19	95	44977	18.95	ug/L	97
35) Methylcyclohexane	6.33	83	25665	7.81	ug/L #	18
37) 1,2-Dichloropropane	6.34	63	12229	5.16	ug/L #	89
46) Tetrachloroethene	8.23	164	3806	2.29	ug/L	95
49) Dibromochloromethane	8.23	129	3526	1.59	ug/L #	11
59) 1,2,3-Trichloropropane	11.49	75	9099	3.07	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052618\
Data File : VU024163.D
Acq On : 26 May 2018 22:37
Operator : MD/SY
Sample : J3091-18 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 28 01:01:53 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 00:49:31 2018
Response via : Initial Calibration

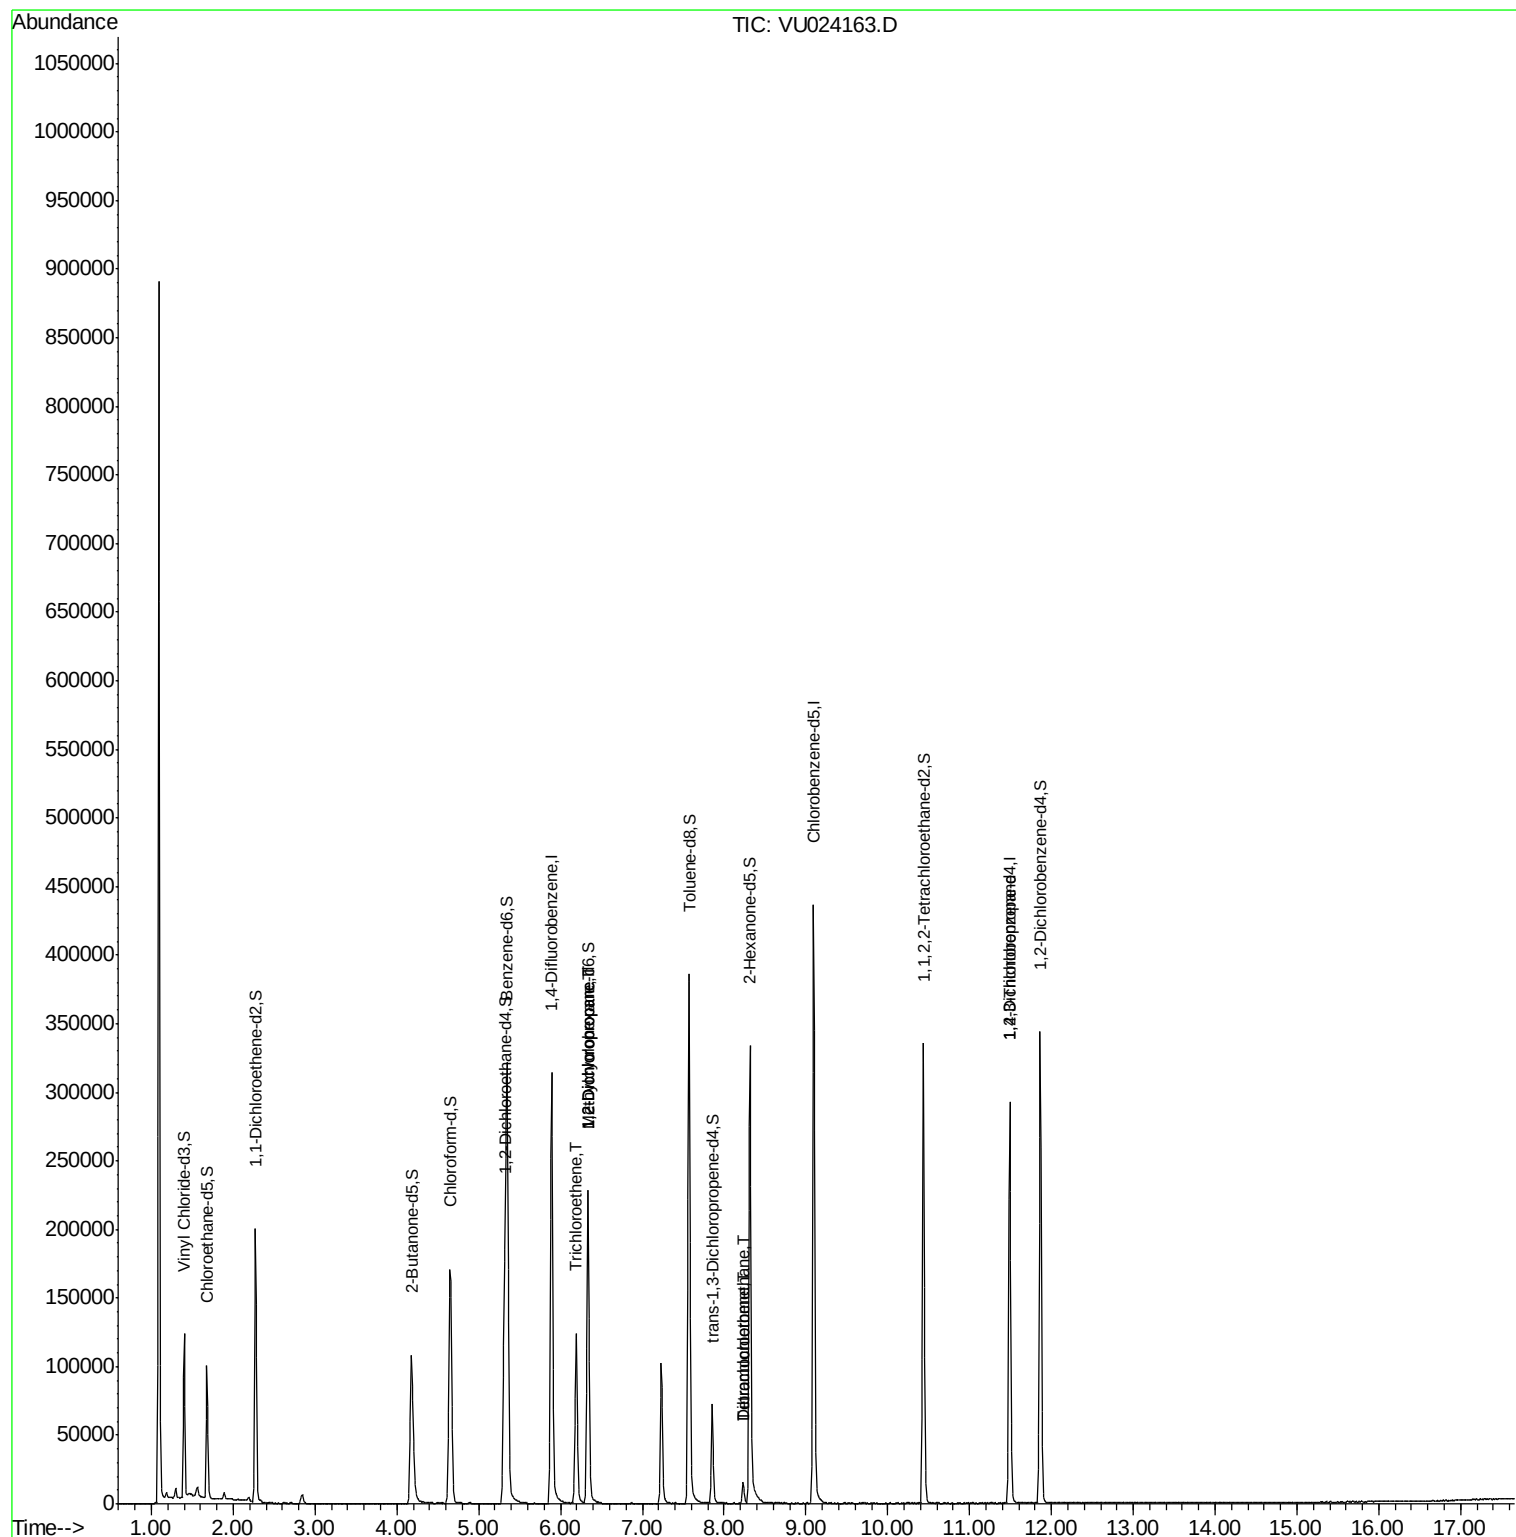

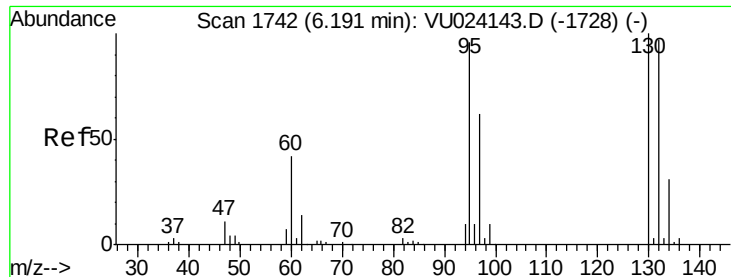

#34

Trichloroethene

Concen: 18.95 ug/L

RT: 6.19 min Scan# 1742

Delta R.T. 0.00 min

Lab File: VU024163.D

Acq: 26 May 2018 22:37

Tgt Ion: 95 Resp: 44977


Ion Ratio Lower Upper

95 100

97 64.9 44.5 82.7

132 100.8 69.0 128.2

130 105.5 70.6 131.0



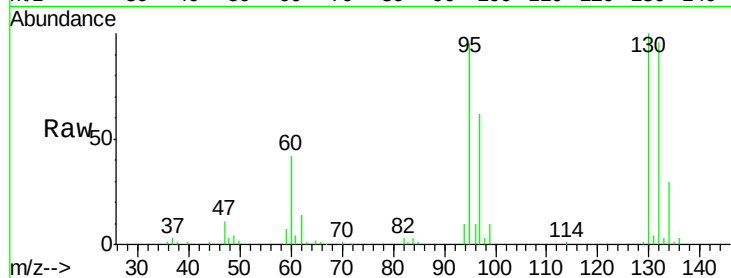


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

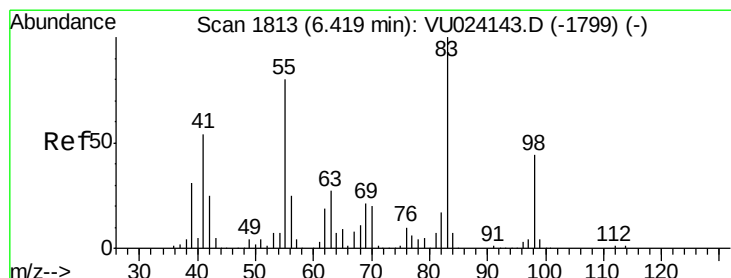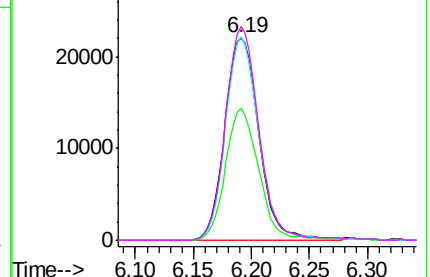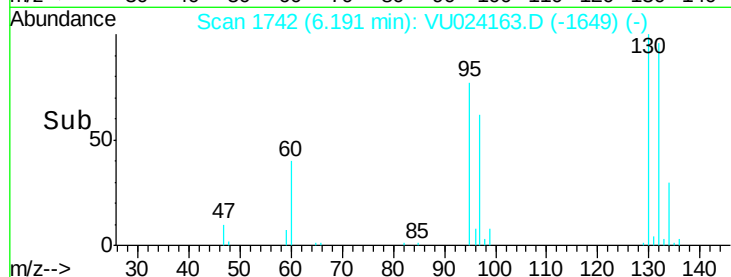

#35

Methylcyclohexane

Concen: 7.81 ug/L

RT: 6.33 min Scan# 1786

Delta R.T. -0.09 min

Lab File: VU024163.D

Acq: 26 May 2018 22:37


Tgt Ion: 83 Resp: 25665

Ion Ratio Lower Upper

83 100

55 0.0 64.1 96.1#



98 1.1 35.8 53.8#

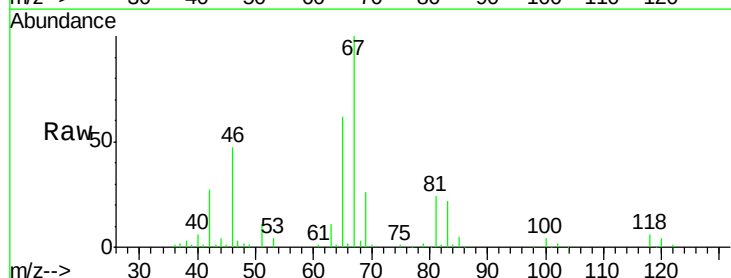


Abundance Ion 83.00 (82.70 to 83.70): VU0

Ion 55.00 (54.70 to 55.70): VU0





Ion 98.00 (97.70 to 98.70): VU0

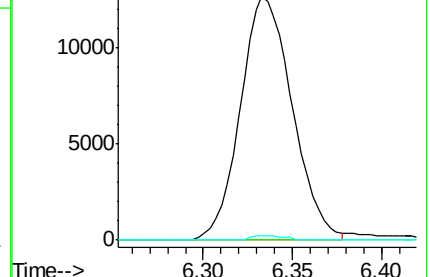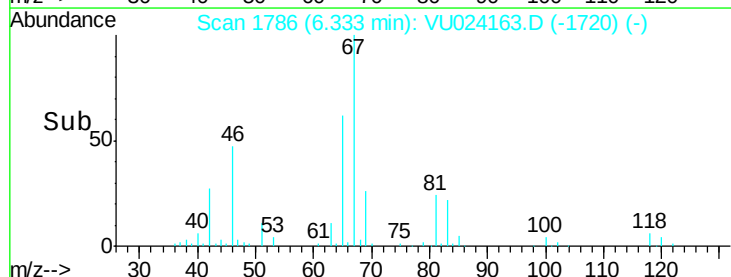

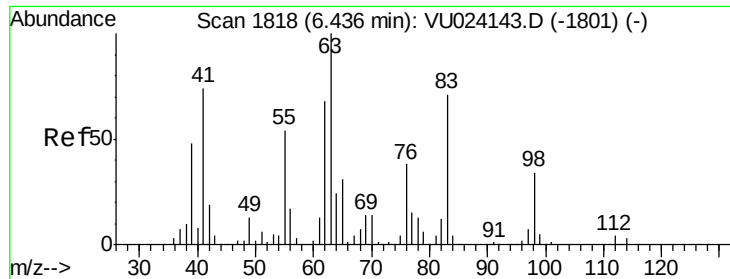




#37
 1,2-Dichloropropane
 Concen: 5.16 ug/L
 RT: 6.34 min Scan# 1787
 Delta R.T. -0.10 min
 Lab File: VU024163.D
 Acq: 26 May 2018 22:37


Tgt Ion: 63 Resp: 12229
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.9 4.3#

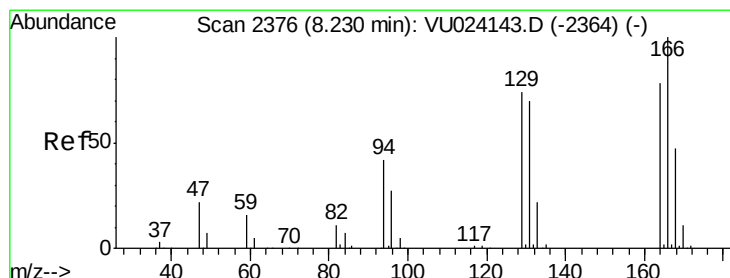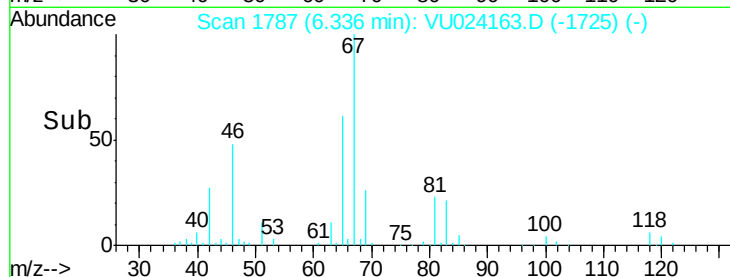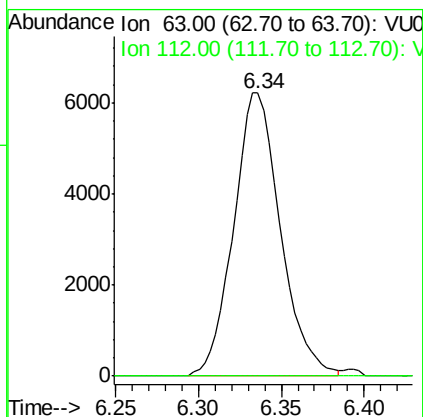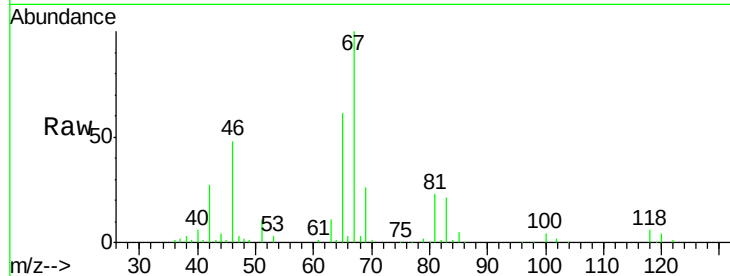

#46
 Tetrachloroethene
 Concen: 2.29 ug/L
 RT: 8.23 min Scan# 2377
 Delta R.T. 0.00 min
 Lab File: VU024163.D
 Acq: 26 May 2018 22:37

Tgt Ion: 164 Resp: 3806
 Ion Ratio Lower Upper
 164 100
 129 91.5 66.6 123.6
 131 87.9 64.5 119.9
 166 119.8 89.3 165.9

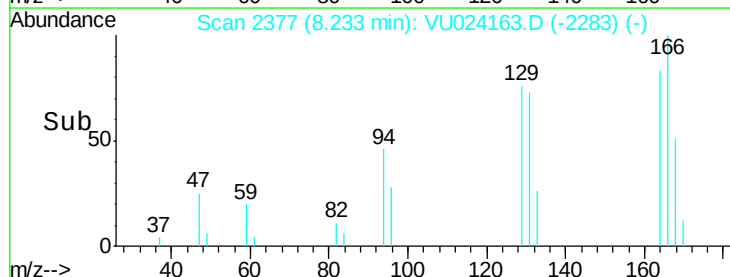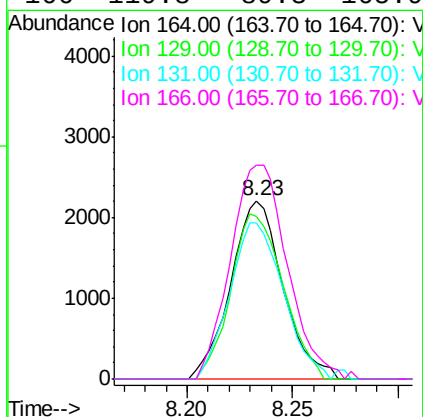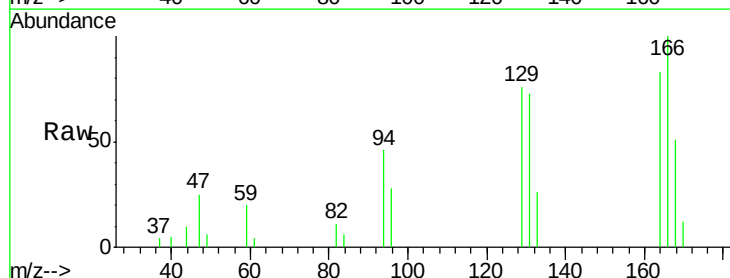

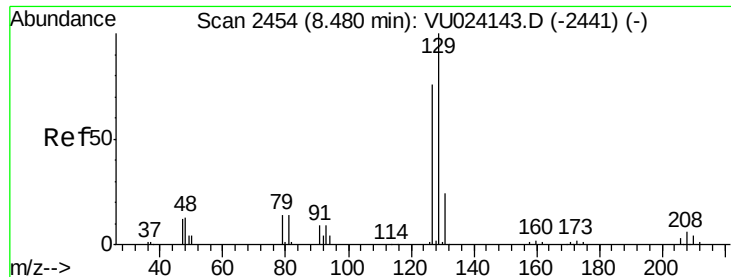

#49

Dibromochloromethane

Concen: 1.59 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. -0.25 min

Lab File: VU024163.D


Acq: 26 May 2018 22:37

Tgt Ion:129 Resp: 3526

Ion Ratio Lower Upper

129 100

127 0.0 54.2 100.6#

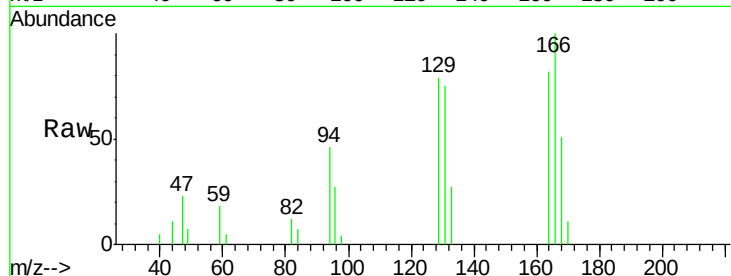

Abundance Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

8.23

2000

1500



1000

500

0

8.20 8.25

Time-->

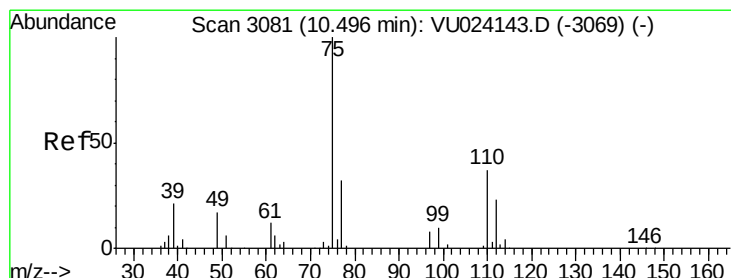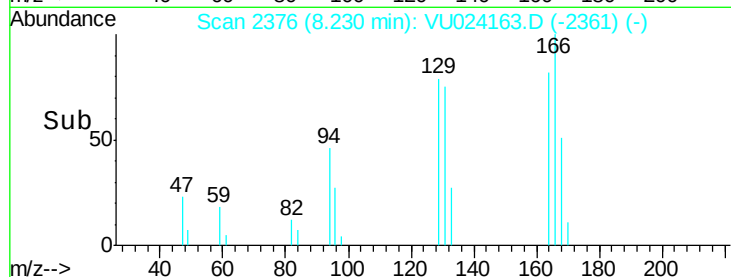

#59

1,2,3-Trichloropropane

Concen: 3.07 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU024163.D


Acq: 26 May 2018 22:37

Tgt Ion: 75 Resp: 9099

Ion Ratio Lower Upper

75 100

77 36.7 25.5 38.3

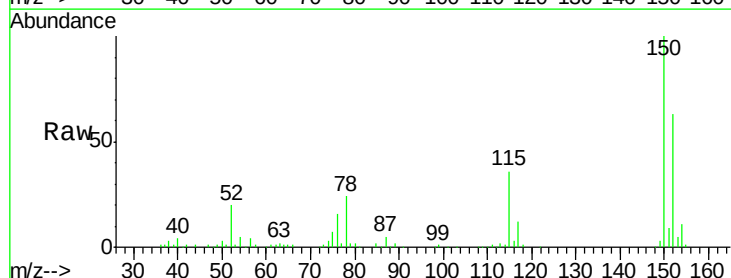

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

11.49

6000

5000

4000

3000

2000

1000

0

11.45 11.50 11.55

Time-->

