


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052618\
Data File : VU024142.D
Acq On : 26 May 2018 13:24
Operator : MD/SY
Sample : BFB59
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Title : VOC Analysis
Last Update : Mon May 28 05:15:39 2018

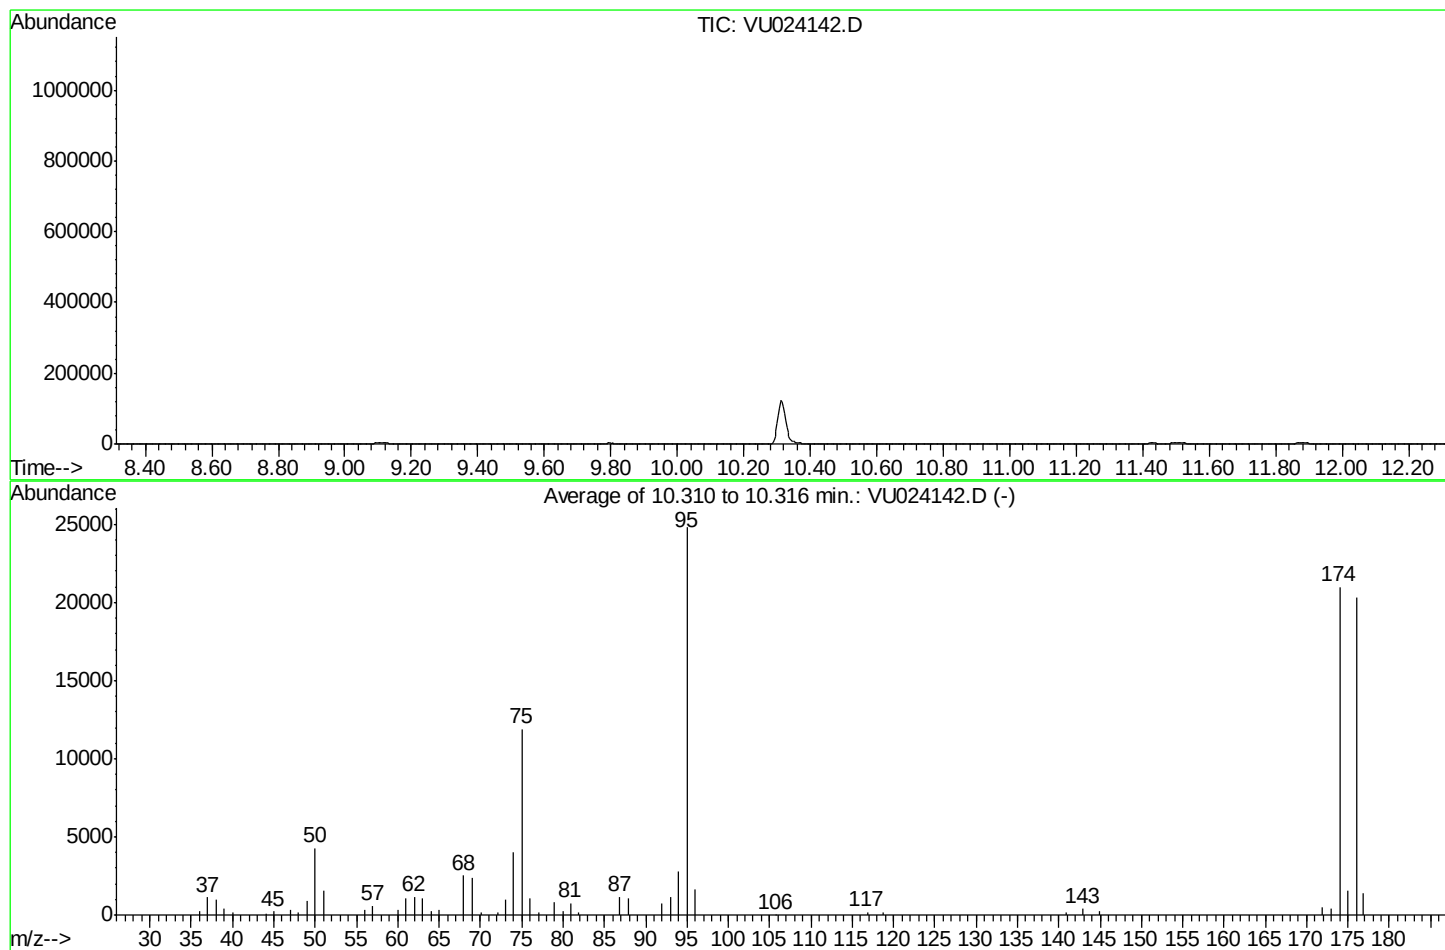

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4260	PASS
75	95	30	80	48.0	11918	PASS
95	95	100	100	100.0	24810	PASS
96	95	5	9	6.6	1640	PASS
173	174	0.00	2	1.9	395	PASS
174	95	50	120	84.6	20986	PASS
175	174	5	9	7.4	1548	PASS
176	174	95	101	96.8	20304	PASS
177	176	5	9	6.9	1394	PASS

Scan 3011 (10.271 min): VU024142.D
BFB59

m/z	Abundance
44.00	373.0

m/z	Abundance
36.00	238.0
37.00	1152.0
38.00	960.0
39.00	458.0
40.00	170.0
44.00	420.0
45.00	192.0
46.90	296.0
47.90	141.0
49.00	958.0
50.00	4342.0
51.00	1583.0
56.00	338.0
57.00	604.0
60.00	245.0
61.00	1067.0
62.00	1146.0
63.00	1056.0
64.00	262.0
65.00	340.0
68.00	2503.0
69.00	2353.0
70.00	203.0
72.10	185.0
73.00	930.0
74.00	4011.0
75.00	11712.0
76.00	1028.0
77.00	163.0
78.90	710.0
80.00	285.0
80.90	737.0
81.90	218.0
86.90	1197.0
87.90	1053.0
92.00	746.0
93.00	1156.0
94.00	2563.0
95.00	24312.0
96.00	1671.0
116.80	201.0
118.80	144.0
140.90	201.0
142.90	384.0
144.90	191.0
171.90	448.0
173.00	375.0
174.00	20232.0
174.90	1470.0
176.00	19640.0
176.90	1358.0

m/z	Abundance
35.90	244.0
37.00	1160.0
38.00	977.0
39.00	474.0
40.00	165.0
44.00	468.0
45.00	228.0
46.90	291.0
47.90	148.0
49.00	931.0
50.00	4385.0
51.00	1617.0
56.00	377.0
56.90	597.0
59.90	308.0
61.00	1070.0
62.00	1230.0
63.00	1075.0
64.00	280.0
65.00	299.0
68.00	2575.0
69.00	2444.0
70.10	166.0
72.10	178.0
73.00	1036.0
74.00	4120.0
75.00	12250.0
76.00	1074.0
77.00	178.0
78.90	790.0
79.90	273.0
80.90	753.0
81.90	207.0
86.90	1251.0
87.90	1105.0
92.00	754.0
93.00	1194.0
94.00	2831.0
95.00	25608.0
96.00	1702.0
105.80	107.0
116.90	178.0
118.80	154.0
140.90	198.0
142.90	426.0
145.00	241.0
171.90	479.0
172.90	415.0
174.00	21648.0
174.90	1599.0
176.00	20968.0
176.90	1418.0

m/z	Abundance
35.90	245.0
37.00	1053.0
38.00	898.0
39.00	423.0
40.00	126.0
44.00	505.0
45.00	220.0
47.00	283.0
47.90	145.0
49.00	811.0
50.00	4053.0
51.00	1451.0
56.00	364.0
56.90	555.0
59.90	322.0
61.00	1026.0
62.00	1158.0
63.00	984.0
64.00	247.0
65.00	234.0
68.00	2441.0
69.00	2332.0
70.00	117.0
72.20	143.0
73.00	1041.0
74.00	3853.0
75.00	11793.0
76.00	1011.0
77.00	182.0
78.90	843.0
79.90	218.0
80.90	727.0
81.80	186.0
86.90	1112.0
87.90	1023.0
92.00	723.0
93.00	1130.0
94.00	2926.0
95.00	24512.0
96.00	1547.0
116.90	178.0
118.80	165.0
140.90	163.0
143.00	380.0
145.00	256.0
171.90	441.0
172.90	395.0
174.00	21080.0
174.90	1575.0
176.00	20304.0
176.90	1407.0