

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052620\
 Data File : VU038299.D
 Acq On : 26 May 2020 16:13
 Operator : JC/MD
 Sample : L2751-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y25

Quant Time: May 27 07:44:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 27 06:51:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	316910	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	304614	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	148953	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	98076	3.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.60%
7) Chloroethane-d5	1.93	69	86812	3.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.20%
11) 1,1-Dichloroethene-d2	2.59	63	146692	3.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.60%
20) 2-Butanone-d5	4.66	46	339063	47.41	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.82%
24) Chloroform-d	5.10	84	203012	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.74	65	117357	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.76	84	421625	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
36) 1,2-Dichloropropane-d6	6.72	67	131310	4.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.20%
41) Toluene-d8	7.92	98	381047	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	8.20	79	52118	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.65	63	272673	48.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.86%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	111482	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	150865	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.65	43	11173	2.490 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052620\
Data File : VU038299.D
Acq On : 26 May 2020 16:13
Operator : JC/MD
Sample : L2751-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y25

Quant Time: May 27 07:44:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 27 06:51:51 2020
Response via : Initial Calibration

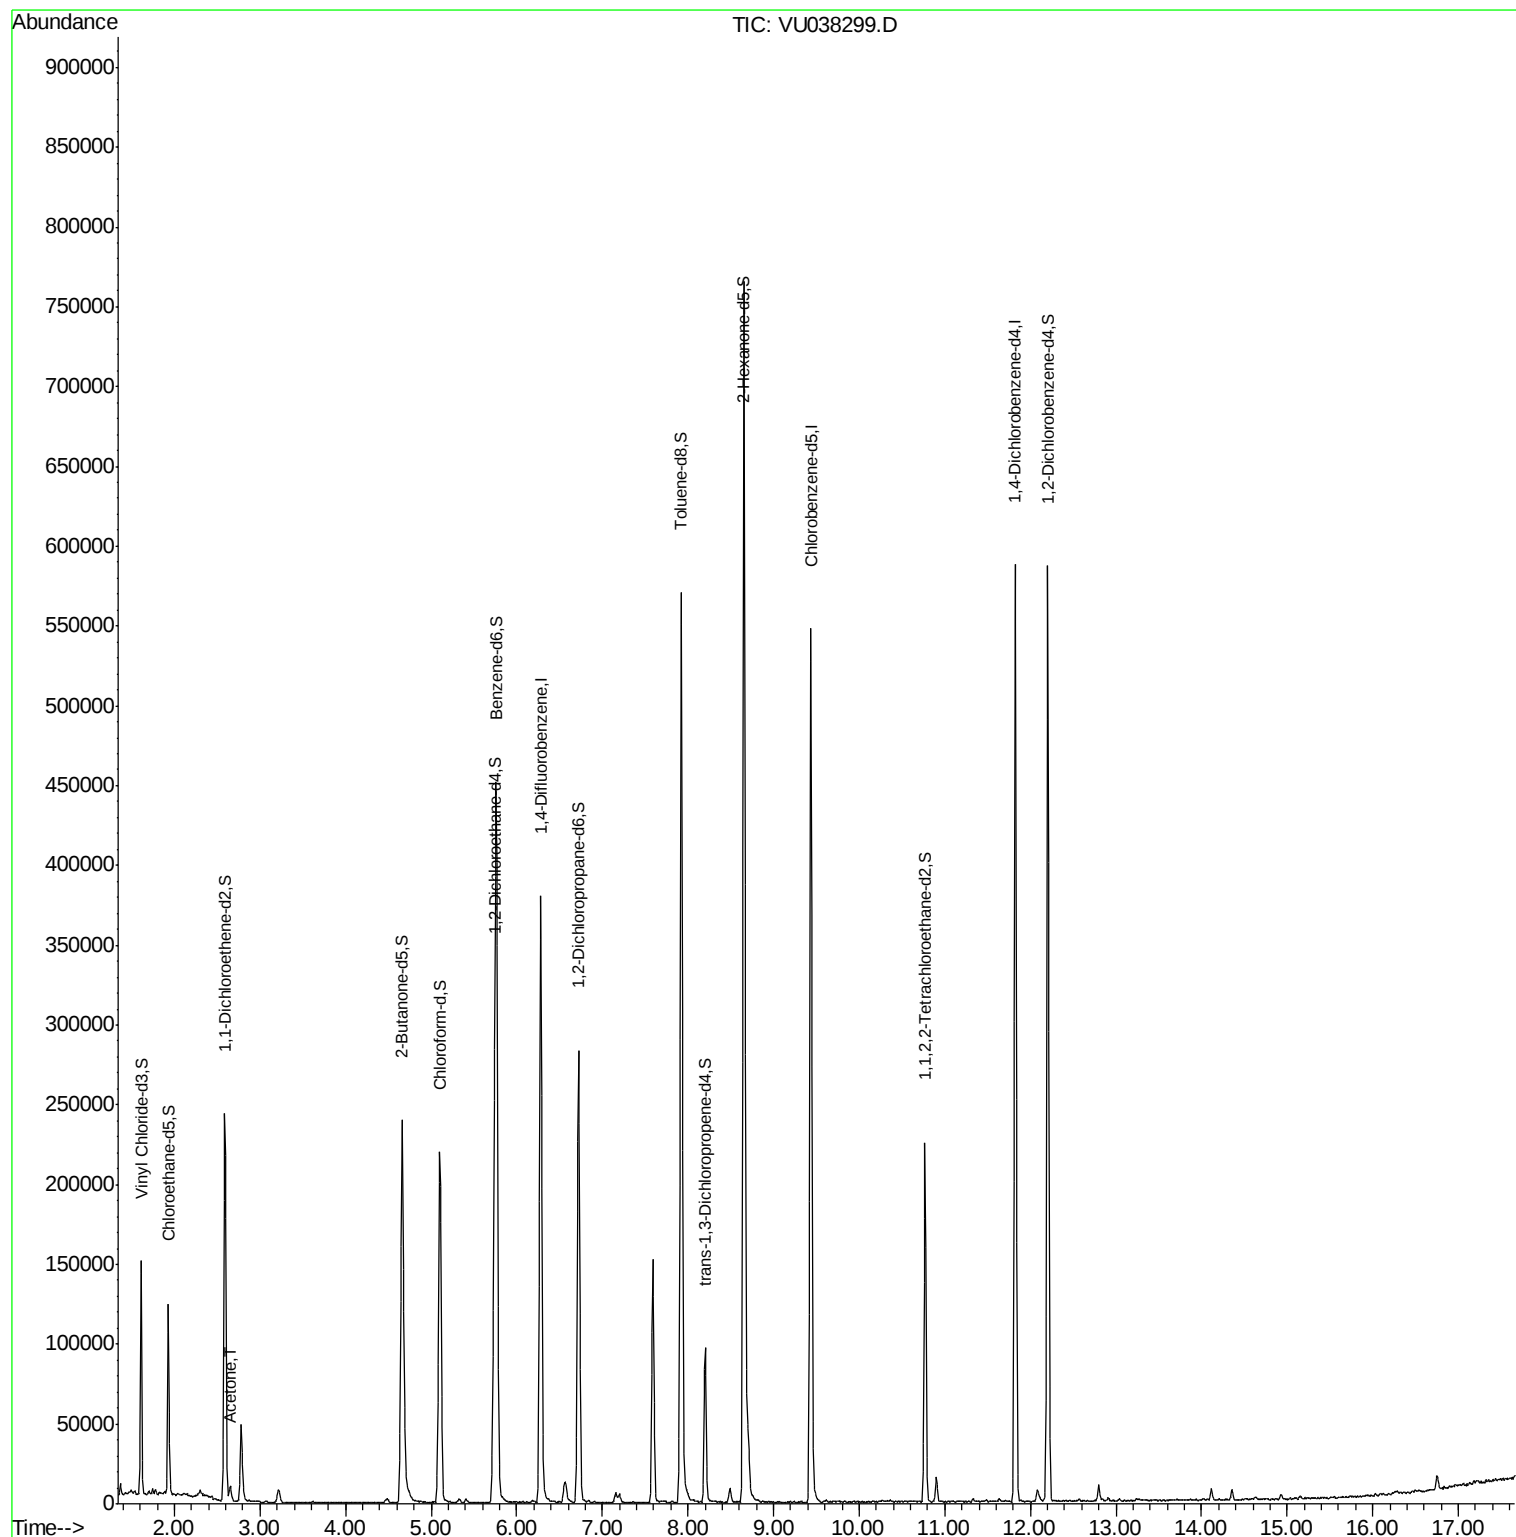

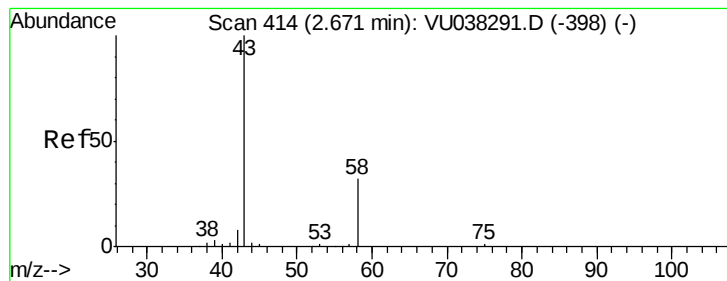

#13
 Acetone
 Concen: 2.490 ug/L
 RT: 2.65 min Scan# 408
 Delta R.T. -0.02 min
 Lab File: VU038299.D
 Acq: 26 May 2020 16:13

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y25

Tot Ion: 43 Resp: 11173
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 63.6

