

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052620\
 Data File : VU038301.D
 Acq On : 26 May 2020 16:59
 Operator : JC/MD
 Sample : L2751-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y27

Quant Time: May 27 07:53:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 27 06:51:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	309137	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	303257	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	147124	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	95042	3.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.20%
7) Chloroethane-d5	1.93	69	84724	3.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.20%
11) 1,1-Dichloroethene-d2	2.59	63	142474	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.66	46	325628	46.67	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.34%
24) Chloroform-d	5.10	84	198409	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.74	65	115105	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.76	84	414085	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.72	67	132168	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.20%
41) Toluene-d8	7.92	98	373557	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	8.20	79	51037	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.65	63	257690	46.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.90%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	105229	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	145602	5.08	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.60%


Target Compounds					Ovalue
13) Acetone	2.65	43	4711	1.076 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052620\
Data File : VU038301.D
Acq On : 26 May 2020 16:59
Operator : JC/MD
Sample : L2751-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y27

Quant Time: May 27 07:53:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 27 06:51:51 2020
Response via : Initial Calibration

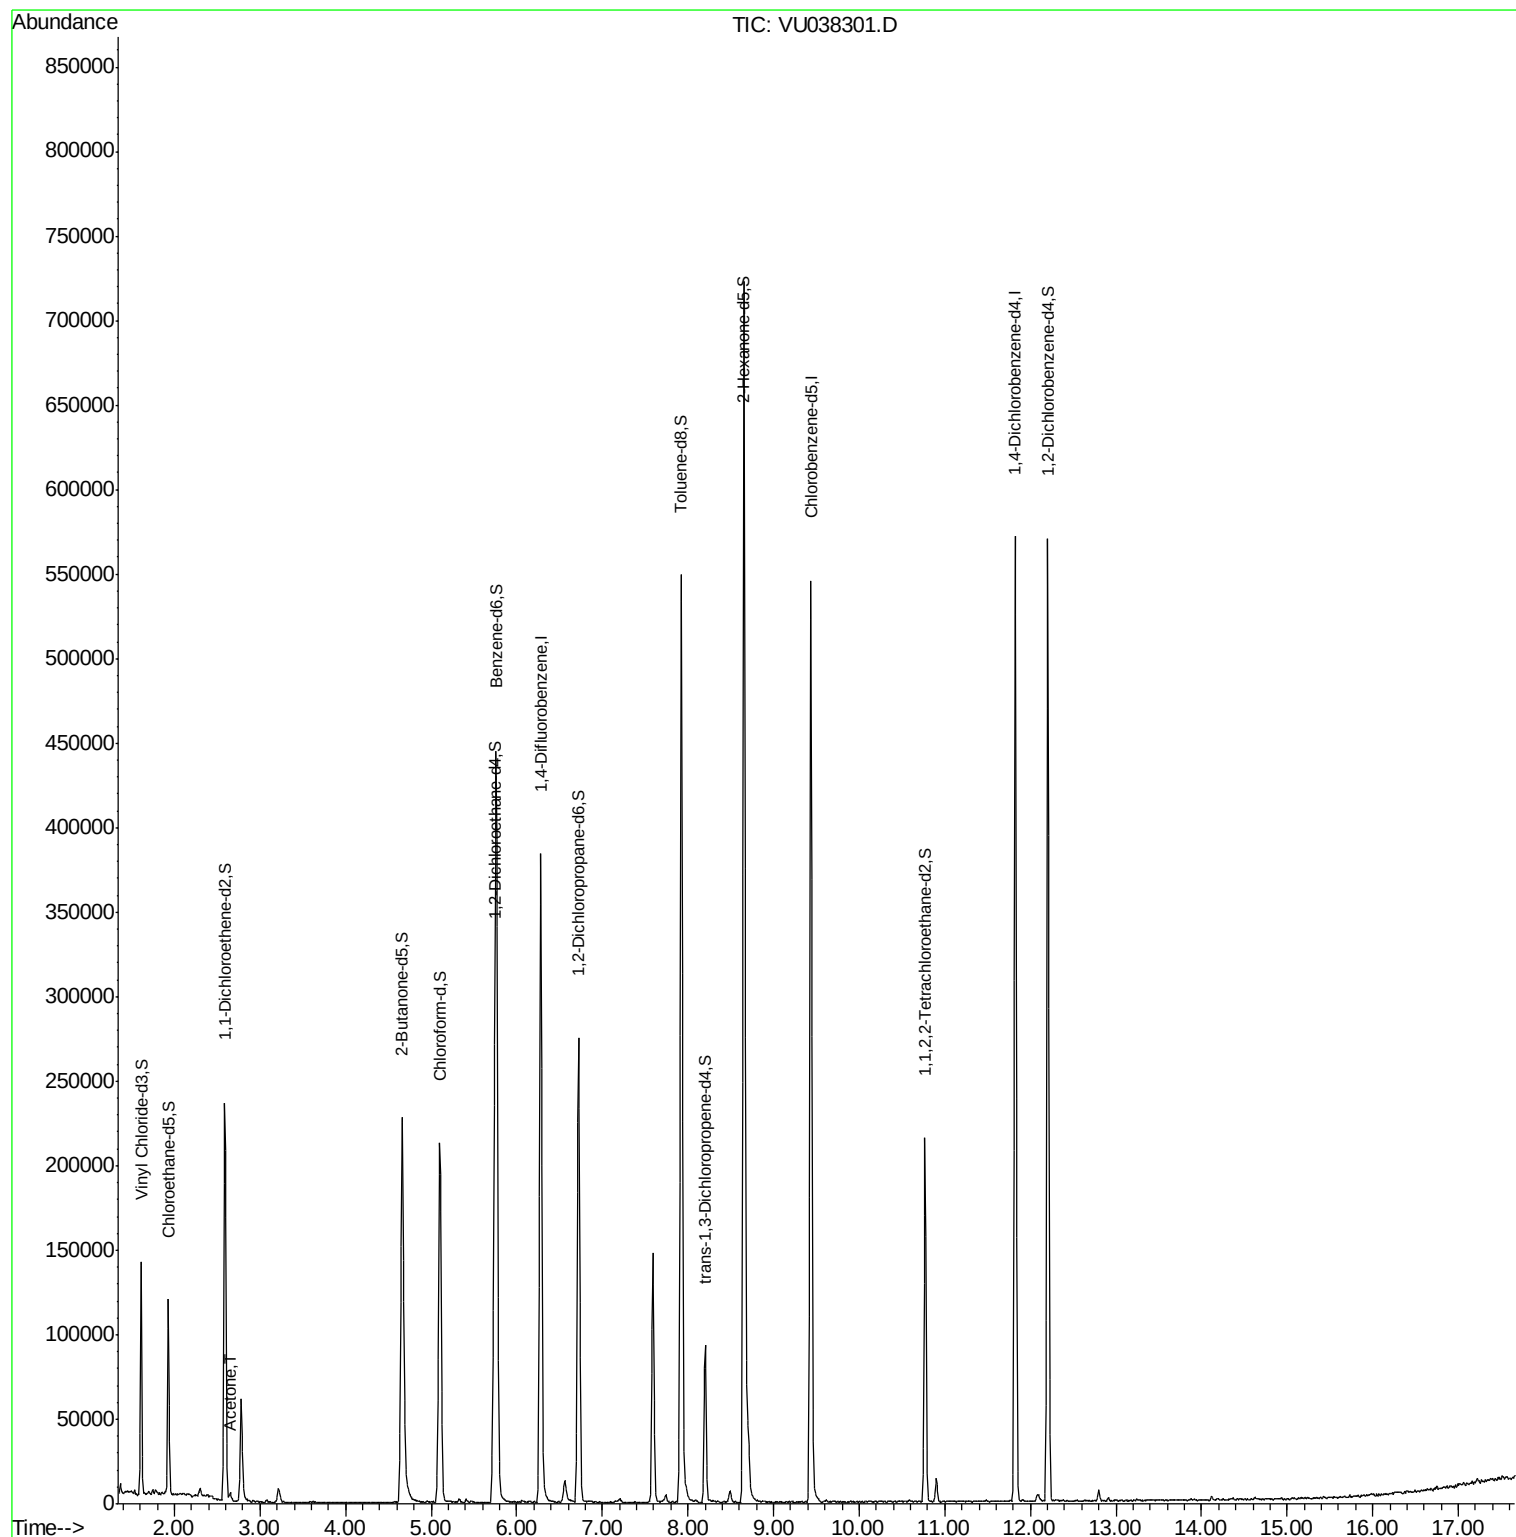

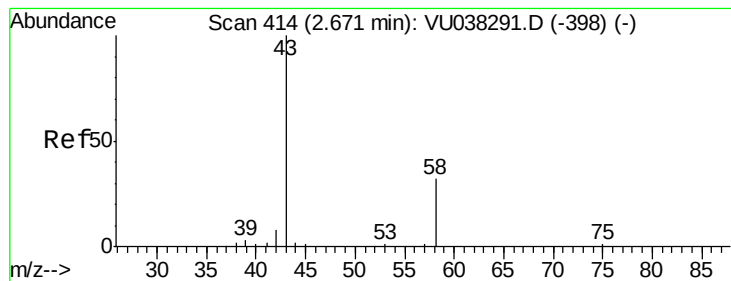

#13
 Acetone
 Concen: 1.076 ug/L
 RT: 2.65 min Scan# 408
 Delta R.T. -0.02 min
 Lab File: VU038301.D
 Acq: 26 May 2020 16:59

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y27

Tot Ion: 43 Resp: 4711
 Ion Ratio Lower Upper
 43 100
 58 34.7 0.0 63.6

