


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU052620\
 Data File : VU038290.D
 Acq On : 26 May 2020 08:55
 Operator : JC/MD
 Sample : BFB30
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB30

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052620W.M
 Title : SW846 8260
 Last Update : Tue May 26 16:32:50 2020

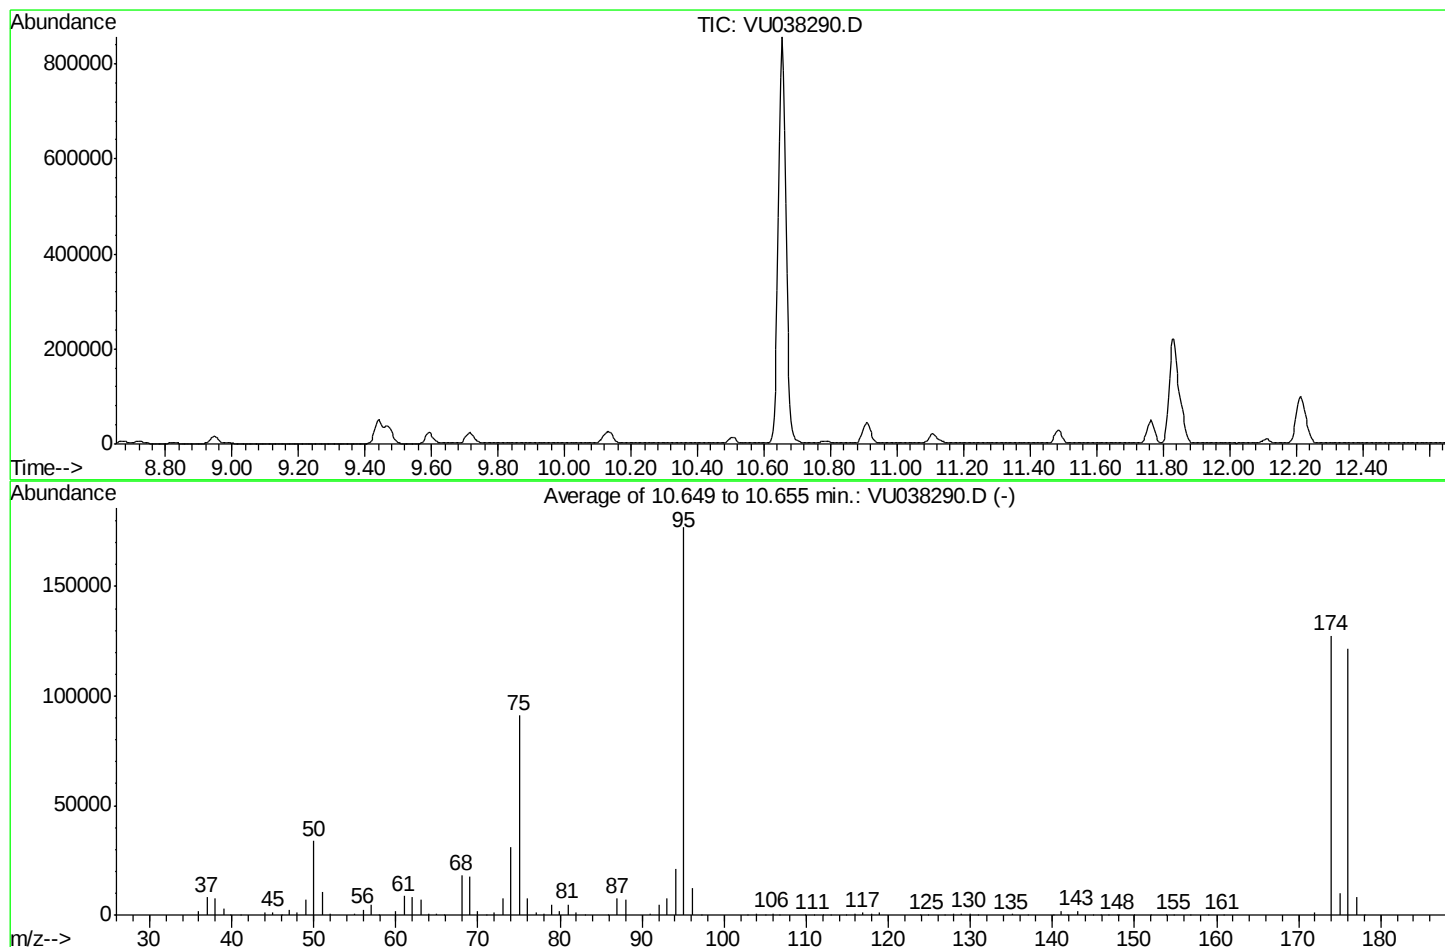

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	33882	PASS
75	95	30	60	51.5	91112	PASS
95	95	100	100	100.0	177066	PASS
96	95	5	9	6.9	12252	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.1	127741	PASS
175	174	5	9	8.0	10180	PASS
176	174	95	101	95.4	121912	PASS
177	176	5	9	6.8	8283	PASS

m/z	Abundance
36.00	2175.0
37.00	7599.0
38.00	7167.0
39.00	2731.0
39.90	293.0
41.00	109.0
43.00	122.0
44.00	1829.0
45.00	1336.0
47.10	2082.0
47.90	1217.0
49.00	6896.0
50.00	32048.0
51.00	10012.0
52.00	355.0
55.00	410.0
56.00	2549.0
57.00	4233.0
57.90	277.0
60.00	1708.0
61.00	7985.0
62.00	7756.0
63.00	6418.0
64.10	532.0
65.00	595.0
65.90	112.0
68.00	16560.0
69.00	16472.0
70.00	1440.0
71.00	153.0
72.00	1065.0
73.10	6803.0
74.00	29424.0
75.00	84888.0
76.10	7191.0
77.10	1105.0
78.10	774.0
78.90	4656.0
80.00	1376.0
81.00	4471.0
82.00	965.0
83.10	109.0
85.80	240.0
87.00	6948.0
88.00	6569.0
91.00	662.0
92.00	4621.0
93.00	7088.0
94.10	20312.0
95.10	166592.0
96.10	11584.0
97.20	161.0
104.00	555.0
104.90	220.0
106.00	755.0
111.00	171.0
112.10	105.0
113.00	183.0
114.90	136.0
115.90	572.0
117.00	1087.0
118.00	861.0
118.90	856.0
123.90	109.0
124.80	113.0
128.00	397.0
128.90	394.0
129.90	576.0
130.90	209.0
135.10	421.0
136.90	306.0
140.10	162.0
141.00	1424.0
141.80	220.0
143.00	1482.0
144.90	279.0
146.00	214.0
146.80	118.0
147.90	302.0
149.90	137.0
153.90	126.0
154.80	242.0
156.80	154.0
160.80	100.0
172.00	923.0
174.00	116984.0
175.10	9689.0
176.10	110864.0
177.00	7713.0
178.00	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
36.00	2277.0
37.00	8184.0
38.00	7903.0
39.00	3079.0
39.90	271.0
41.00	122.0
44.00	1994.0
45.00	1363.0
46.10	196.0
47.00	2206.0
47.90	1283.0
49.00	7330.0
50.00	34880.0
51.00	10944.0
52.00	523.0
55.00	381.0
56.00	2716.0
57.00	4568.0
57.80	264.0
60.00	1587.0
61.00	8843.0
62.00	8464.0
63.00	6927.0
64.10	556.0
64.90	566.0
65.90	119.0
68.00	18456.0
69.00	18008.0
70.00	1567.0
71.00	161.0
72.00	1161.0
73.00	7694.0
74.00	31680.0
75.00	94208.0
76.10	7698.0
77.10	1139.0
78.00	838.0
78.90	5018.0
79.90	1554.0
81.00	5028.0
81.90	1097.0
83.10	143.0
85.80	191.0
87.00	7792.0
88.00	7040.0
91.00	696.0
92.00	5062.0
93.00	7571.0
94.10	22032.0
95.10	182400.0
96.10	12645.0
97.20	213.0
102.90	104.0
104.00	634.0
105.00	318.0
106.00	727.0
106.70	112.0
110.90	224.0
112.00	123.0
113.00	191.0
114.80	184.0
115.90	665.0
117.00	1113.0
118.00	898.0
118.90	1045.0
127.90	557.0
129.00	373.0
129.90	674.0
130.80	206.0
135.10	534.0
137.00	275.0
140.10	181.0
141.00	1510.0
141.90	236.0
143.00	1824.0
144.90	312.0
146.00	267.0
146.80	101.0
148.10	316.0
149.90	180.0
153.90	135.0
154.80	296.0
156.90	196.0
159.00	153.0
160.90	157.0
172.00	965.0
174.00	131392.0
175.10	10460.0
176.10	125144.0
177.10	8515.0
178.00	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	2296.0
37.00	8282.0
38.00	8079.0
39.00	3025.0
39.90	259.0
44.00	1882.0
45.00	1346.0
46.10	173.0
47.00	2199.0
48.00	1104.0
49.00	7159.0
50.00	34720.0
51.00	10771.0
52.00	571.0
54.90	369.0
56.10	2567.0
57.00	4526.0
57.80	240.0
60.00	1406.0
61.00	8984.0
62.00	8443.0
63.00	6965.0
64.00	457.0
64.90	462.0
68.00	18712.0
69.10	17896.0
70.00	1512.0
71.00	100.0
72.00	1191.0
73.00	7824.0
74.00	31176.0
75.00	94240.0
76.00	7847.0
77.10	1079.0
78.00	899.0
78.90	4953.0
79.90	1525.0
80.90	5223.0
81.90	1097.0
83.10	141.0
85.80	109.0
87.00	7850.0
88.00	6964.0
91.00	726.0
92.10	5245.0
93.00	7429.0
94.10	21424.0
95.10	182208.0
96.10	12529.0
97.10	279.0
102.90	106.0
104.00	697.0
105.00	313.0
105.90	776.0
106.80	126.0
109.90	107.0
110.90	211.0
111.90	133.0
113.00	181.0
114.80	209.0
115.90	725.0
116.90	1069.0
118.00	821.0
118.90	1096.0
126.90	107.0
127.90	693.0
129.00	289.0
129.90	703.0
130.80	217.0
135.10	470.0
137.00	267.0
140.10	167.0
141.00	1546.0
142.00	223.0
143.00	2075.0
144.90	300.0
145.90	297.0
148.00	327.0
149.90	193.0
151.90	104.0
153.90	103.0
154.90	348.0
156.90	238.0
158.90	192.0
160.90	198.0
172.00	872.0
174.00	134848.0
175.00	10392.0
176.00	129728.0
177.10	8623.0
178.00	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

Scan 2882 (10.607 min): VU038290.D
BFB30

m/z	Abundance
36.00	763.0
37.90	250.0
39.80	220.0
42.90	113.0
44.00	792.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30