

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
 Data File : VU043981.D
 Acq On : 26 May 2021 13:24
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 27 01:37:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 27 01:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	15366	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	13806	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.759	152	6230	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	3821	0.41	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	82.00%		
4) 1,2-Dichloroethane-d4	5.679	65	6544	0.47	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.00%		
7) 1,2-Dichloropropane-d6	6.658	67	7610	0.57	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	114.00%		
8) Toluene-d8	7.845	98	14802	0.54	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	108.00%		
10) 1,1,2,2-Tetrachloroeth...	10.696	84	7076	0.56	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	112.00%		
Target Compounds						
12) 1,2,3-Trichloropropane	10.748	75	207	0.02	ug/L	Qvalue # 89
13) 1,2-Dibromo-3-chloropr...	12.924	75	86	0.05	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
Data File : VU043981.D
Acq On : 26 May 2021 13:24
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :

Quant Time: May 27 01:37:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 27 01:35:45 2021
Response via : Initial Calibration




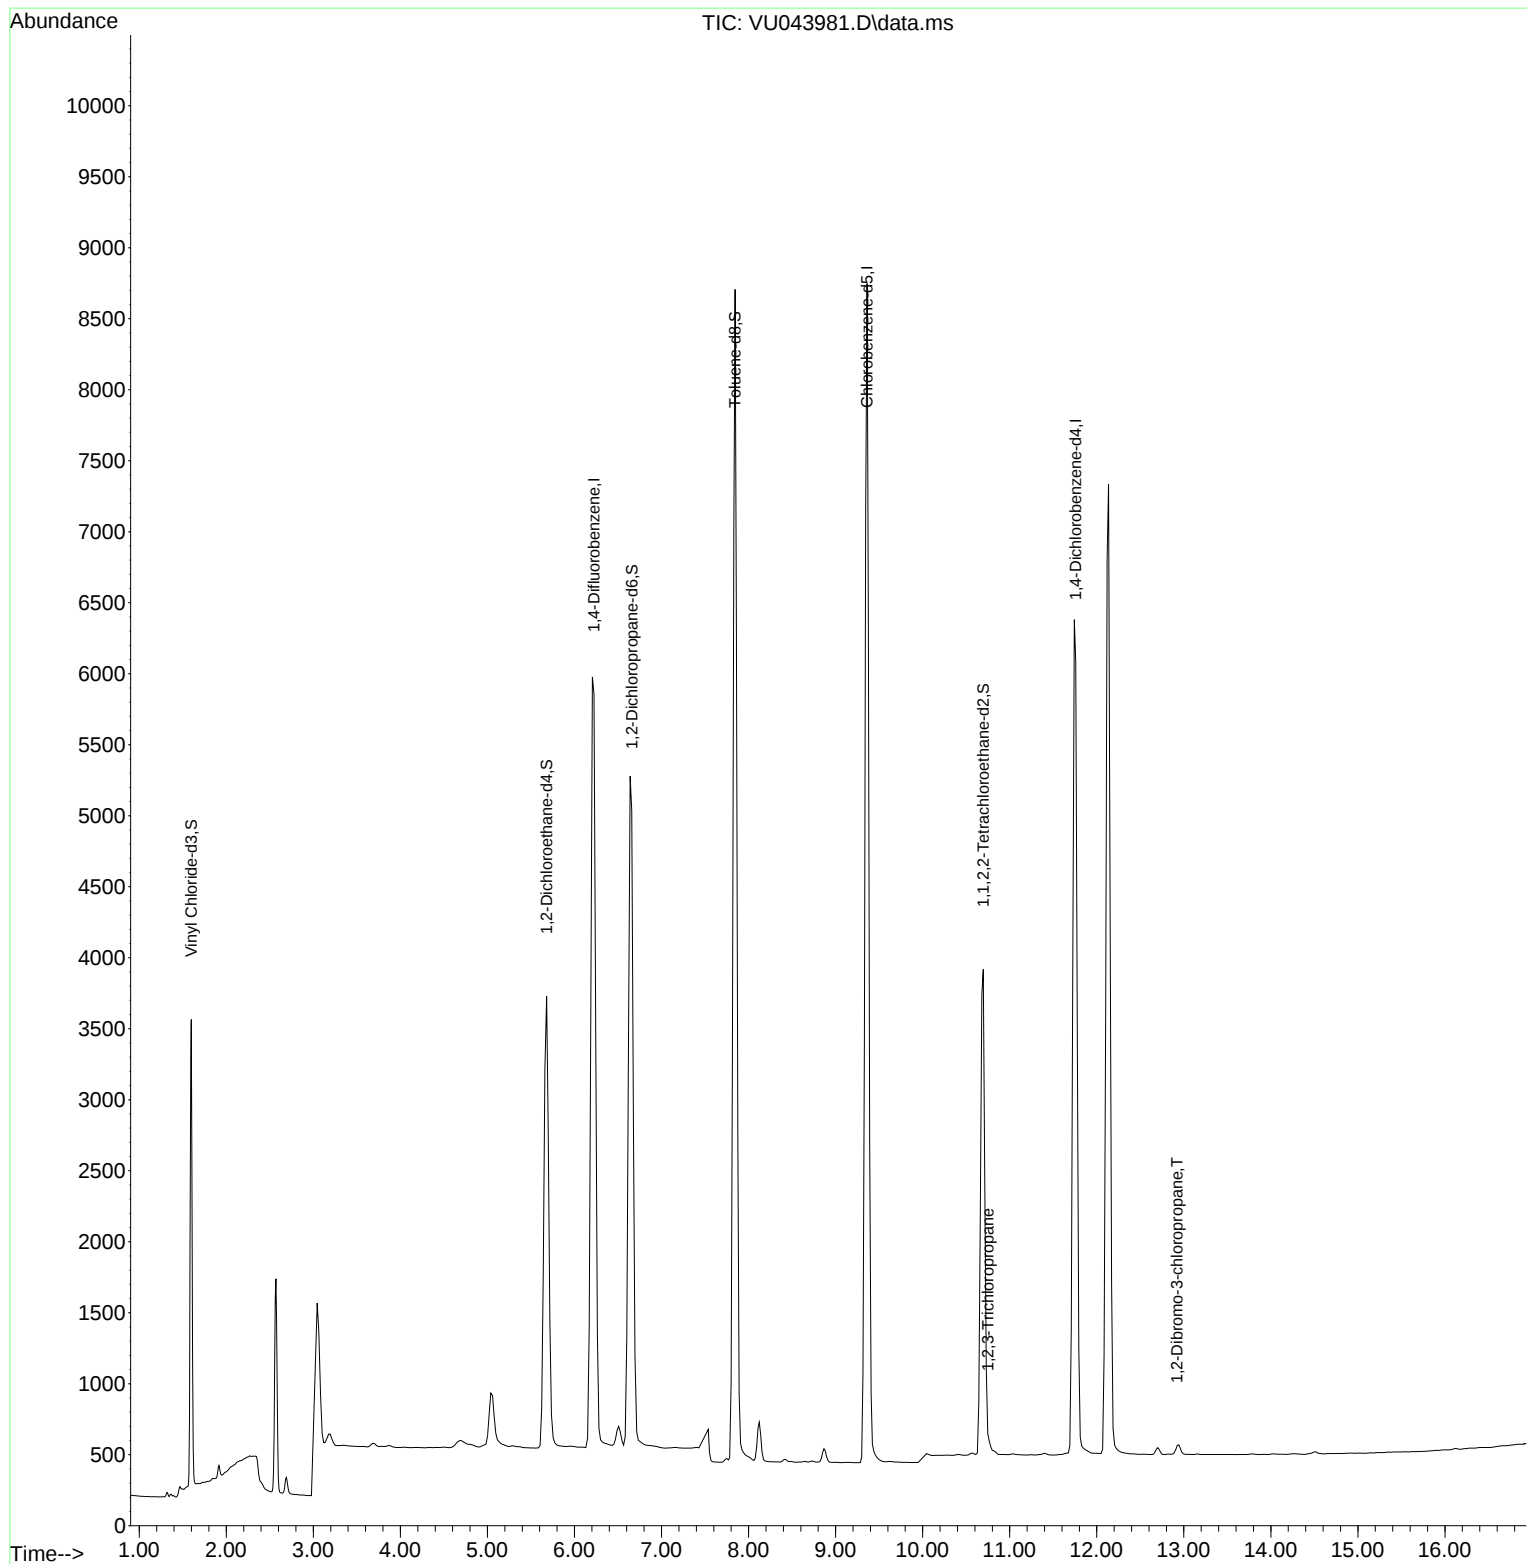


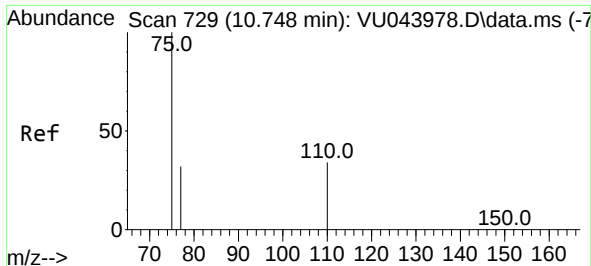

#12
1,2,3-Trichloropropane
Concen: 0.02 ug/L
RT: 10.748 min Scan# 729
Delta R.T. -0.000 min
Lab File: VU043981.D
Acq: 26 May 2021 13:24

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion:	75	Resp:	207
Ion	Ratio	Lower	Upper
75	100		
110	34.8	30.8	46.2
77	41.5	26.2	39.2

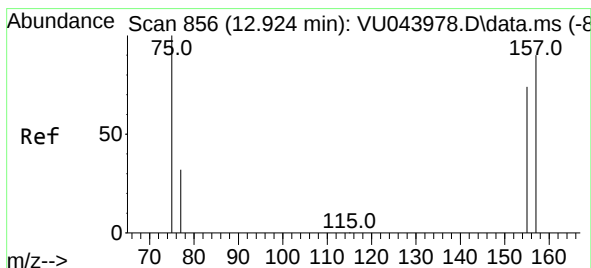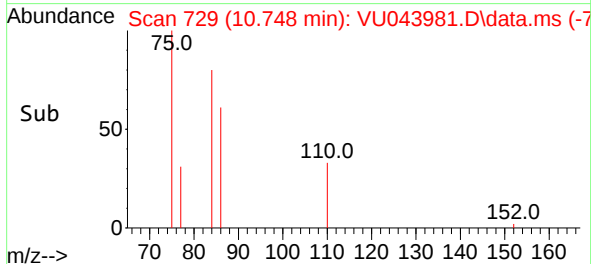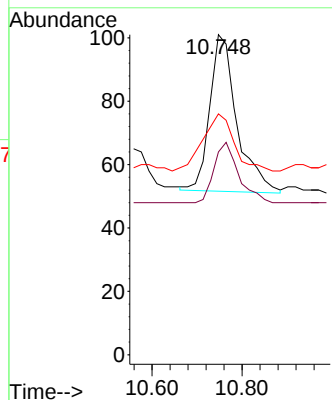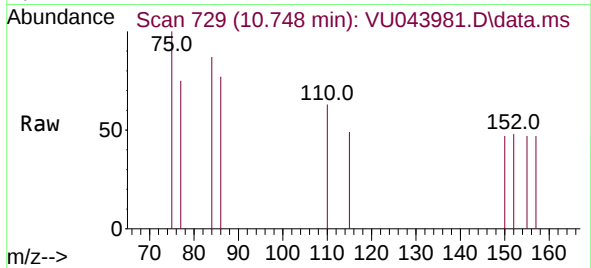

#13
1,2-Dibromo-3-chloropropane
Concen: 0.05 ug/L
RT: 12.924 min Scan# 856
Delta R.T. -0.000 min
Lab File: VU043981.D
Acq: 26 May 2021 13:24

Tgt Ion:	75	Resp:	86
Ion	Ratio	Lower	Upper
75	100		
157	90.5	71.8	107.8
155	85.1	61.2	91.8

