

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
 Data File : VU043984.D
 Acq On : 26 May 2021 17:42
 Operator : SY/MD
 Sample : VU0526WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 27 01:37:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 27 01:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	15024	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	14041	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.759	152	6308	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.605	65	4366	0.48	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	96.00%		
4) 1,2-Dichloroethane-d4	5.679	65	6358	0.46	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.00%		
7) 1,2-Dichloropropane-d6	6.658	67	7386	0.55	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	110.00%		
8) Toluene-d8	7.845	98	13914	0.50	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.00%		
10) 1,1,2,2-Tetrachloroeth...	10.696	84	7413	0.58	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	116.00%		
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.924	75	25	0.01	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
Data File : VU043984.D
Acq On : 26 May 2021 17:42
Operator : SY/MD
Sample : VU0526WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :


Quant Time: May 27 01:37:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 27 01:35:45 2021
Response via : Initial Calibration

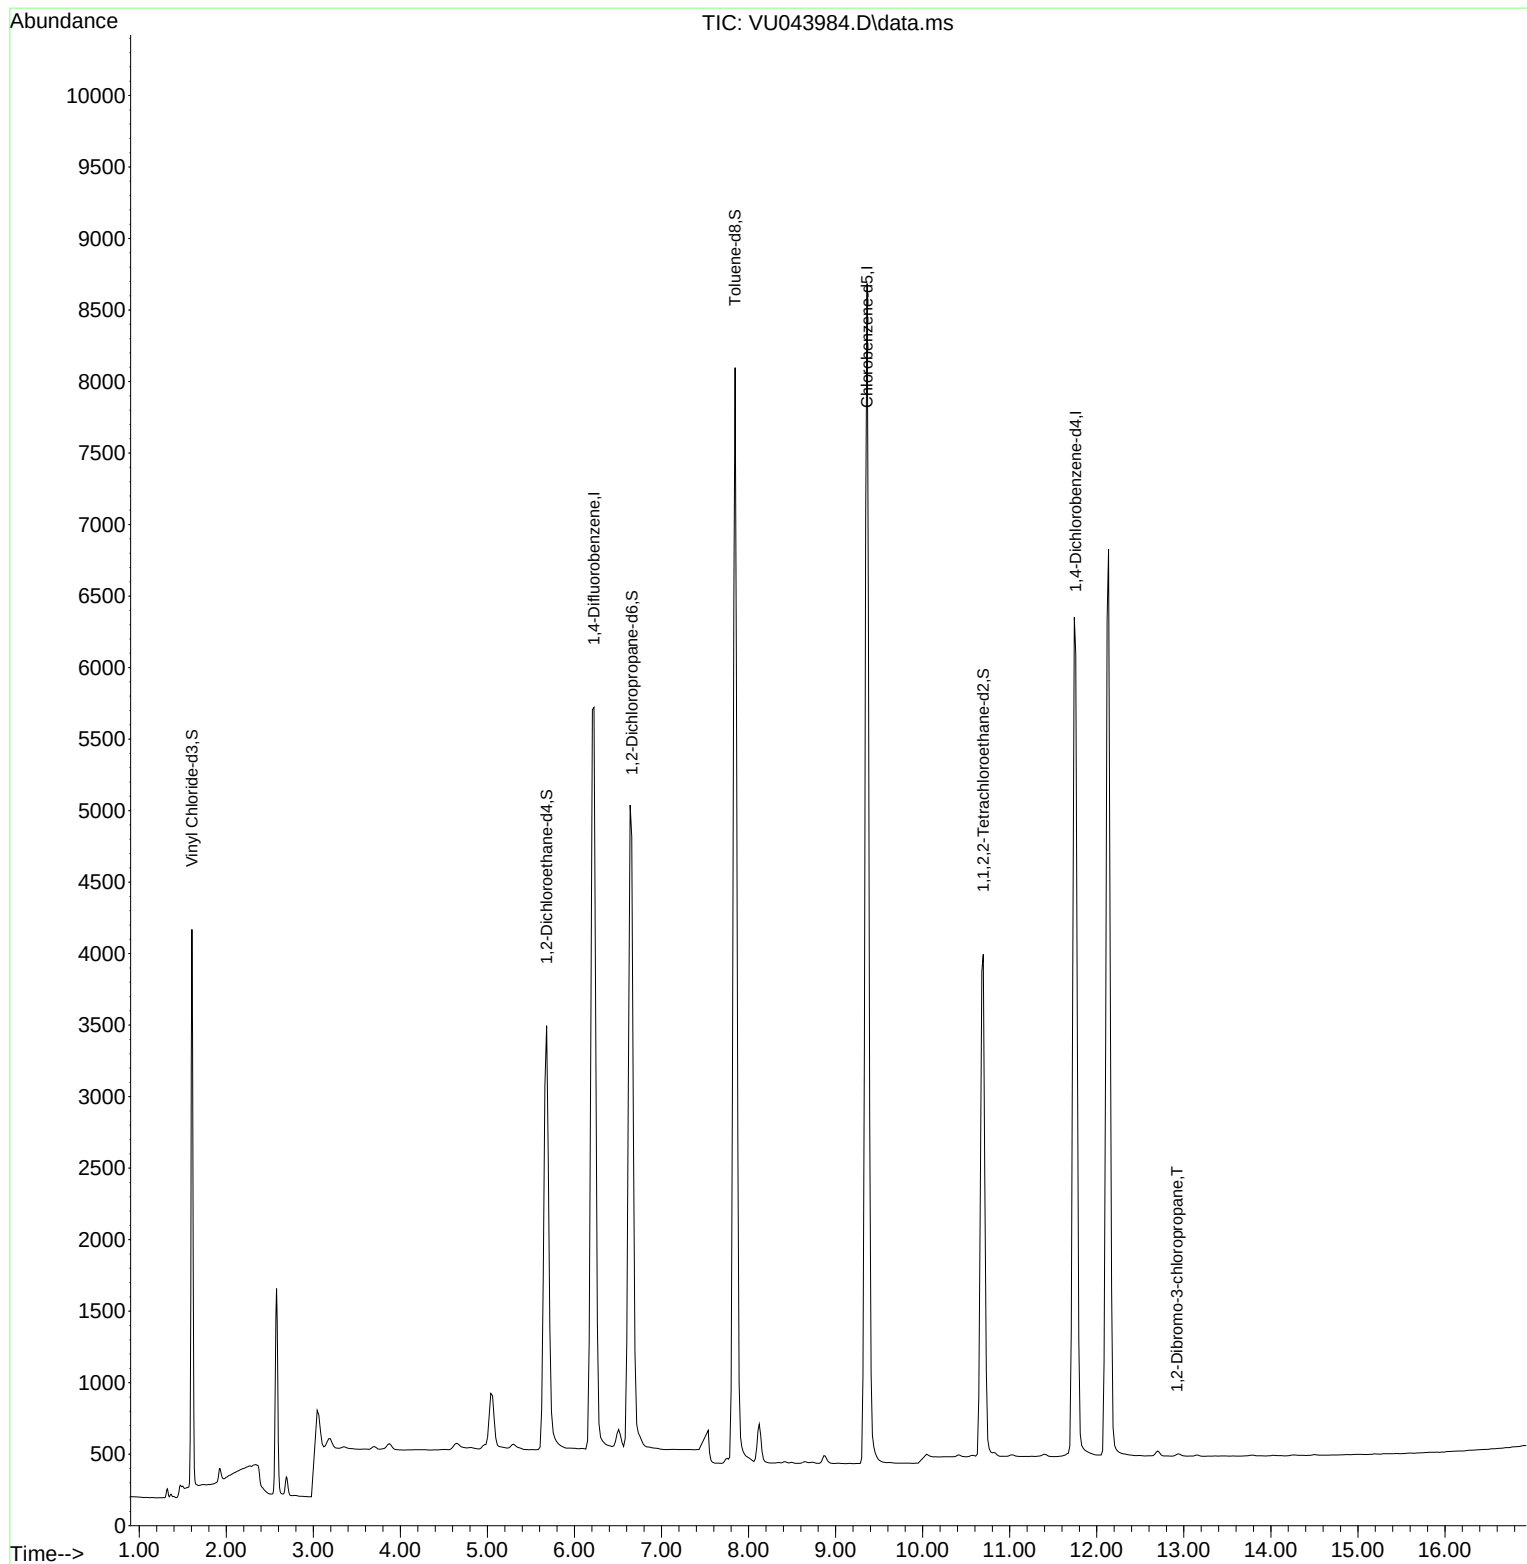

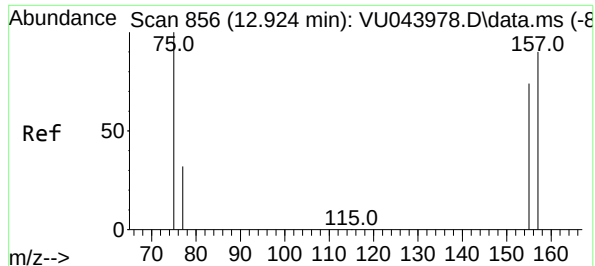

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.01 ug/L
 RT: 12.924 min Scan# 856
 Delta R.T. -0.000 min
 Lab File: VU043984.D
 Acq: 26 May 2021 17:42

Instrument :
 MSVOA_U
 ClientSampleId :

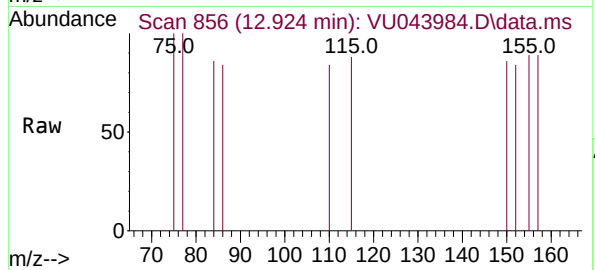

Tgt Ion: 75	Resp: 25
Ion Ratio	Lower Upper
75 100	
157 89.3	71.8 107.8
155 89.3	61.2 91.8

