




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
 Data File : VU043977.D
 Acq On : 26 May 2021 11:44
 Operator : SY/MD
 Sample : VSTD0.131
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.1131

Manual Integrations
 APPROVED

MMDadoda
 5/28/2021 3:04:58 PM

Quant Time: May 27 01:28:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 27 01:26:40 2021
 Response via : Initial Calibration

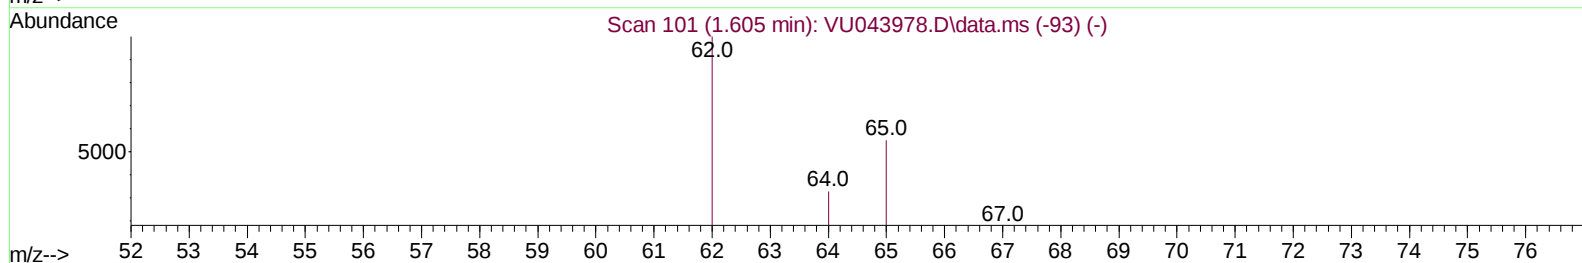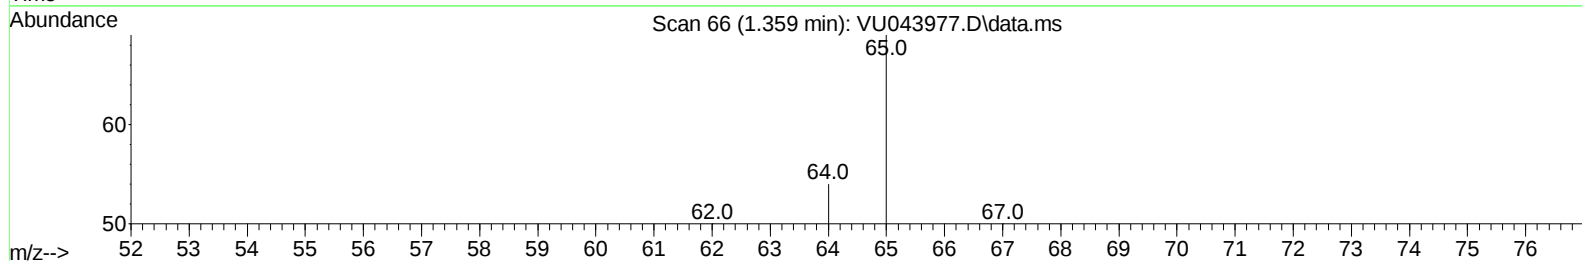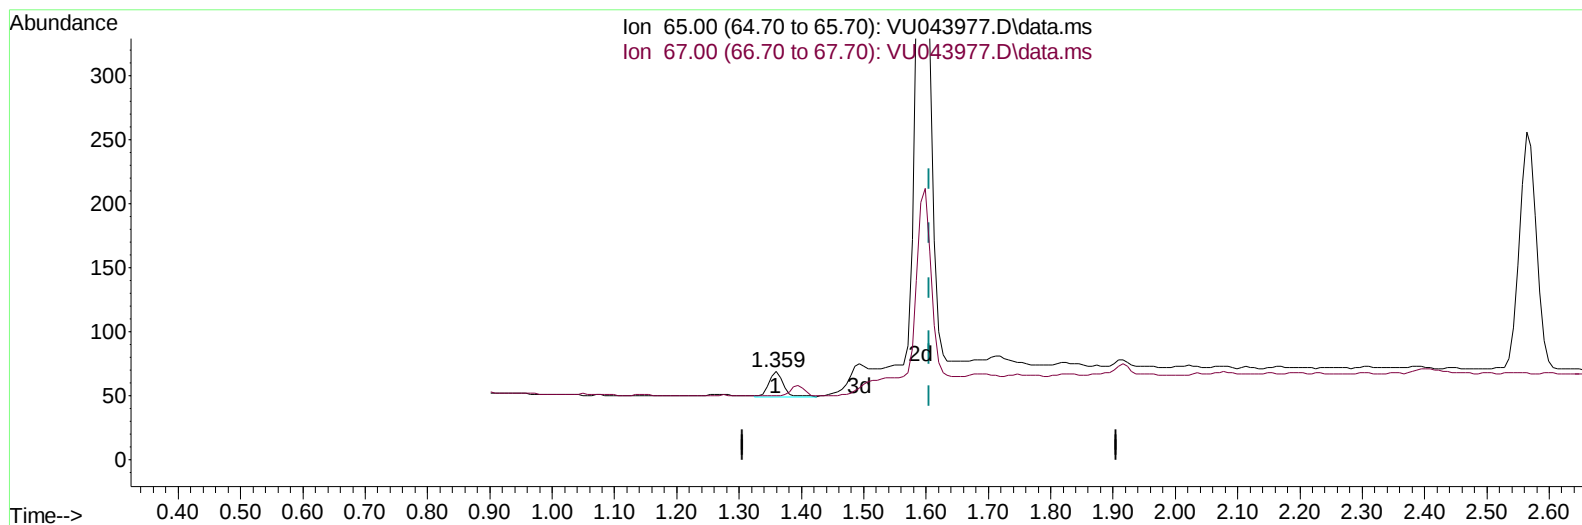

TIC: VU043977.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.359min (-0.246) 0.00 ug/L

response 32

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	34.10	37.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
 Data File : VU043977.D
 Acq On : 26 May 2021 11:44
 Operator : SY/MD
 Sample : VSTD0.131
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.1131

Manual Integrations
 APPROVED

MMDadoda
 5/28/2021 3:04:58 PM

Quant Time: May 27 01:28:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 27 01:26:40 2021
 Response via : Initial Calibration

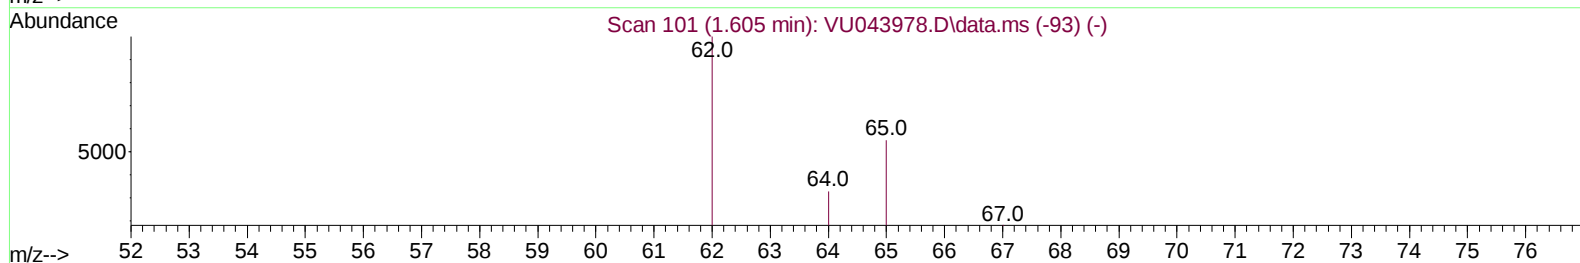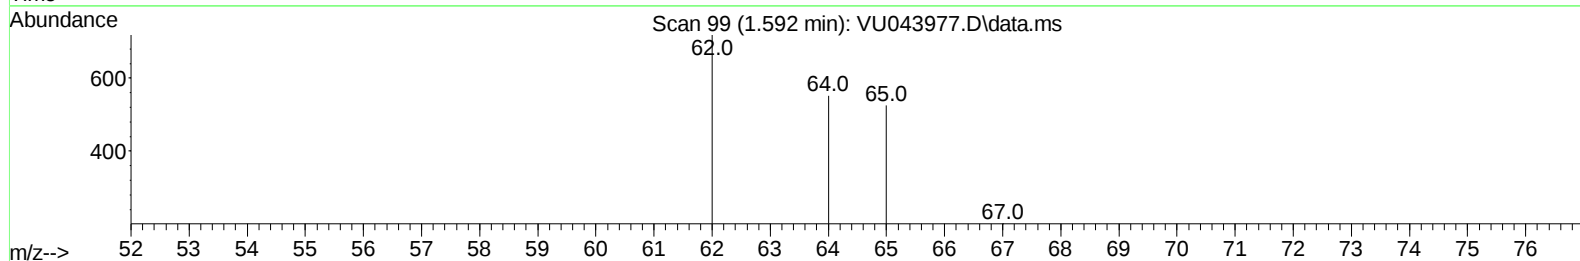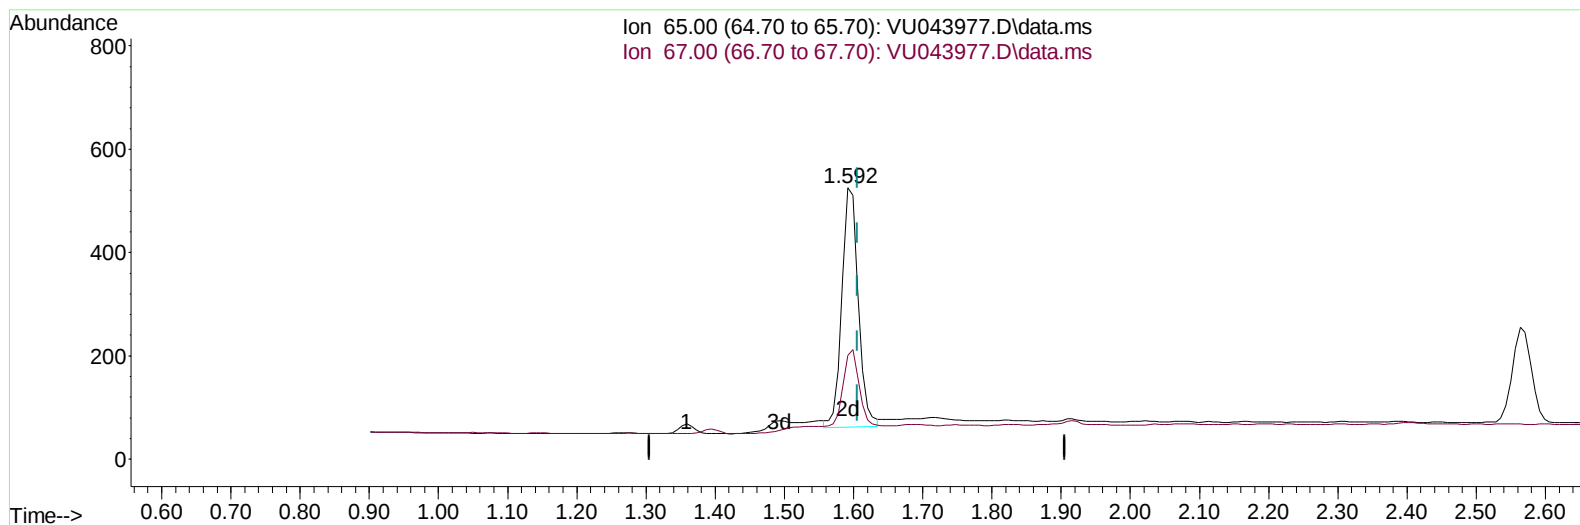

TIC: VU043977.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.592min (-0.014) 0.08 ug/L m

response 765

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	34.10	1.57#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
 Data File : VU043977.D
 Acq On : 26 May 2021 11:44
 Operator : SY/MD
 Sample : VSTD0.131
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.1131

Manual Integrations
 APPROVED

MMDadoda
 5/28/2021 3:04:58 PM

Quant Time: May 27 01:28:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 27 01:26:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	16639	0.50	ug/L	-0.02
5) Chlorobenzene-d5	9.361	117	14570	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	6625	0.50	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.592	65	765m	0.08	ug/L	-0.01
4) 1,2-Dichloroethane-d4	5.680	65	1777	0.12	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.640	67	1404	0.10	ug/L	-0.02
8) Toluene-d8	7.846	98	3102	0.11	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.679	84	1271	0.10	ug/L	-0.02
Target Compounds						Qvalue
3) Vinyl chloride	1.599	62	1272	0.07	ug/L #	28
6) Trichloroethene	6.508	95	1186	0.09	ug/L	96
9) 1,2-Dibromoethane	8.866	107	816	0.09	ug/L #	97
12) 1,2,3-Trichloropropane	10.748	75	772	0.08	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.924	75	174	0.09	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
Data File : VU043977.D
Acq On : 26 May 2021 11:44
Operator : SY/MD
Sample : VSTD0.131
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.1131

Manual Integrations
APPROVED

MMDadoda
5/28/2021 3:04:58 PM

Quant Time: May 27 01:28:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 27 01:26:40 2021
Response via : Initial Calibration

