


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052621\
Data File : VU043975.D
Acq On : 26 May 2021 10:28
Operator : SY/MD
Sample : BFB36
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB136

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
Title : TRACE VOA SOM01.0
Last Update : Thu May 27 01:35:45 2021

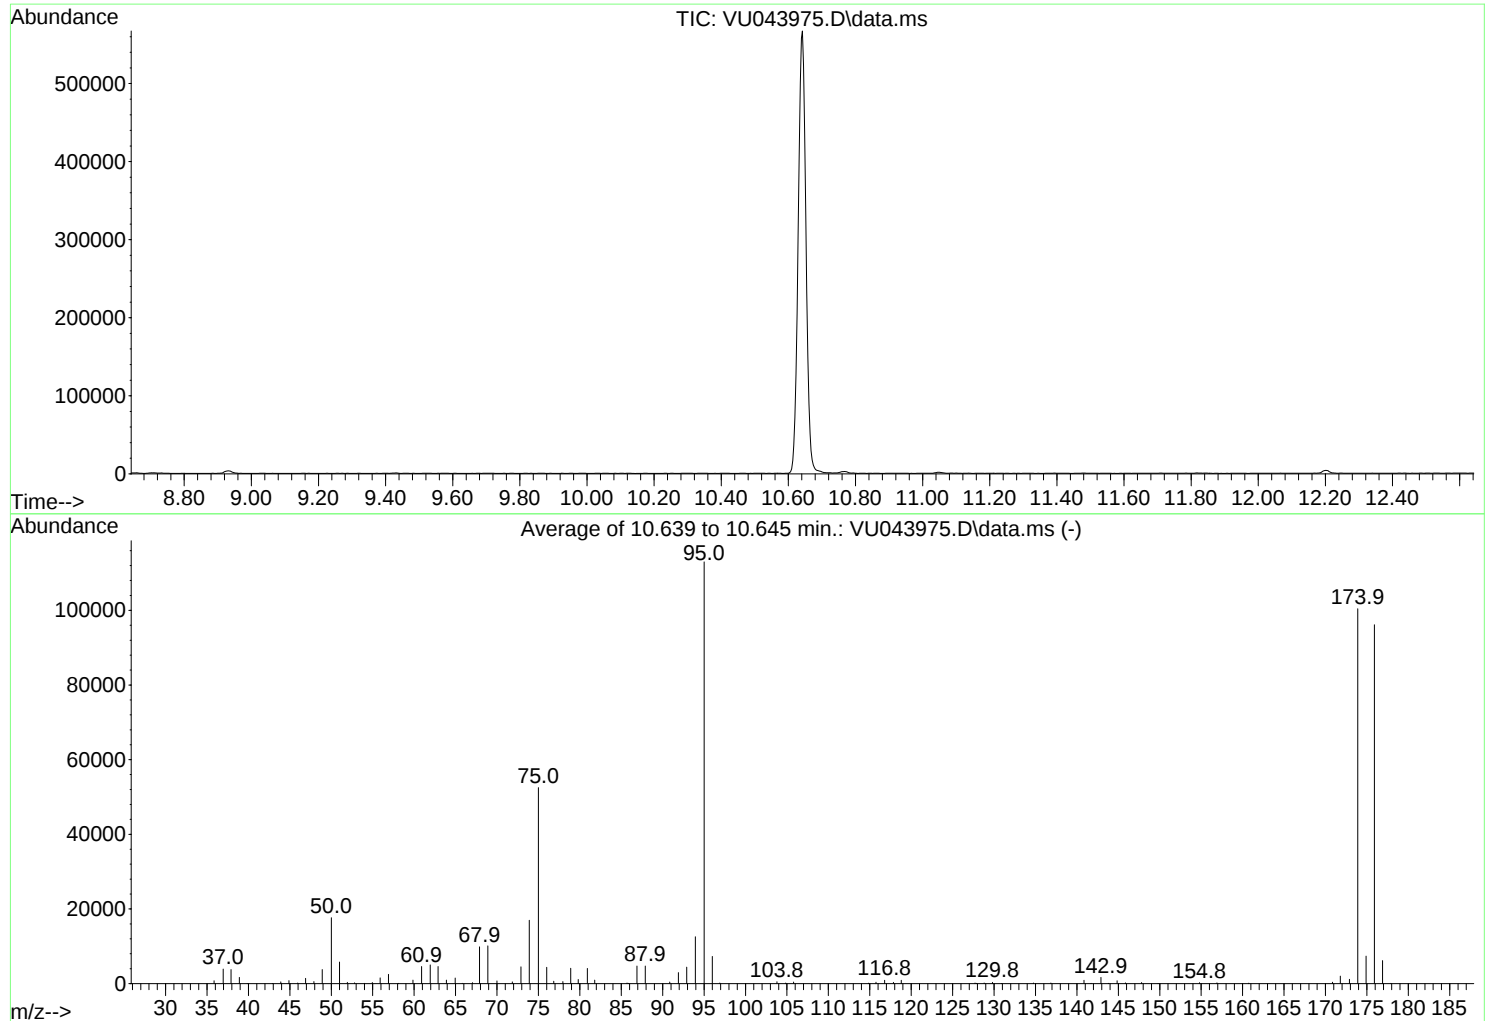

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	17664	PASS
75	95	30	80	46.5	52488	PASS
95	95	100	100	100.0	112992	PASS
96	95	5	9	6.5	7311	PASS
173	174	0.00	2	1.2	1183	PASS
174	95	50	120	88.9	100437	PASS
175	174	5	9	7.3	7374	PASS
176	174	95	101	95.7	96155	PASS
177	176	5	9	6.4	6183	PASS

m/z	Abundance
35.80	748.0
37.00	3919.0
37.90	3863.0
38.90	1712.0
39.90	219.0
43.90	1165.0
44.90	818.0
45.90	172.0
46.90	1422.0
47.90	572.0
48.90	3829.0
50.00	18272.0
51.00	5962.0
51.90	377.0
52.80	214.0
54.00	143.0
54.90	263.0
55.90	1542.0
56.90	2685.0
58.10	124.0
59.90	1026.0
60.90	4550.0
61.90	5126.0
62.90	4636.0
63.90	970.0
65.00	1480.0
65.80	139.0
67.00	226.0
67.90	10160.0
68.90	10616.0
70.00	790.0
71.80	493.0
72.90	4516.0
73.90	17408.0
75.00	53816.0
76.00	4459.0
76.90	625.0
78.00	531.0
78.90	4304.0
79.80	1170.0
80.90	4059.0
81.80	862.0
85.70	228.0
86.90	4921.0
87.90	4983.0
90.80	367.0
91.90	2903.0
92.90	4644.0
93.90	13021.0
95.00	115376.0
96.00	7644.0
96.90	181.0
103.80	569.0
104.90	154.0
105.80	495.0
114.80	130.0
115.80	344.0
116.80	903.0
117.80	393.0
118.80	824.0
127.70	290.0
128.80	151.0
129.80	344.0
130.90	131.0
134.70	169.0
136.90	172.0
140.80	1007.0
141.70	109.0
142.90	1682.0
143.80	178.0
144.90	812.0
145.80	205.0
147.80	334.0
149.80	110.0
154.80	252.0
156.90	225.0
160.80	133.0
170.90	378.0
171.80	2104.0
172.90	1227.0
173.90	100528.0
174.90	7537.0
175.90	95408.0
176.90	6359.0
177.90	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
39.80	182.0
43.90	668.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	742.0
36.90	3839.0
37.90	3568.0
38.90	1591.0
40.00	211.0
42.90	109.0
43.90	1123.0
44.90	808.0
46.00	168.0
46.90	1343.0
47.90	522.0
48.90	3573.0
50.00	16488.0
51.00	5461.0
52.00	273.0
52.80	184.0
55.00	278.0
55.90	1460.0
56.90	2200.0
59.80	862.0
60.90	4458.0
62.00	4742.0
62.90	4369.0
63.90	928.0
64.90	1467.0
67.10	270.0
67.90	9302.0
68.90	9229.0
70.00	630.0
71.90	443.0
72.90	4381.0
73.90	15923.0
75.00	49432.0
76.00	4129.0
76.80	620.0
77.90	536.0
78.90	3841.0
79.80	1058.0
80.90	3956.0
81.80	960.0
85.90	260.0
86.90	4374.0
87.90	4279.0
90.90	445.0
91.90	2936.0
92.90	4035.0
94.00	11724.0
95.00	107048.0
96.00	6732.0
96.90	131.0
103.80	446.0
104.80	180.0
105.80	381.0
114.90	127.0
115.70	397.0
116.80	859.0
117.90	335.0
118.80	899.0
127.90	248.0
128.80	178.0
129.80	374.0
134.80	168.0
136.70	152.0
140.90	800.0
141.70	105.0
142.90	1597.0
144.80	753.0
145.90	187.0
147.80	281.0
154.80	285.0
156.90	165.0
160.70	108.0
170.80	381.0
171.80	1915.0
172.90	1147.0
173.90	97016.0
174.90	7001.0
175.90	93872.0
176.90	5829.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.80	782.0
36.90	3935.0
37.90	3888.0
38.90	1687.0
40.00	202.0
43.90	1154.0
44.90	869.0
45.90	180.0
46.90	1444.0
47.90	587.0
48.90	3896.0
50.00	18232.0
51.00	6007.0
52.00	346.0
52.80	208.0
54.00	119.0
55.00	300.0
55.90	1585.0
56.90	2528.0
58.10	117.0
59.90	1000.0
60.90	4712.0
61.90	5229.0
62.90	4737.0
63.90	990.0
64.90	1593.0
65.80	127.0
67.00	251.0
67.90	10148.0
68.90	10445.0
70.00	727.0
71.80	474.0
72.90	4648.0
73.90	17568.0
75.00	54216.0
76.00	4484.0
76.90	663.0
77.90	566.0
78.90	4266.0
79.80	1182.0
80.90	4166.0
81.80	962.0
85.70	237.0
86.90	4894.0
87.90	4938.0
90.90	443.0
91.90	3036.0
92.90	4510.0
94.00	12991.0
95.00	116552.0
96.00	7558.0
96.90	163.0
103.80	557.0
104.80	168.0
105.80	448.0
114.80	138.0
115.70	388.0
116.80	918.0
117.80	356.0
118.80	949.0
127.70	268.0
128.80	169.0
129.80	380.0
134.70	179.0
136.90	183.0
140.90	937.0
141.70	102.0
142.90	1727.0
143.80	147.0
144.80	799.0
145.90	208.0
147.80	340.0
154.80	291.0
156.90	213.0
160.80	138.0
170.90	431.0
171.80	2081.0
172.90	1175.0
173.90	103768.0
174.90	7585.0
175.90	99184.0
176.90	6361.0
177.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136