


Bromomethane

Response Ratio

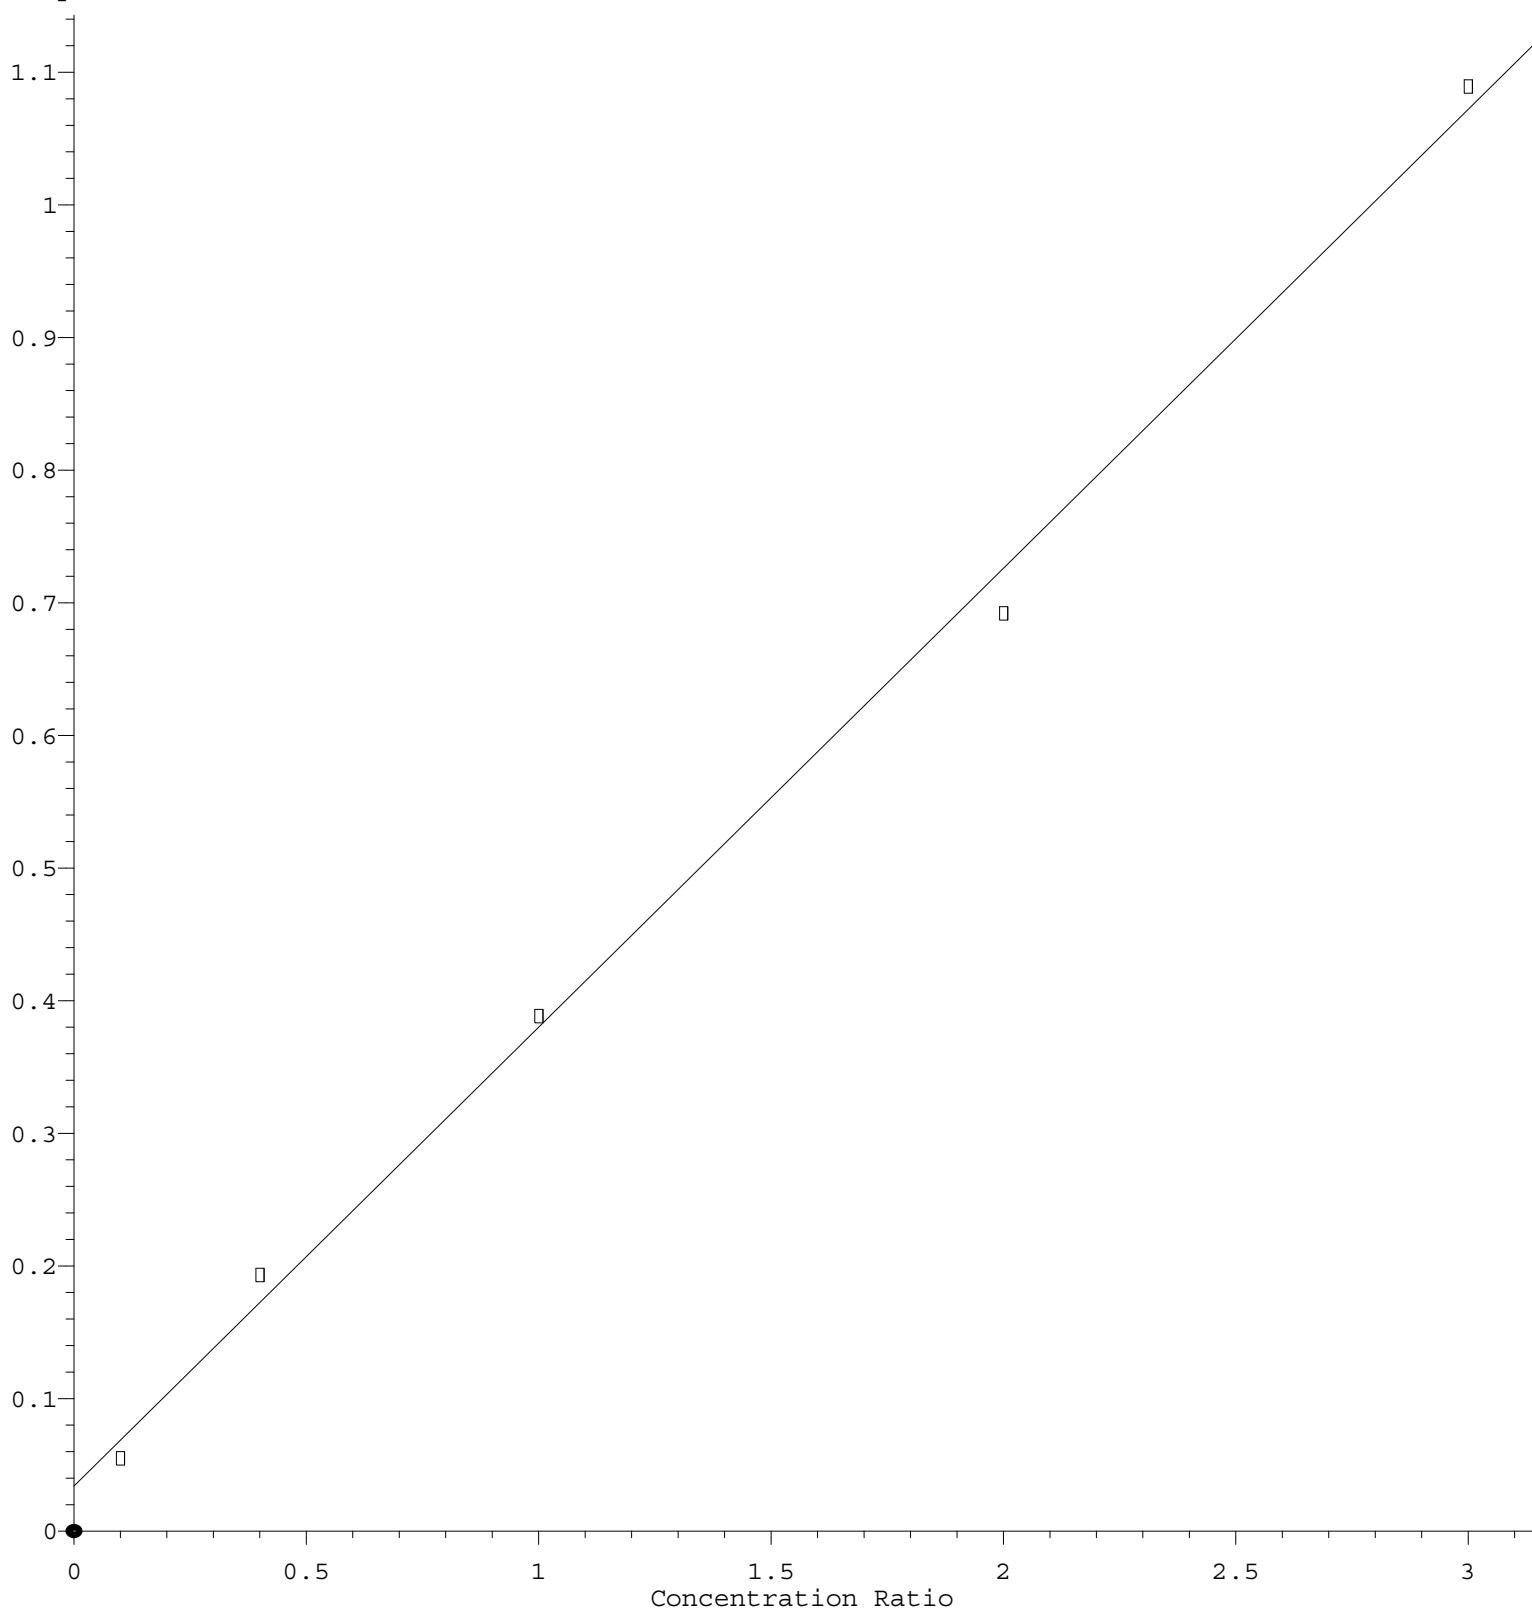

$$\text{Response} = 3.461\text{e-}001 * \text{Amt} + 3.354\text{e-}002$$


Coef of Det (r^2) = 0.996877 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

Chloroethane


Response Ratio

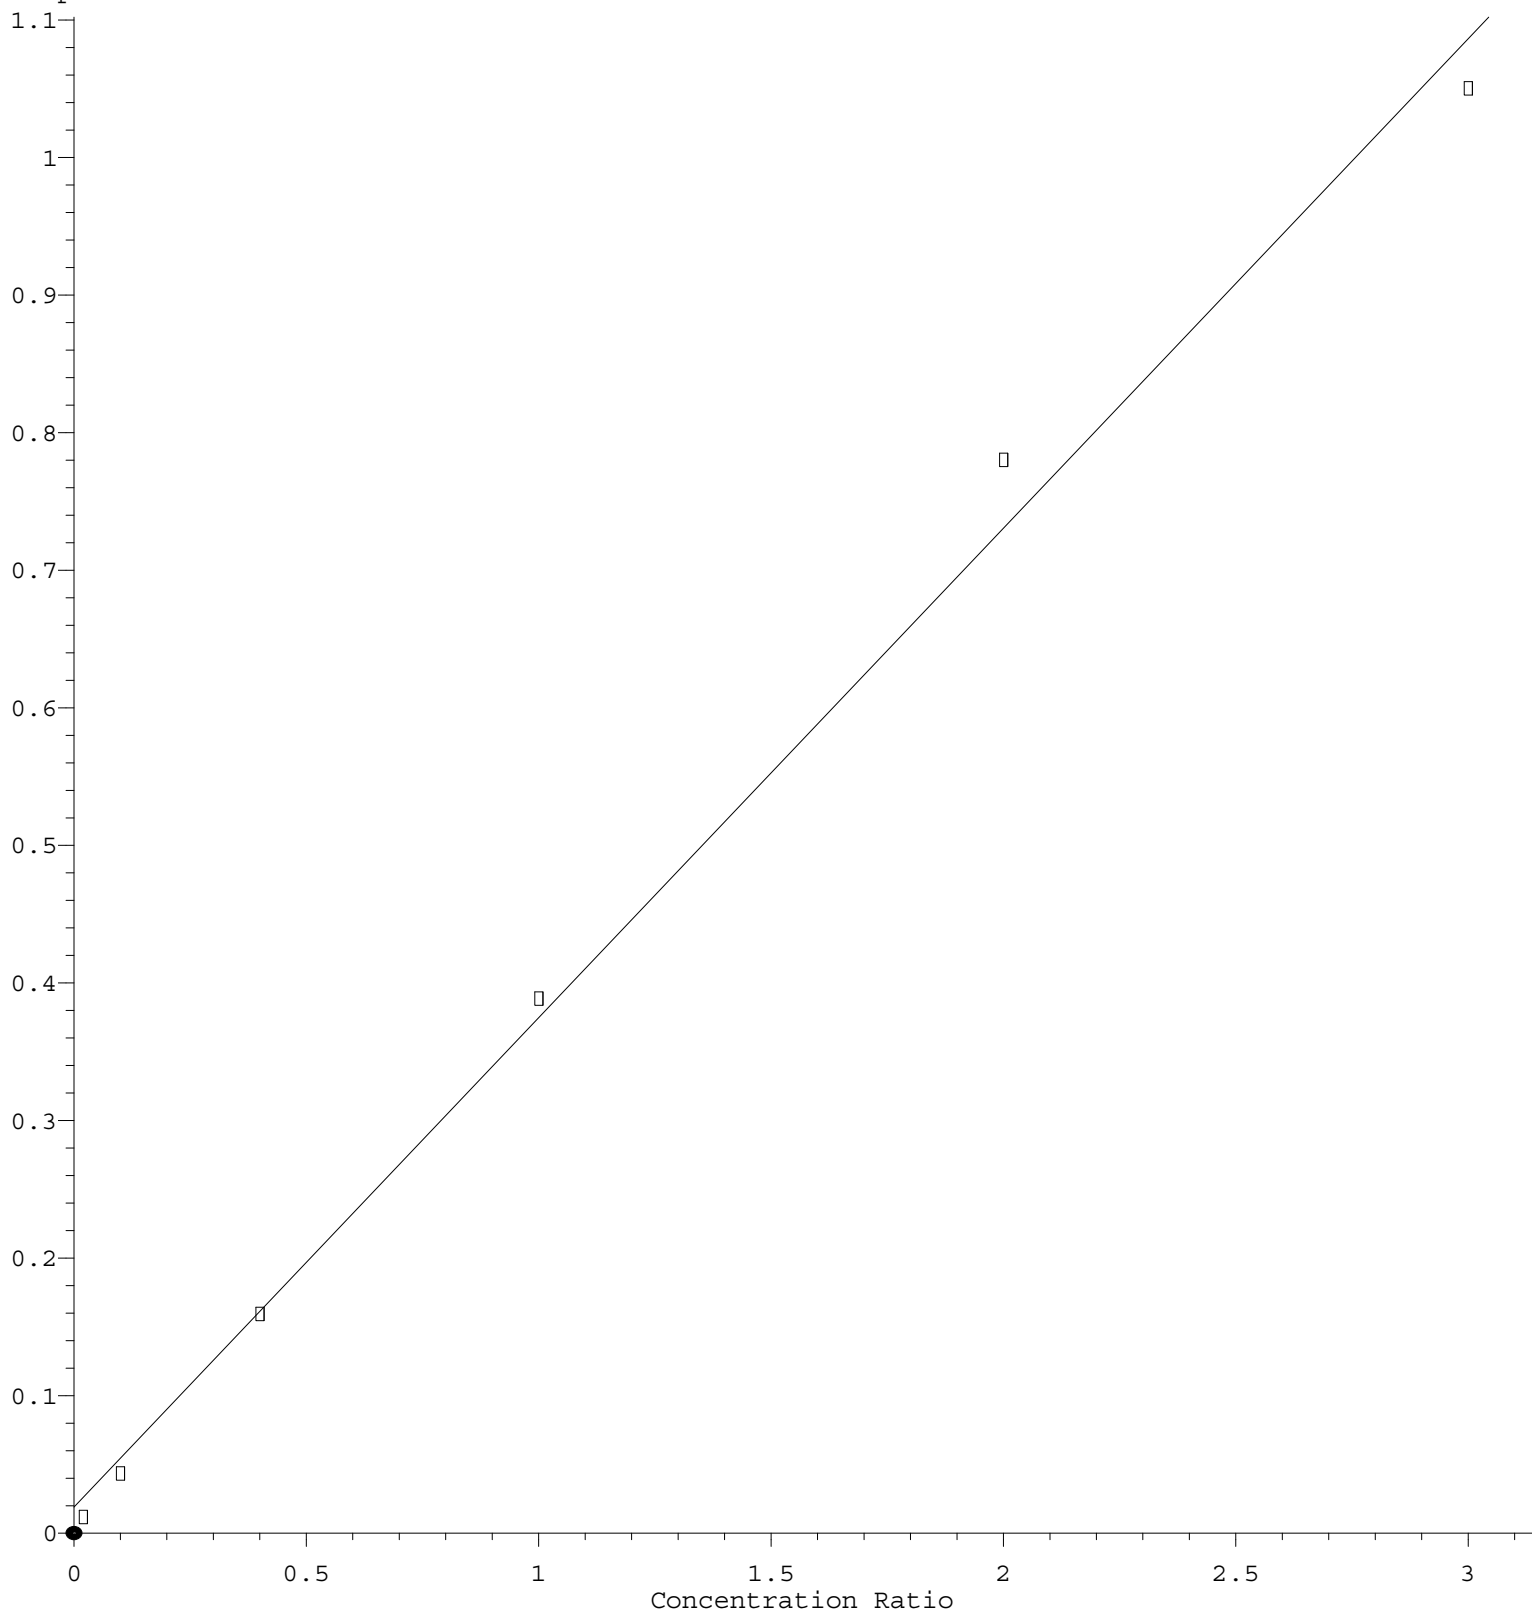

Response = 3.562e-001 * Amt + 1.857e-002
Coef of Det (r^2) = 0.995249 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M
Calibration Table Last Updated: Fri May 27 06:42:31 2022

Methyl Iodide

Response Ratio

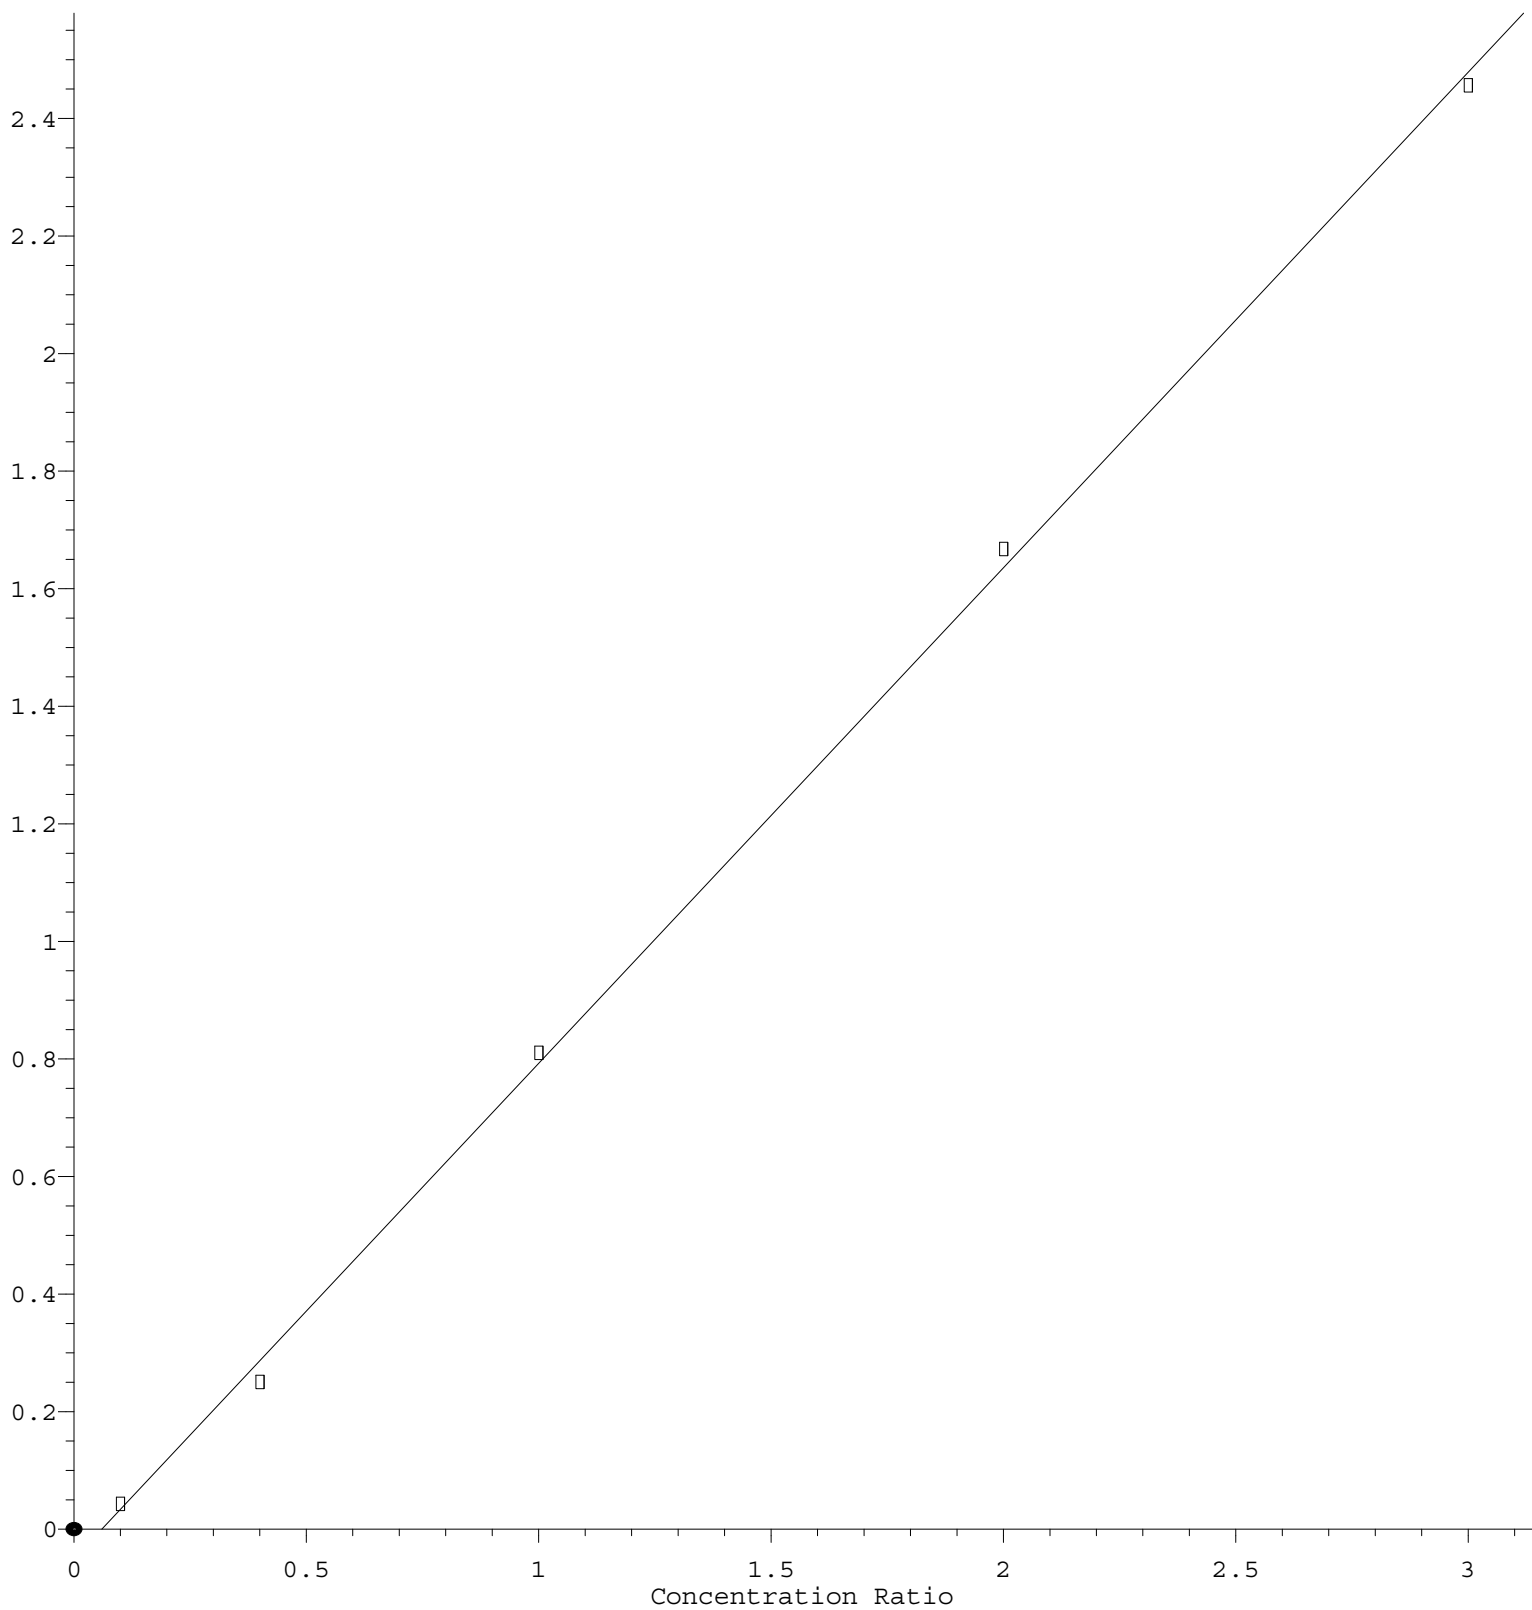

$$\text{Response} = 8.432\text{e-}001 * \text{Amt} - 5.067\text{e-}002$$


Coef of Det (r^2) = 0.999209 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

Acrolein

Response Ratio

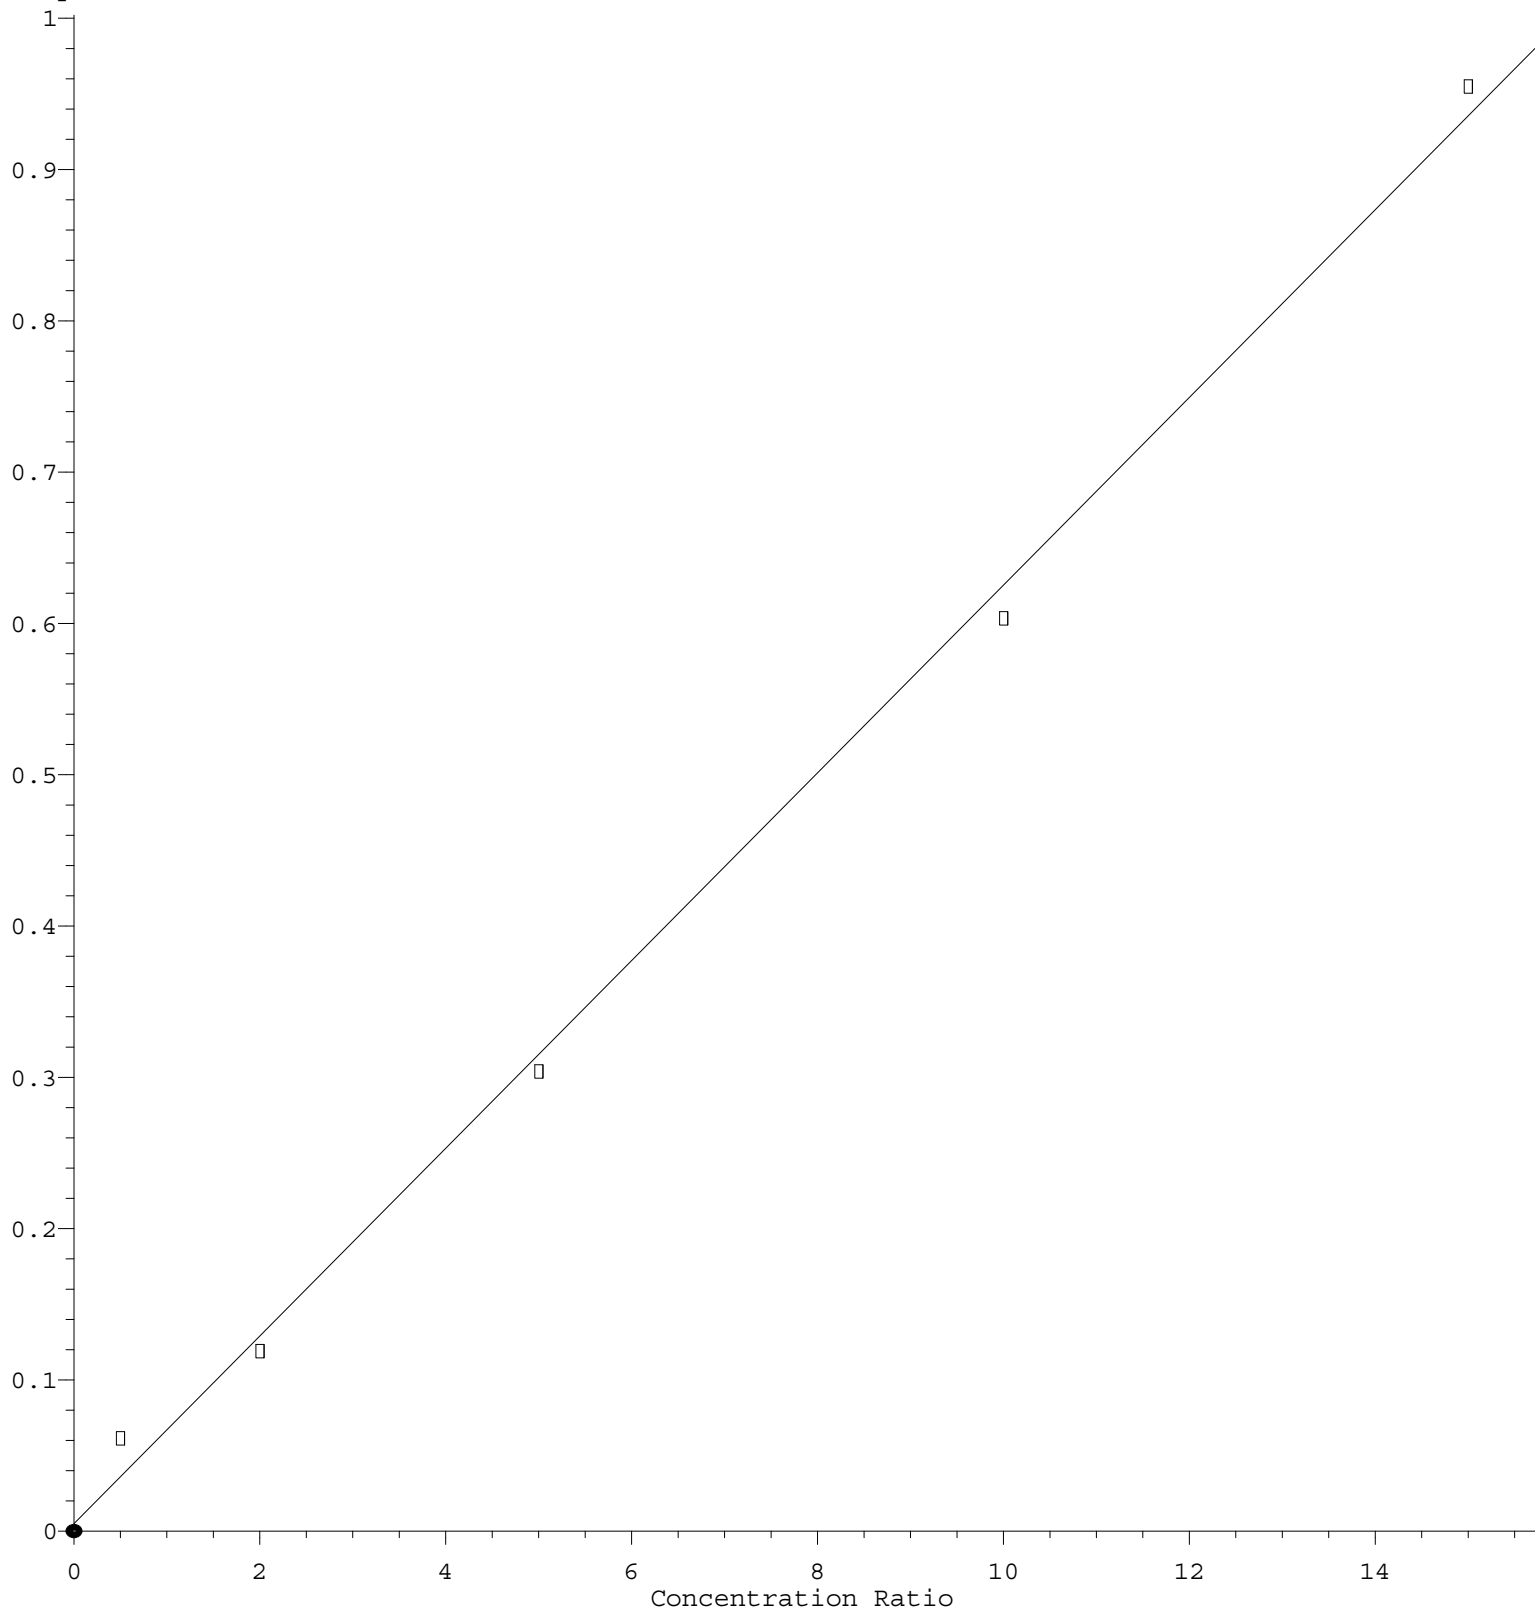

$$\text{Response} = 6.202\text{e-}002 * \text{Amt} + 5.362\text{e-}003$$


Coef of Det (r^2) = 0.996864 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

Ethyl methacrylate


Response Ratio

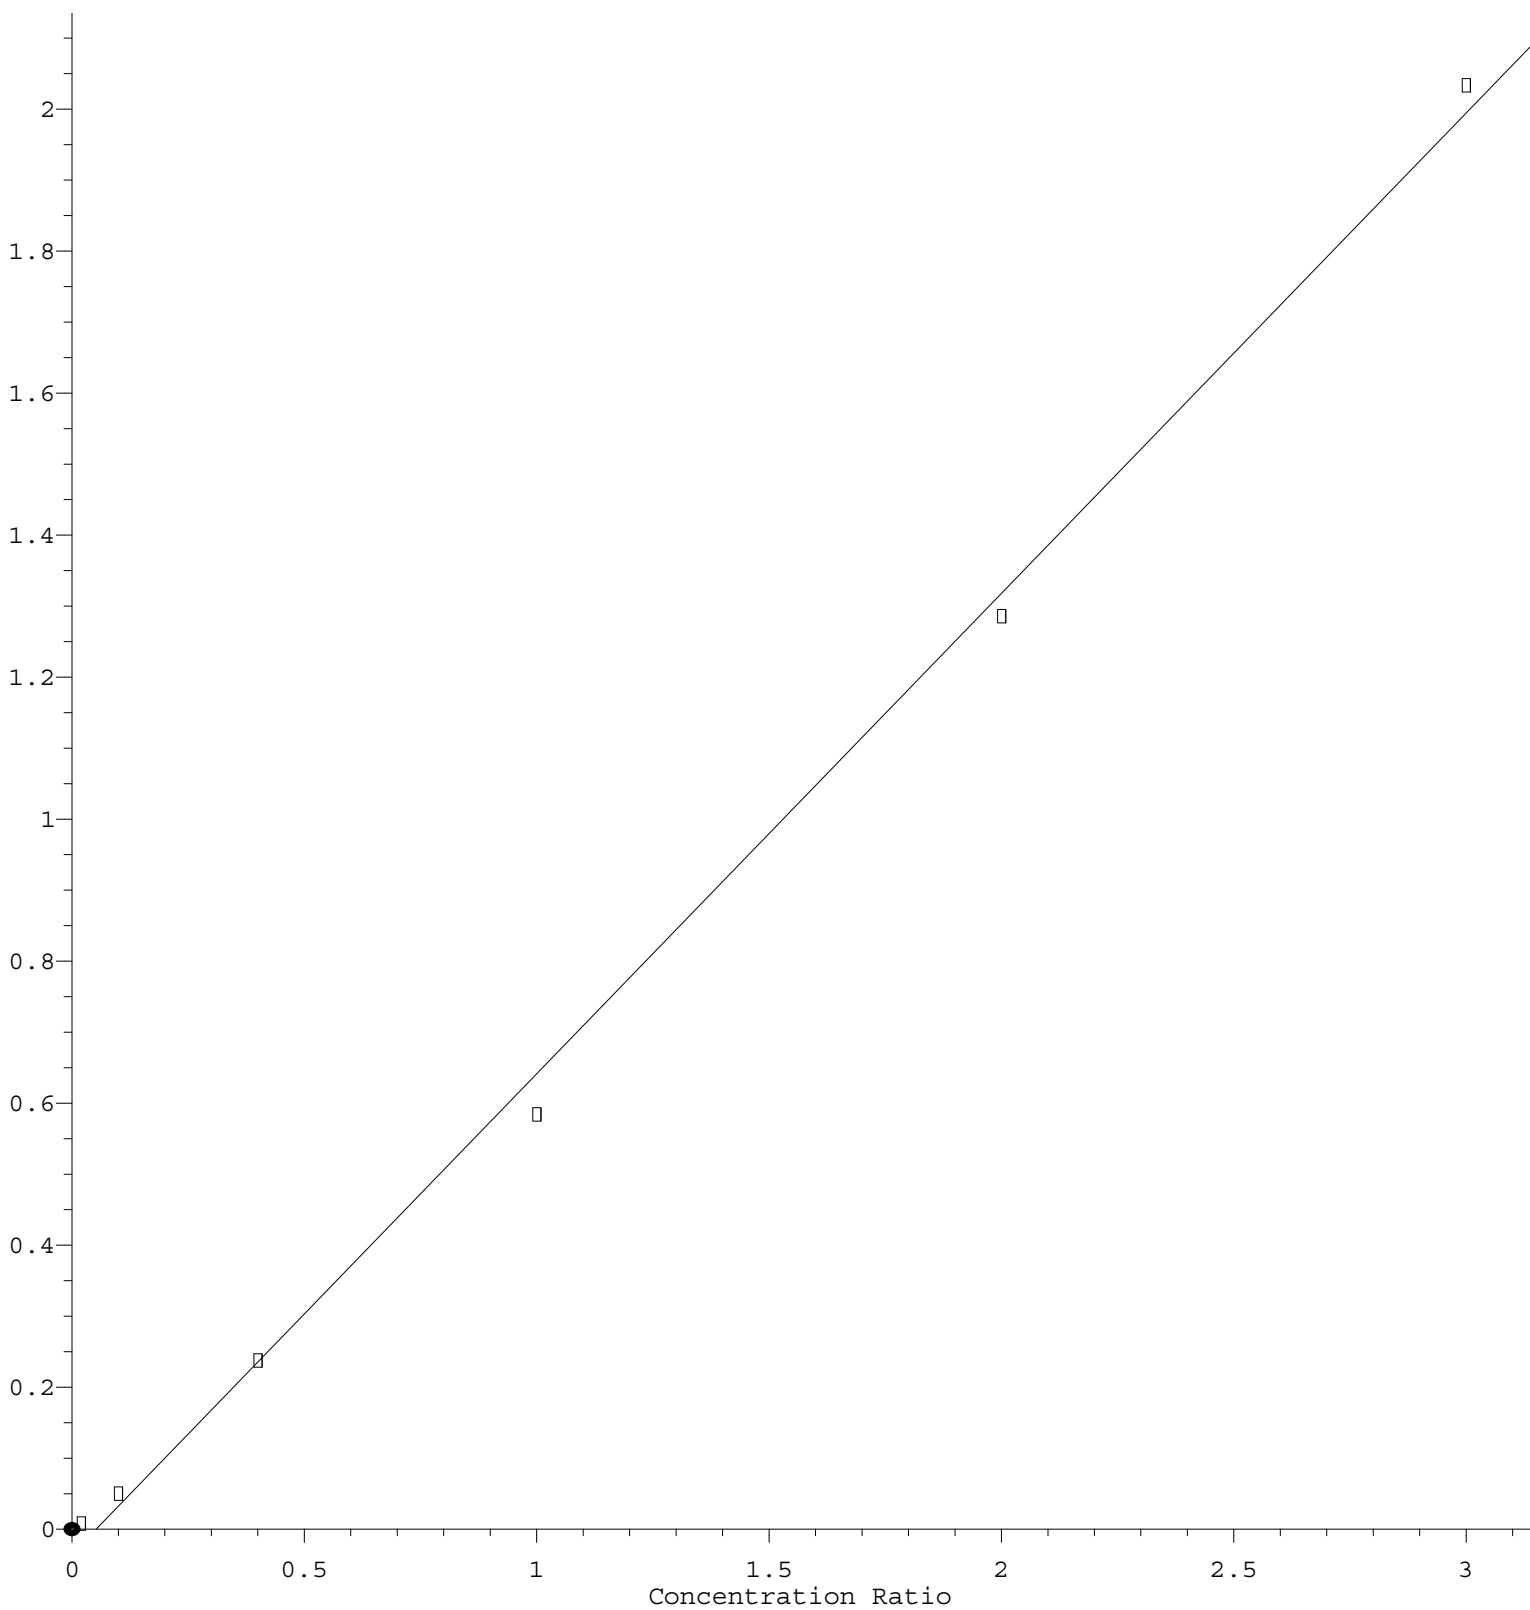

Response = 6.765e-001 * Amt - 3.536e-002
 Coef of Det (r^2) = 0.997839 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M
 Calibration Table Last Updated: Fri May 27 06:42:31 2022

2-Chloroethyl Vinyl ether

Response Ratio

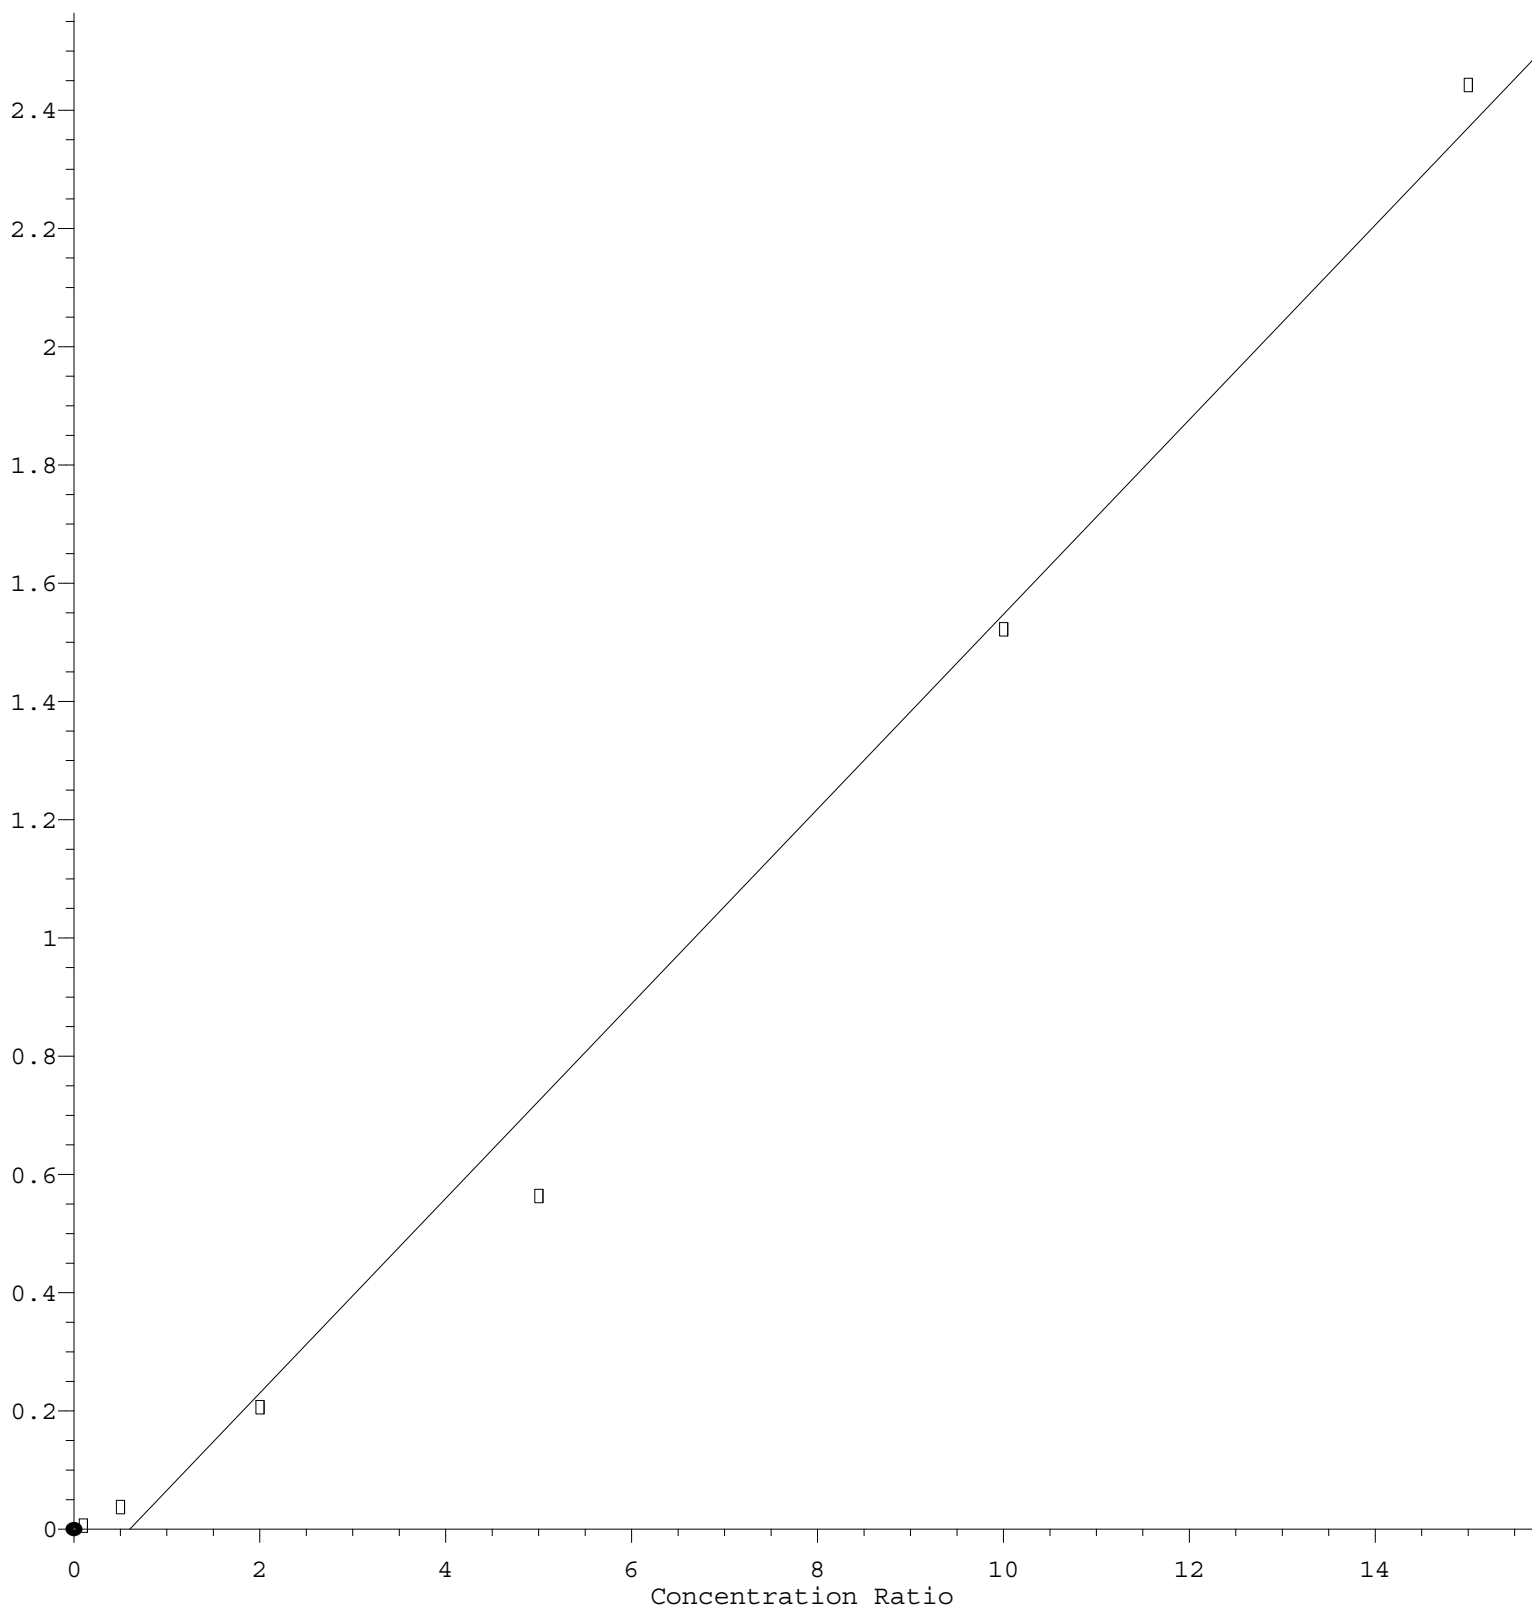

$$\text{Response} = 1.646\text{e-}001 * \text{Amt} - 9.794\text{e-}002$$


Coef of Det (r^2) = 0.991102 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

Tetrachloroethene

Response Ratio

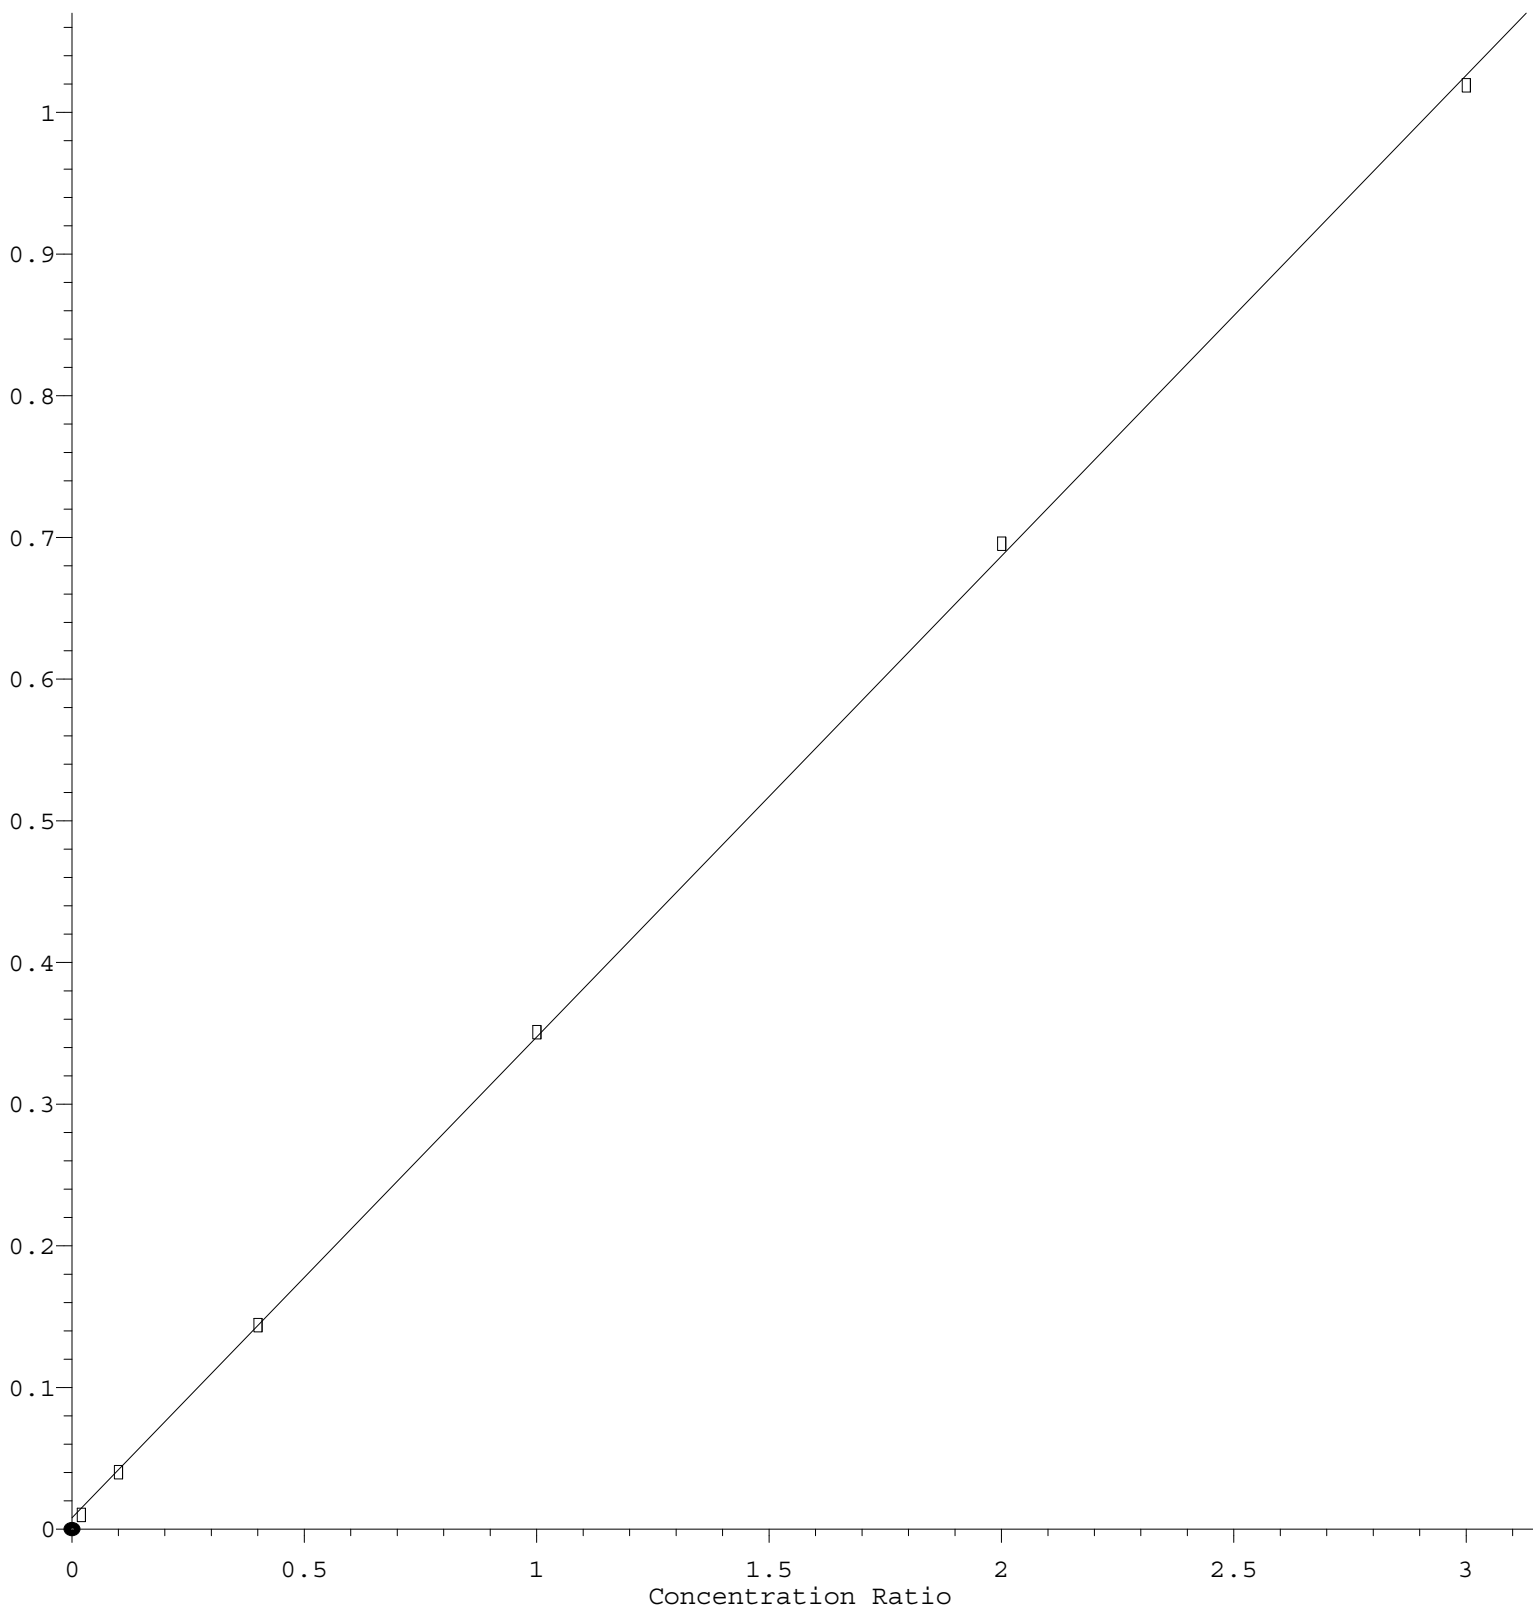

$$\text{Response} = 3.395\text{e-}001 * \text{Amt} + 7.698\text{e-}003$$


Coef of Det (r^2) = 0.999800 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

N-amyl acetate


Response Ratio

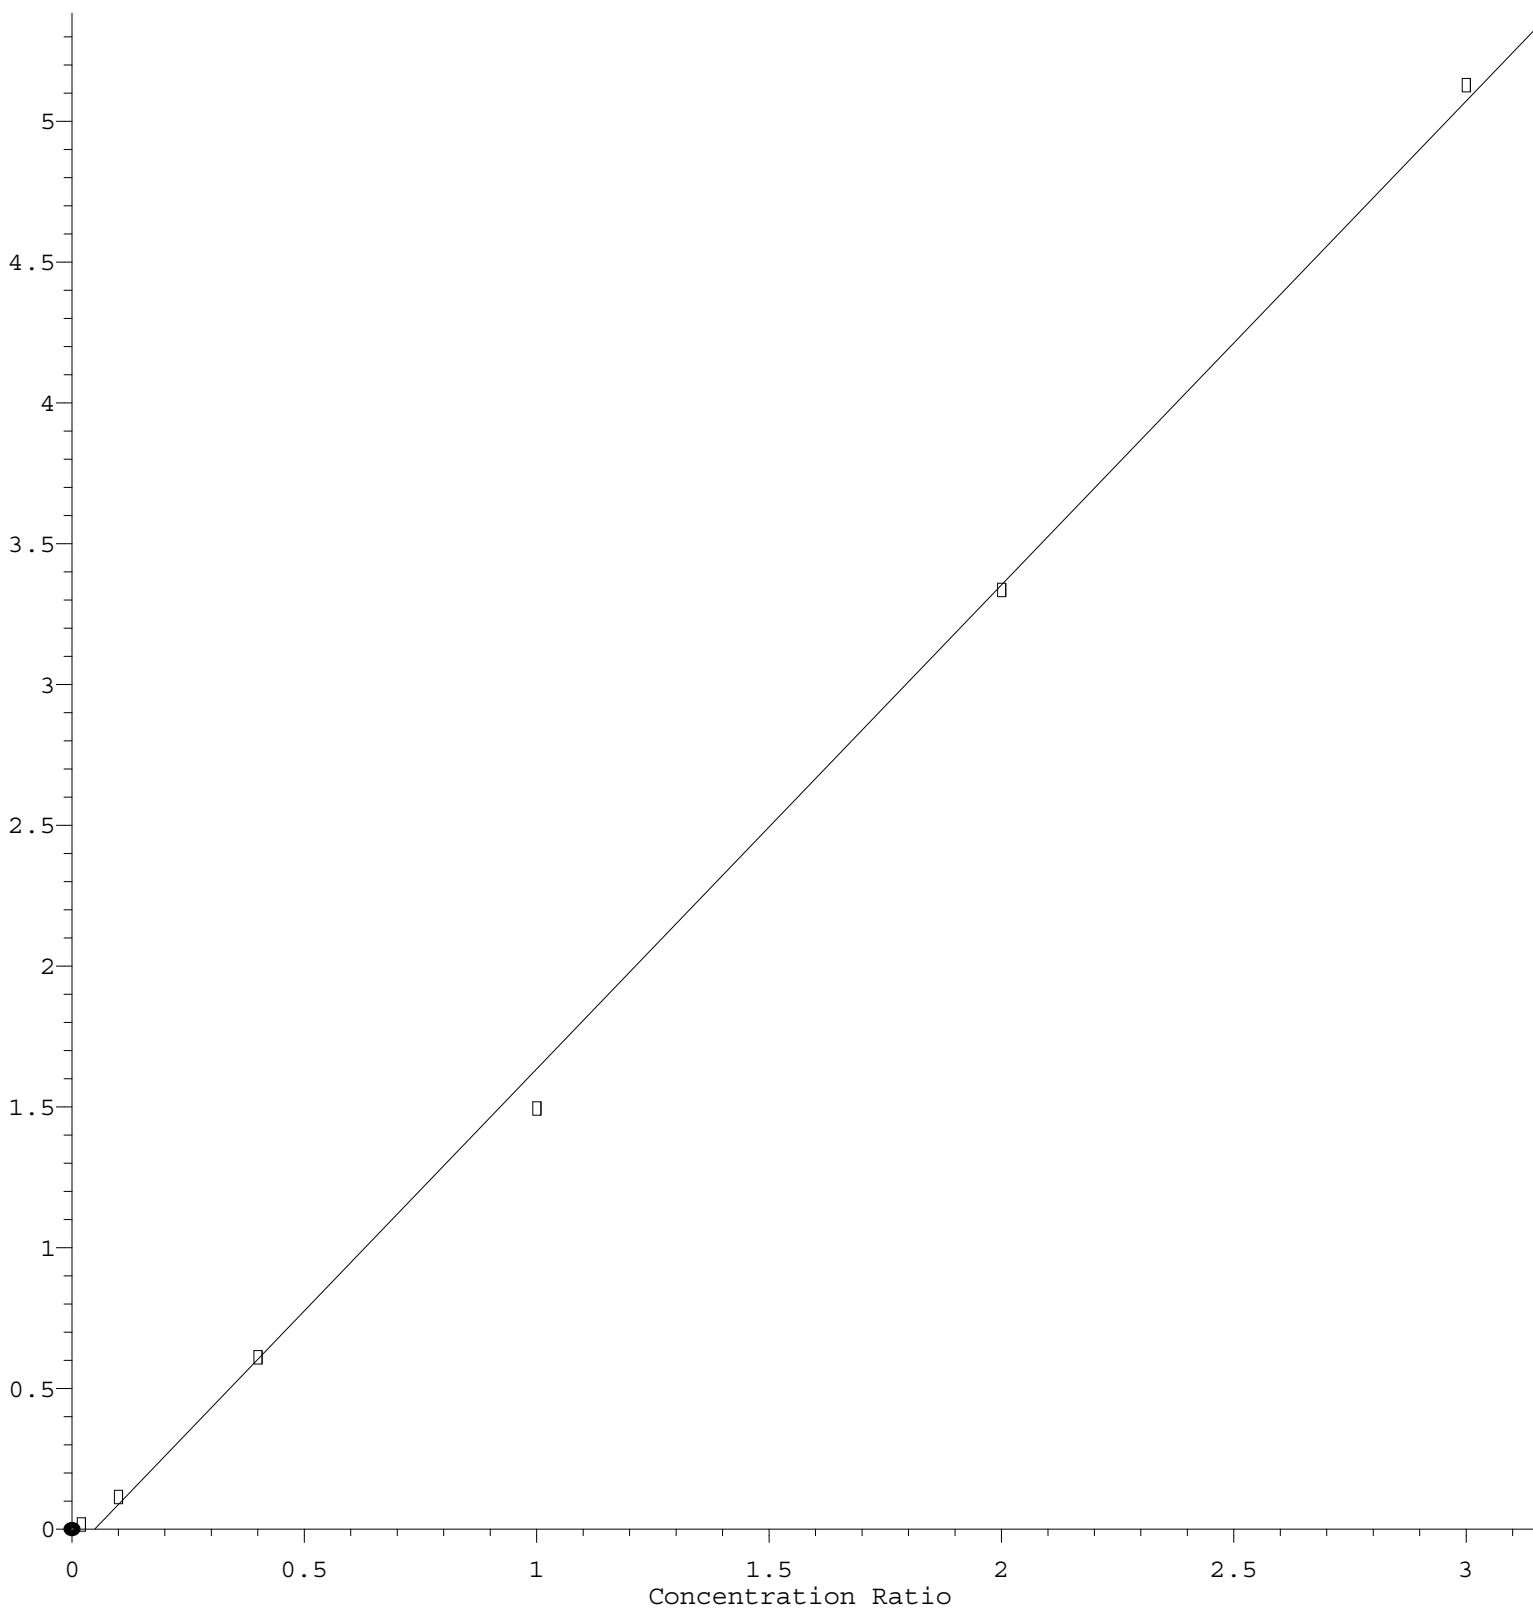

$\text{Response} = 1.719\text{e}+000 * \text{Amt} - 8.481\text{e}-002$
 Coef of Det (r^2) = 0.998642 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M
 Calibration Table Last Updated: Fri May 27 06:42:31 2022

1,2,4-Trimethylbenzene

Response Ratio

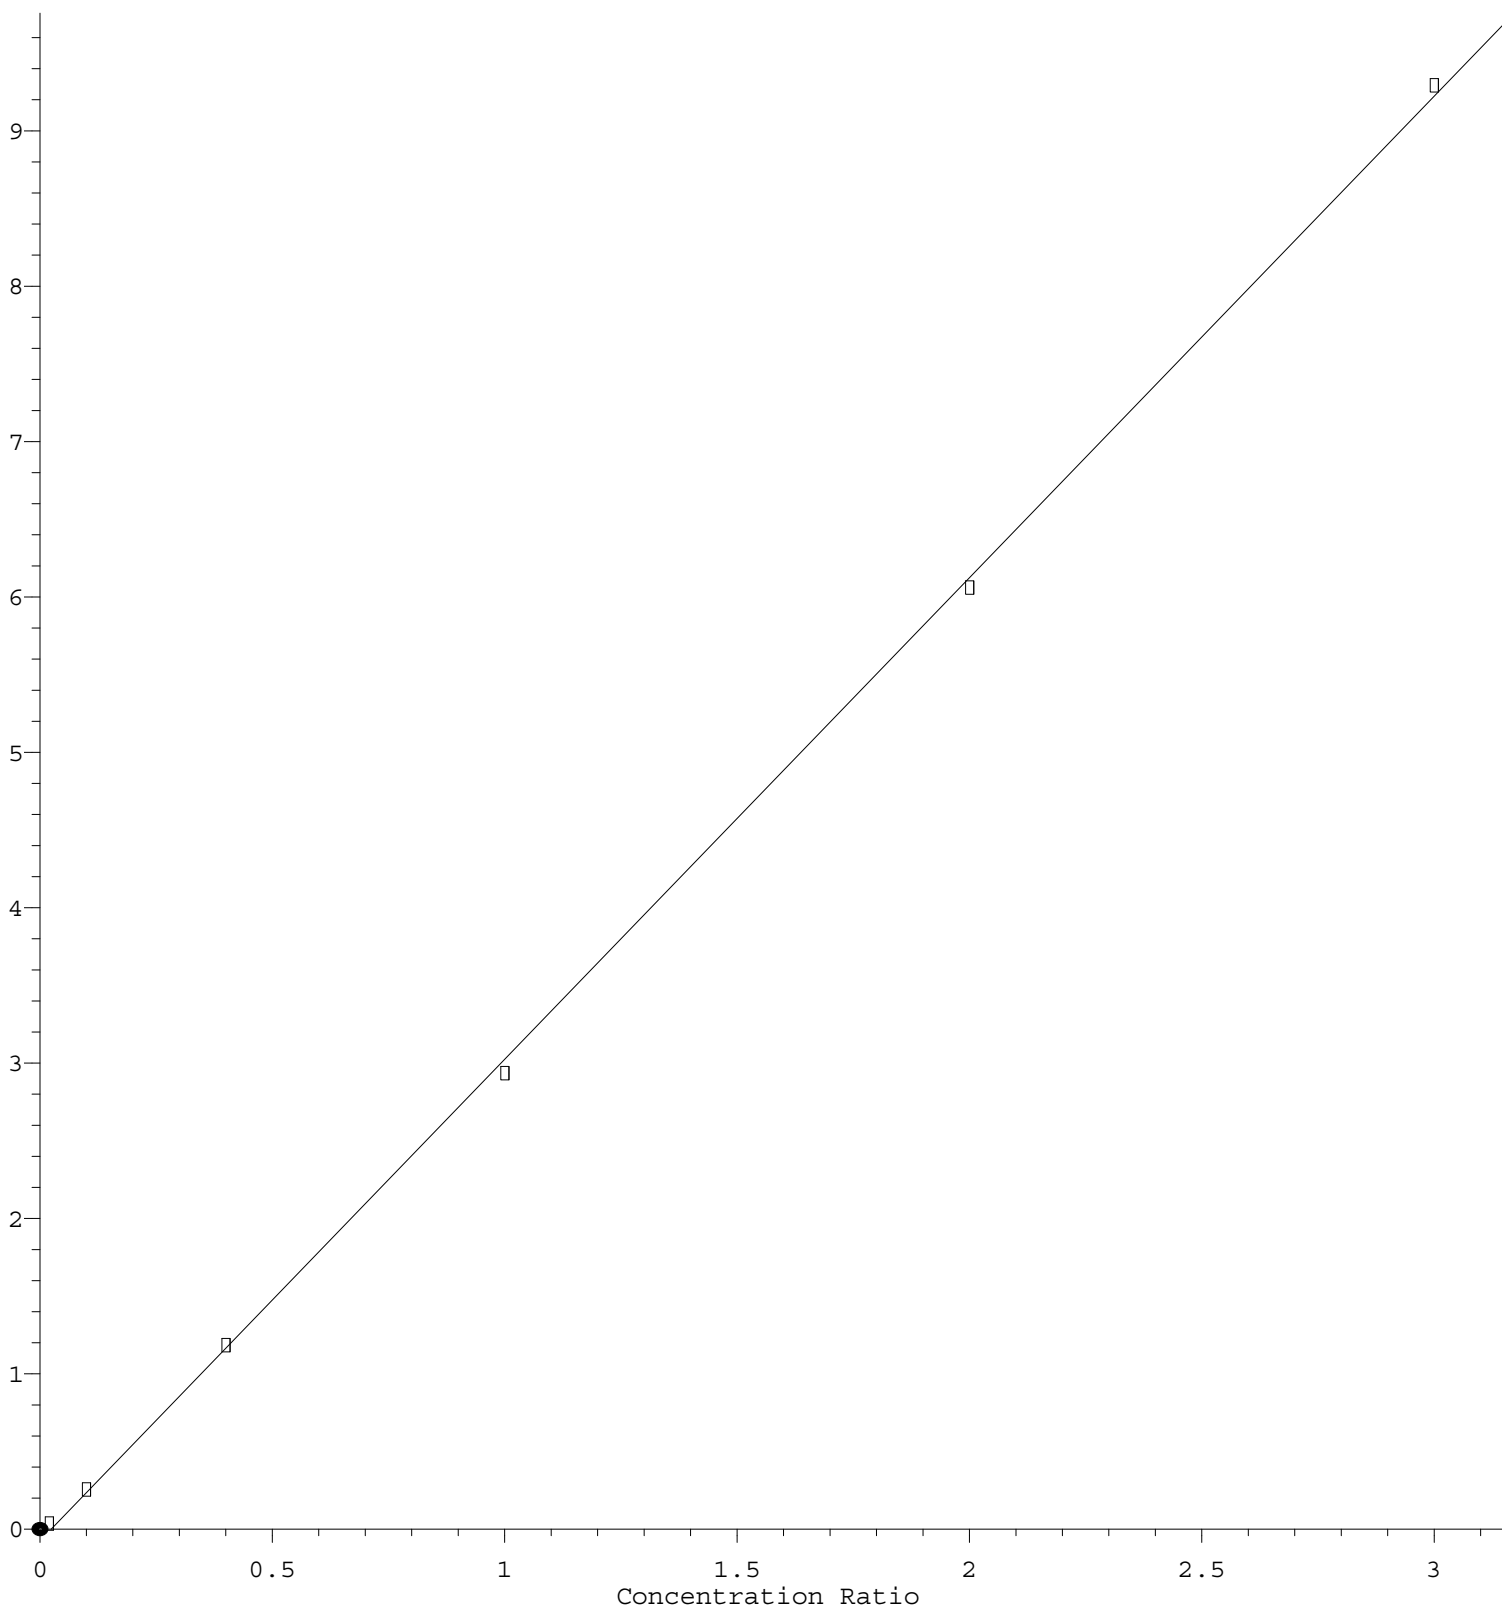

$$\text{Response} = 3.099\text{e}+000 * \text{Amt} - 7.356\text{e}-002$$


Coef of Det (r^2) = 0.999704 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

n-Butylbenzene

Response Ratio

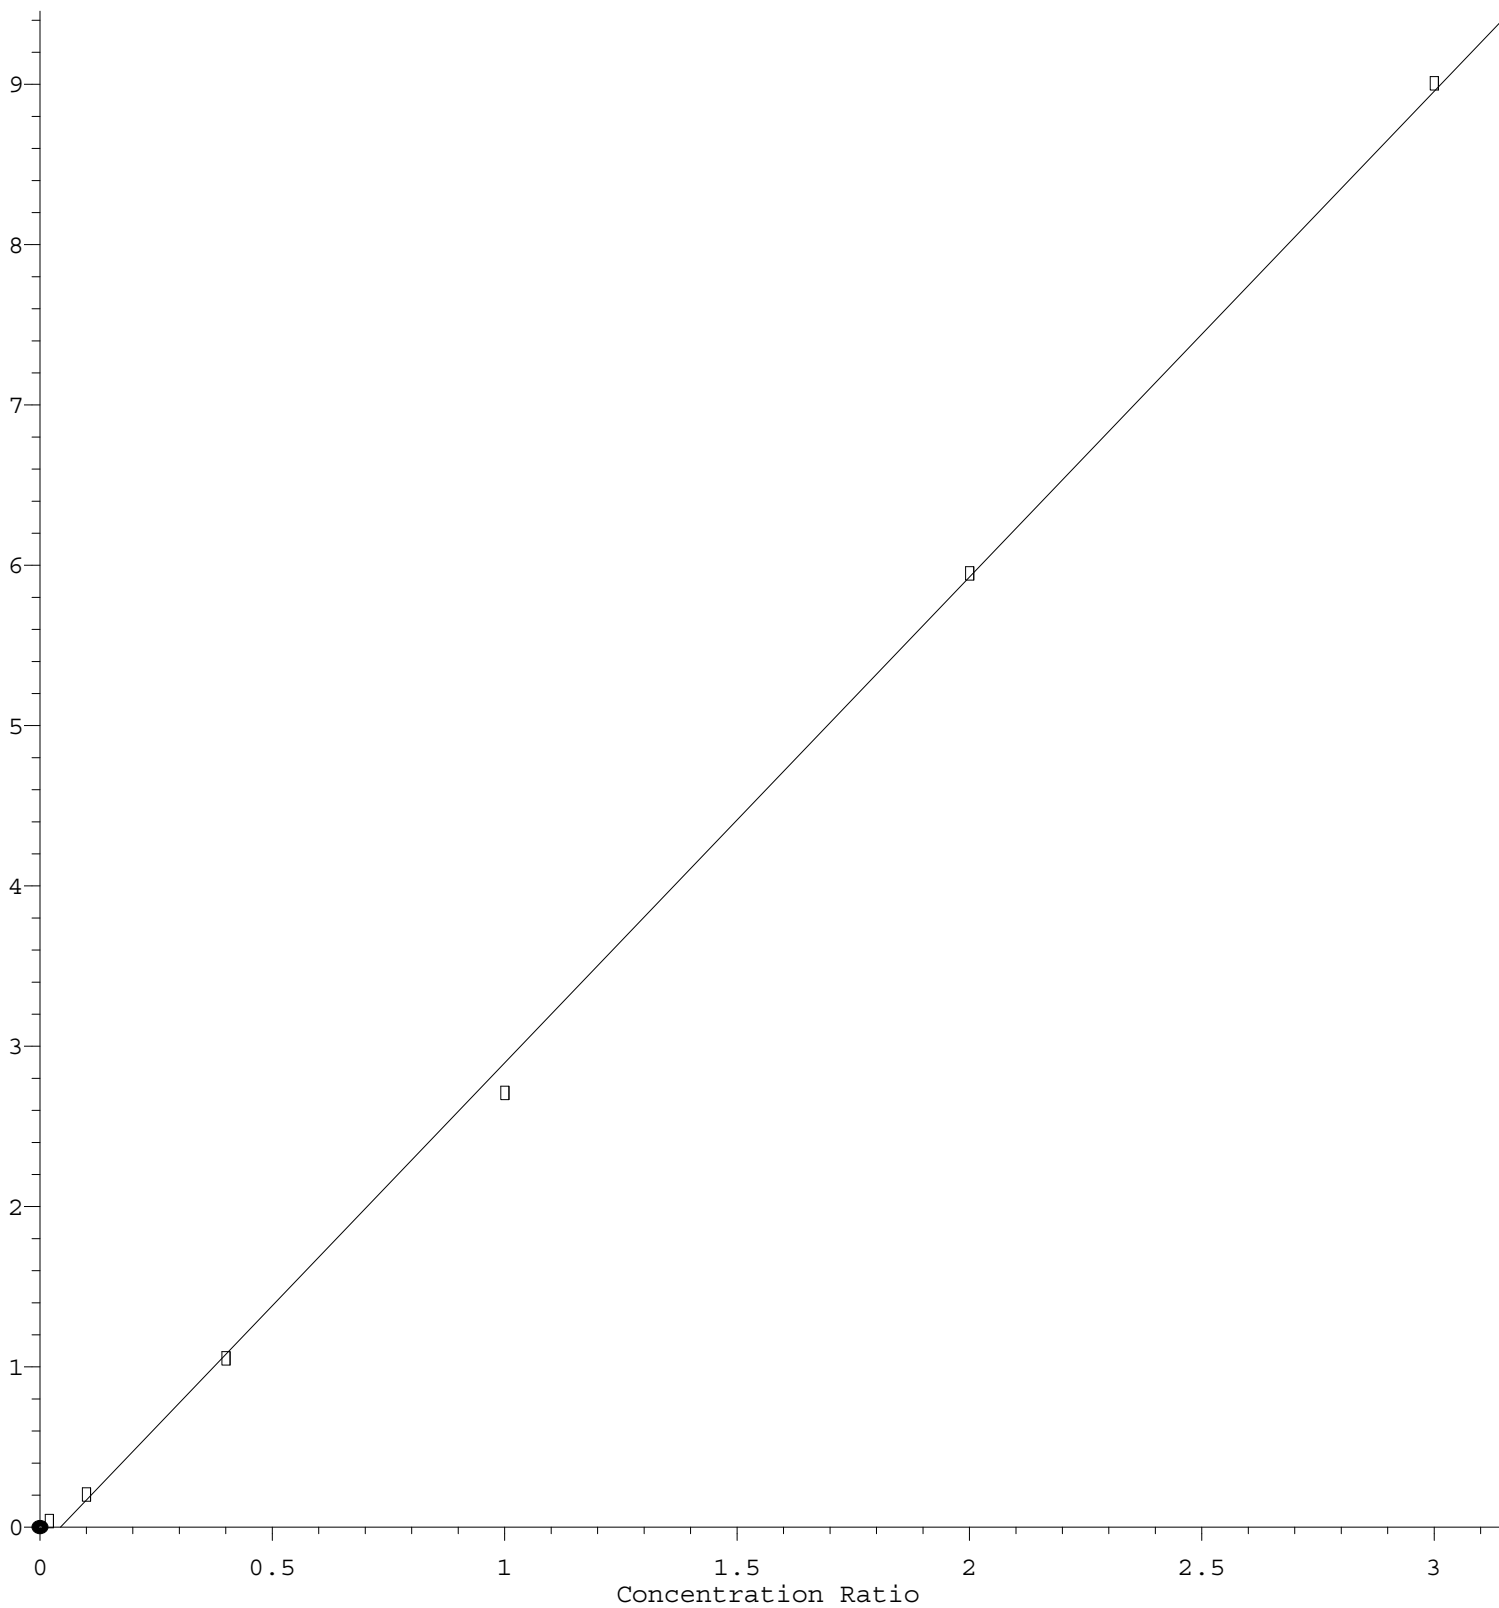

$$\text{Response} = 3.030\text{e}+000 * \text{Amt} - 1.324\text{e}-001$$


Coef of Det (r^2) = 0.999194 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022

Naphthalene

Response Ratio

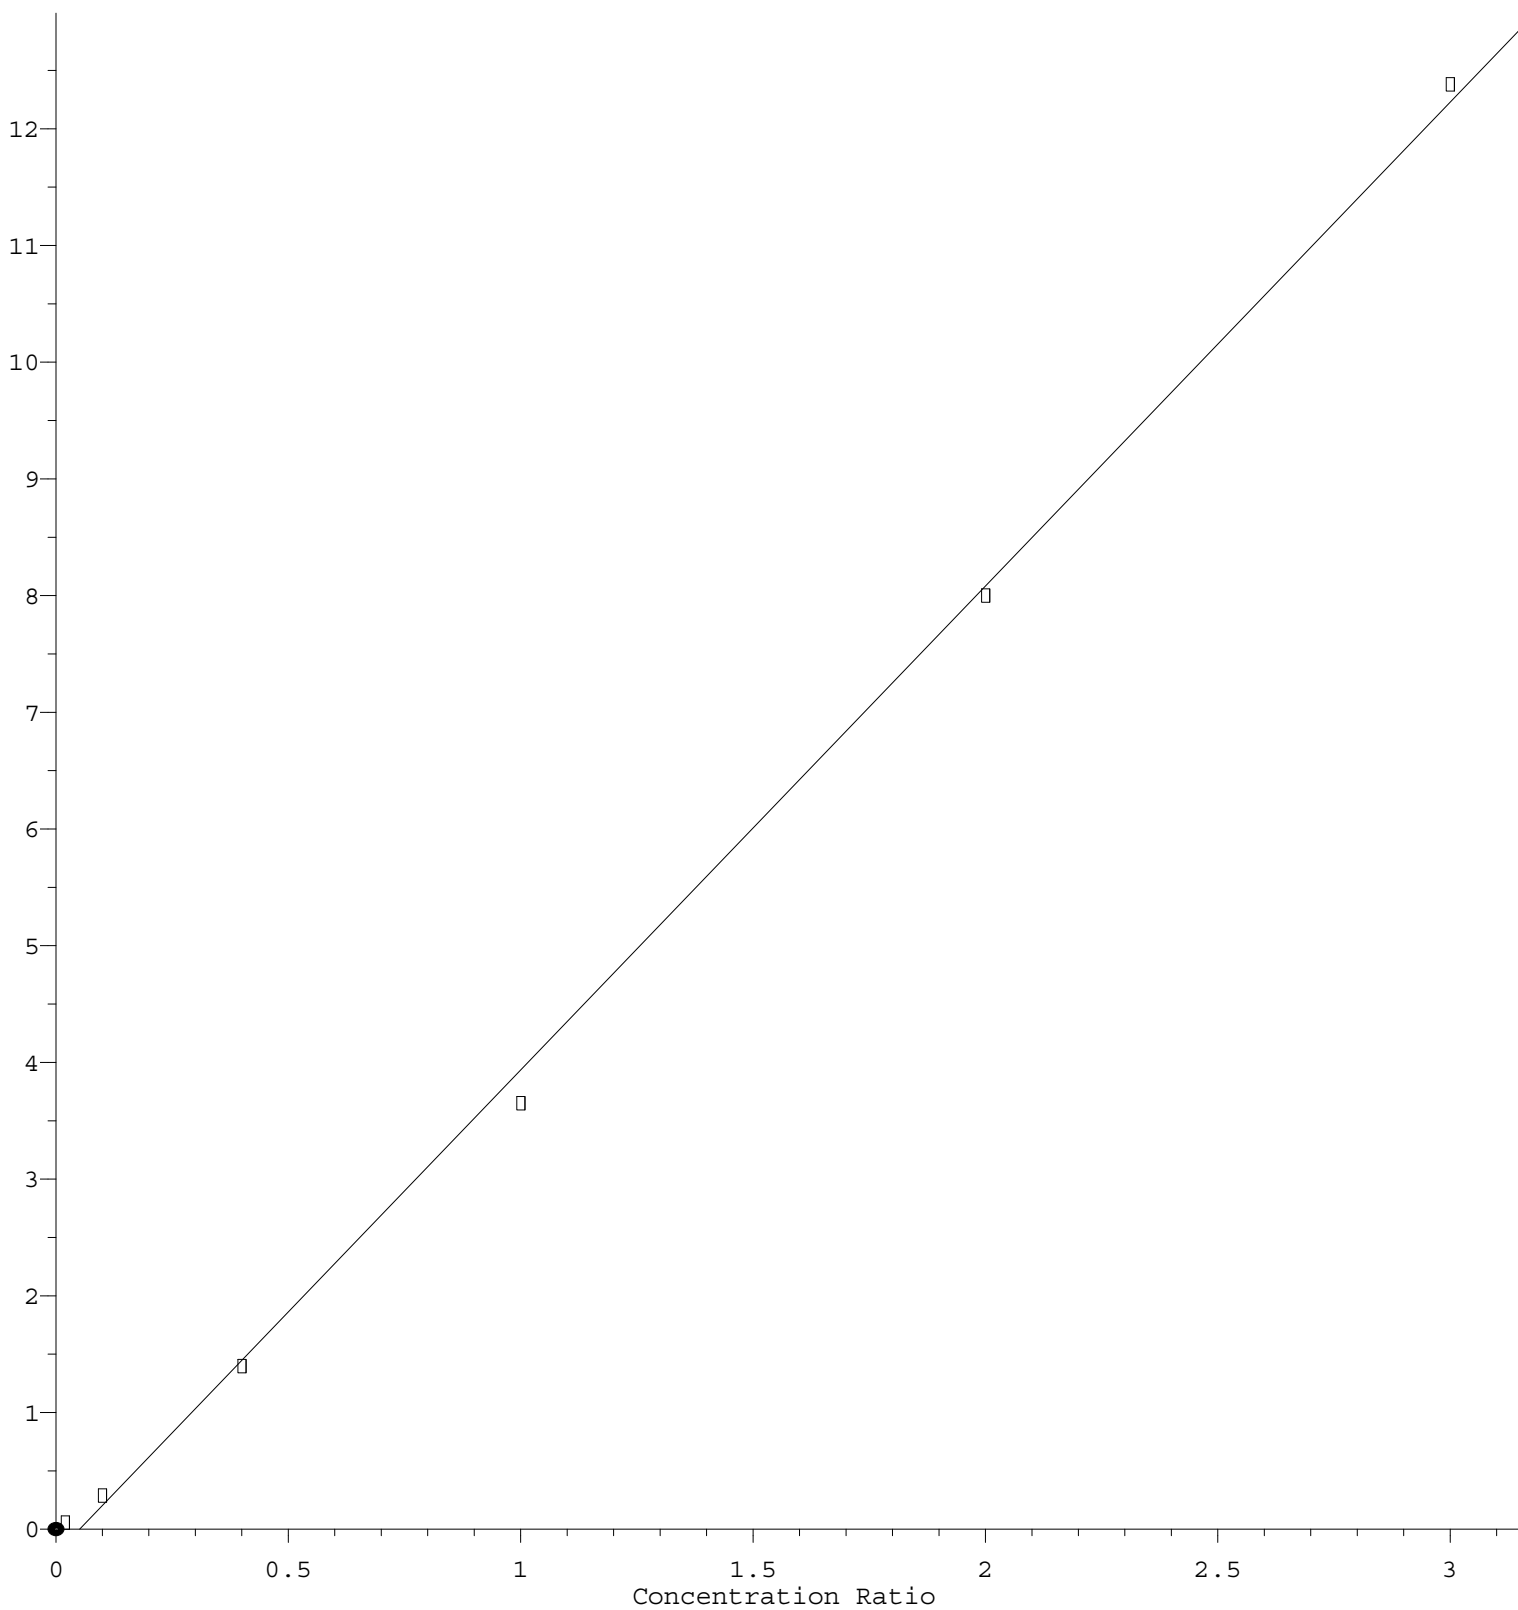

$$\text{Response} = 4.146 \times 10^0 \times \text{Amt} - 2.100 \times 10^{-1}$$

Coef of Det (r^2) = 0.998726 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U052622W.M

Calibration Table Last Updated: Fri May 27 06:42:31 2022