
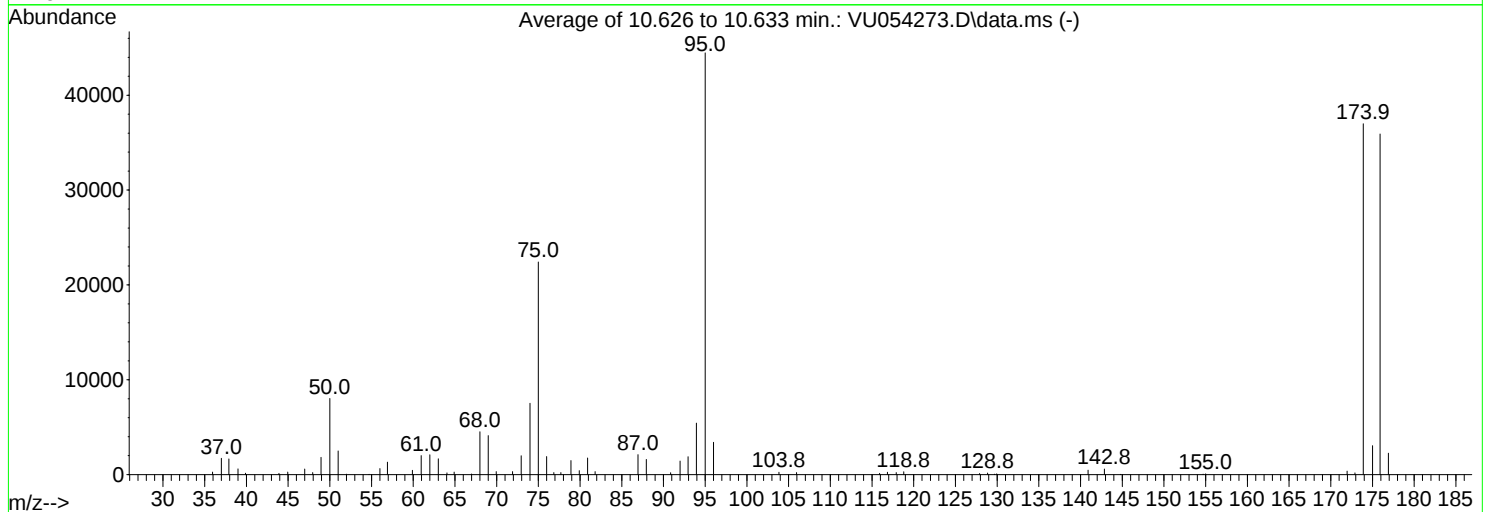


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052623\
 Data File : VU054273.D
 Acq On : 26 May 2023 09:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
 Title : SW846 8260
 Last Update : Fri May 26 06:40:51 2023

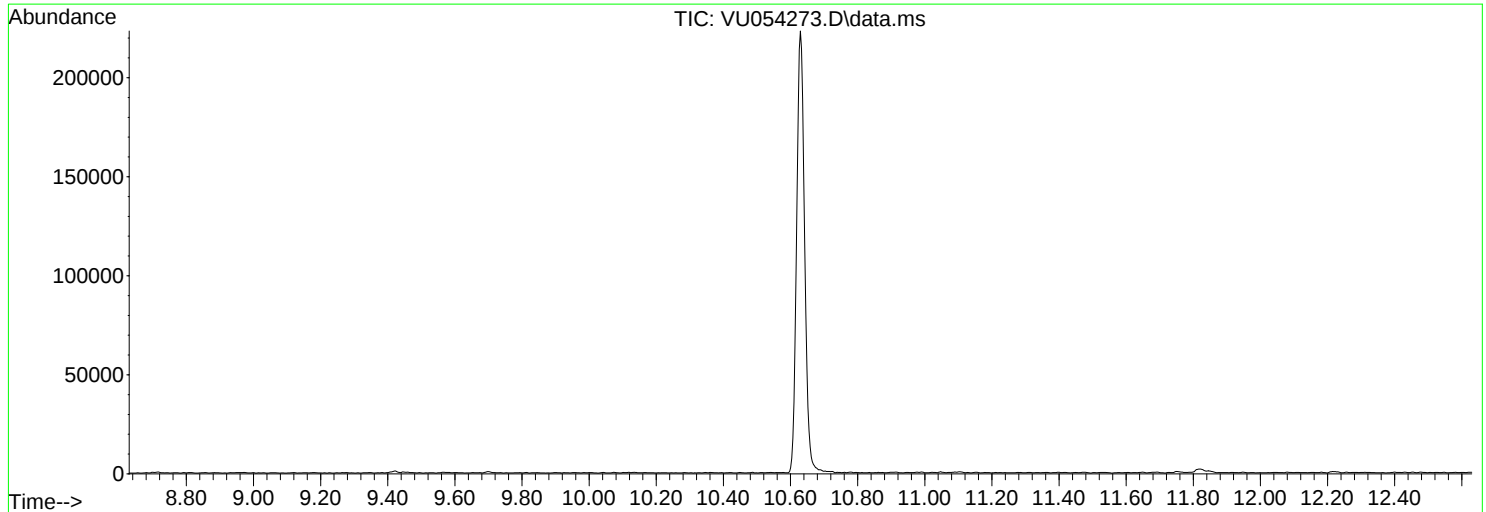

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8038	PASS
75	95	30	60	50.4	22424	PASS
95	95	100	100	100.0	44467	PASS
96	95	5	9	7.7	3403	PASS
173	174	0.00	2	0.5	185	PASS
174	95	50	100	83.2	36992	PASS
175	174	5	9	8.2	3049	PASS
176	174	95	101	97.1	35909	PASS
177	176	5	9	6.3	2267	PASS