

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052718\
 Data File : VU024183.D
 Acq On : 27 May 2018 12:55
 Operator : MD/SY
 Sample : VU0527WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 28 04:18:33 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 04:17:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	305628	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	283930	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	102900	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	124423	53.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.10%
7) Chloroethane-d5	1.68	69	100094	54.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.50%
11) 1,1-Dichloroethene-d2	2.27	63	171023	39.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.14%
21) 2-Butanone-d5	4.18	46	165032	89.34	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.34%
24) Chloroform-d	4.65	84	207517	49.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.68%
26) 1,2-Dichloroethane-d4	5.31	65	136364	51.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.40%
32) Benzene-d6	5.35	84	428790	54.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.14%
36) 1,2-Dichloropropane-d6	6.34	67	144054	53.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.98%
41) Toluene-d8	7.57	98	371677	51.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.08%
43) trans-1,3-Dichloropropene-	7.85	79	54102	50.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.04%
47) 2-Hexanone-d5	8.31	63	111866	87.06	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.06%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	184877	47.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.12%
64) 1,2-Dichlorobenzene-d4	11.87	152	127203	56.38	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.76%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	11.49	75	11997	3.62	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052718\
Data File : VU024183.D
Acq On : 27 May 2018 12:55
Operator : MD/SY
Sample : VU0527WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 28 04:18:33 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 04:17:49 2018
Response via : Initial Calibration

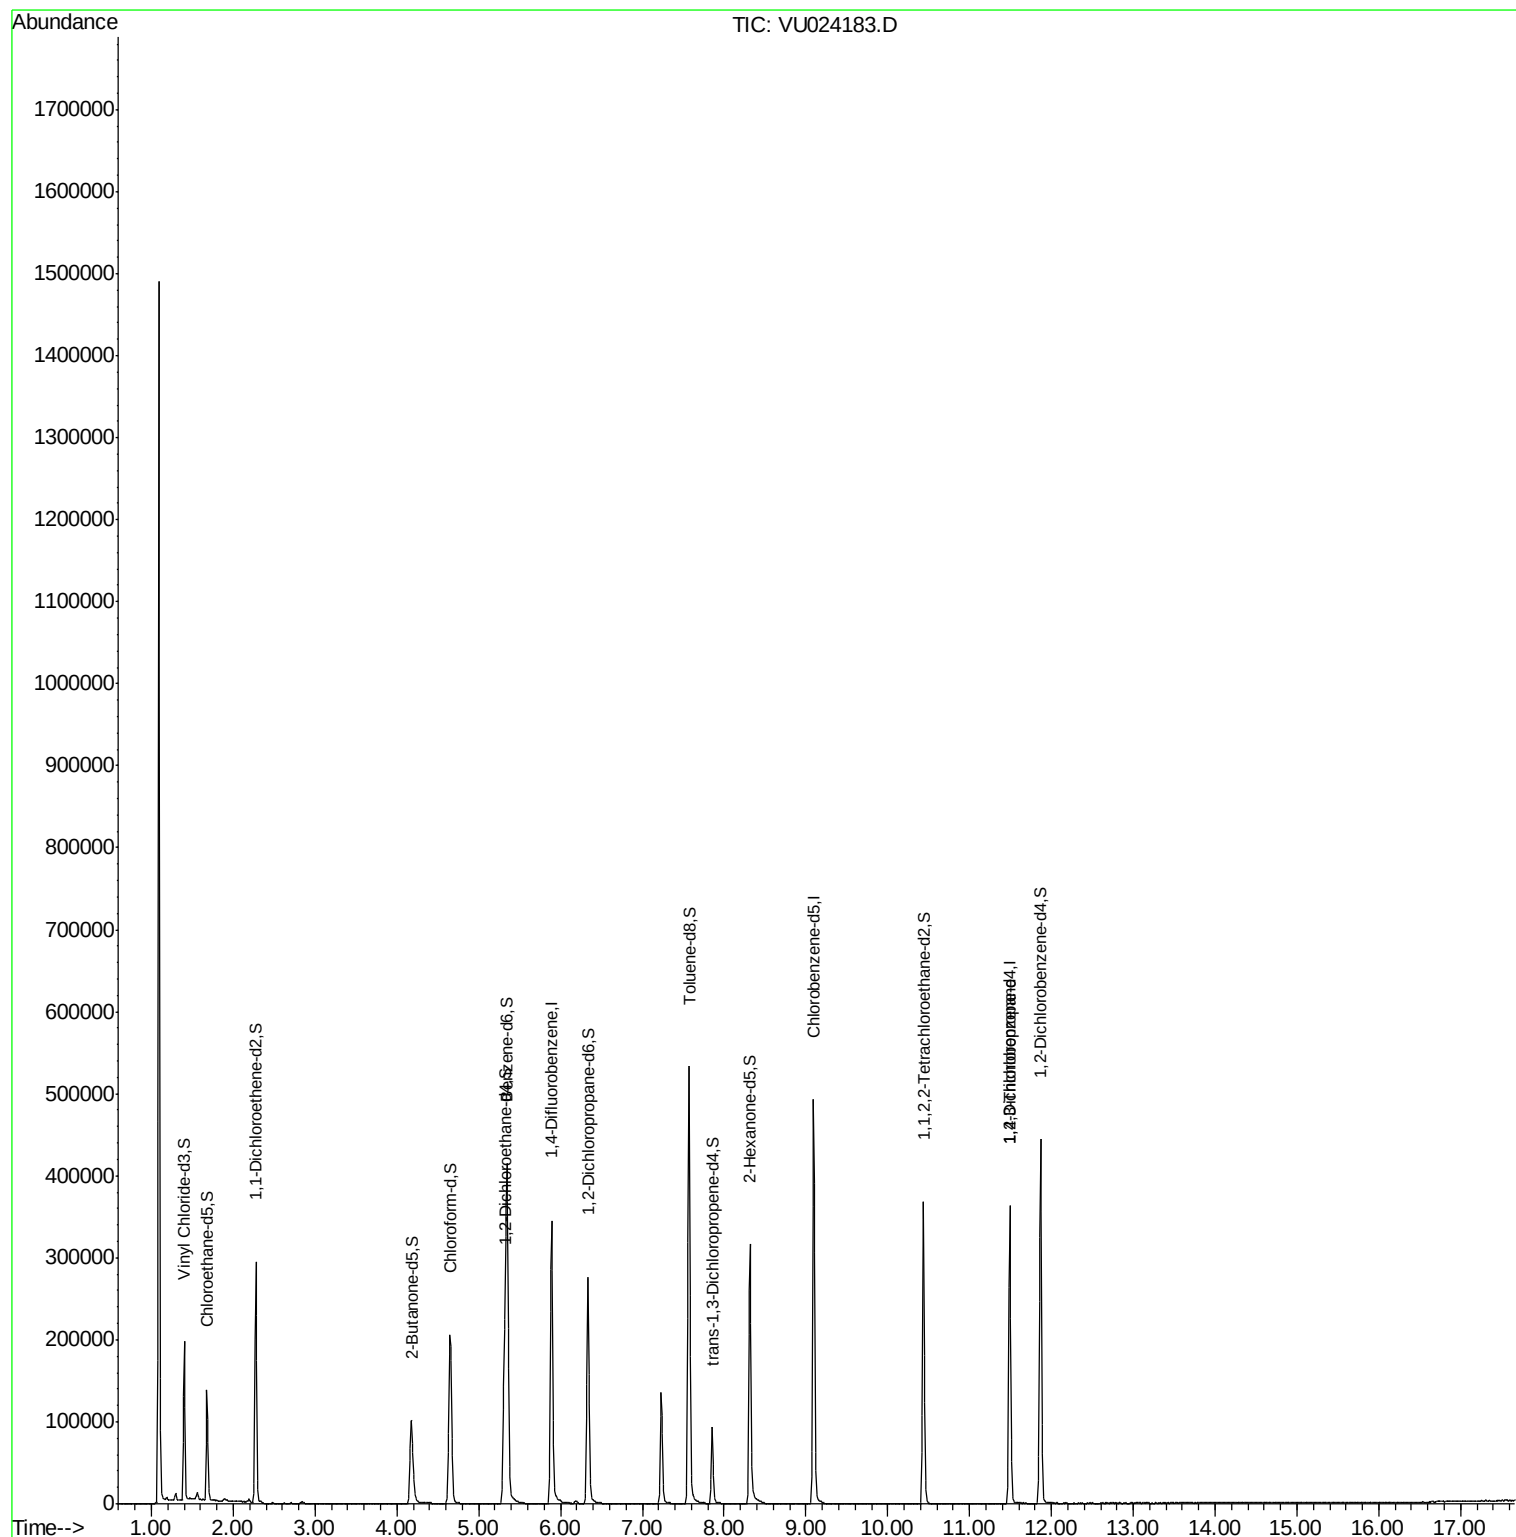

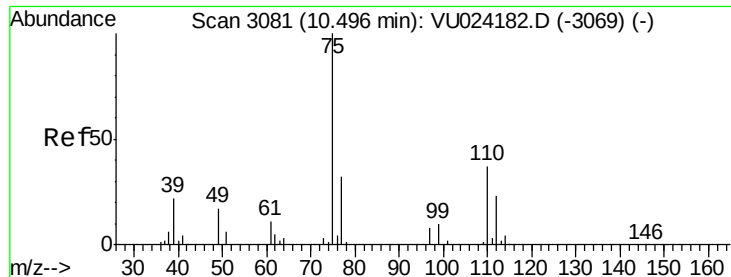

#59

1,2,3-Trichloropropane

Concen: 3.62 ug/L

RT: 11.49 min Scan# 3390

Delta R.T. 0.99 min

Lab File: VU024183.D

Acq: 27 May 2018 12:55

Tgt Ion: 75 Resp: 11997

Ion Ratio Lower Upper

75 100

77 37.5 25.5 38.3

