

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052718\
 Data File : VU024194.D
 Acq On : 27 May 2018 17:33
 Operator : MD/SY
 Sample : J3092-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 28 04:20:56 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 04:17:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	291411	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	269692	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	92626	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	105782	47.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.50%
7) Chloroethane-d5	1.68	69	88214	50.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.28%
11) 1,1-Dichloroethene-d2	2.27	63	146327	35.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.02%
21) 2-Butanone-d5	4.18	46	150937	85.70	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.70%
24) Chloroform-d	4.65	84	183713	46.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.56%
26) 1,2-Dichloroethane-d4	5.31	65	121117	48.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.32%
32) Benzene-d6	5.35	84	372994	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
36) 1,2-Dichloropropane-d6	6.34	67	127335	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.56%
41) Toluene-d8	7.57	98	323555	46.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.56%
43) trans-1,3-Dichloropropene-	7.85	79	46472	45.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.38%
47) 2-Hexanone-d5	8.31	63	100234	82.13	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.13%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	164923	44.20	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.40%
64) 1,2-Dichlorobenzene-d4	11.87	152	107539	52.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.90%


Target Compounds


						Qvalue
9) Trichlorofluoromethane	1.89	101	5480	1.55	ug/L	97
34) Trichloroethene	6.19	95	340959	135.20	ug/L	99
35) Methylcyclohexane	6.34	83	27915	8.00	ug/L #	18
37) 1,2-Dichloropropane	6.33	63	13257	5.27	ug/L #	89
46) Tetrachloroethene	8.23	164	7882	4.47	ug/L	98
49) Dibromochloromethane	8.23	129	7481	3.18	ug/L #	11
59) 1,2,3-Trichloropropane	11.49	75	10630	3.37	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU052718\
Data File : VU024194.D
Acq On : 27 May 2018 17:33
Operator : MD/SY
Sample : J3092-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1





Quant Time: May 28 04:20:56 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 04:17:49 2018
Response via : Initial Calibration

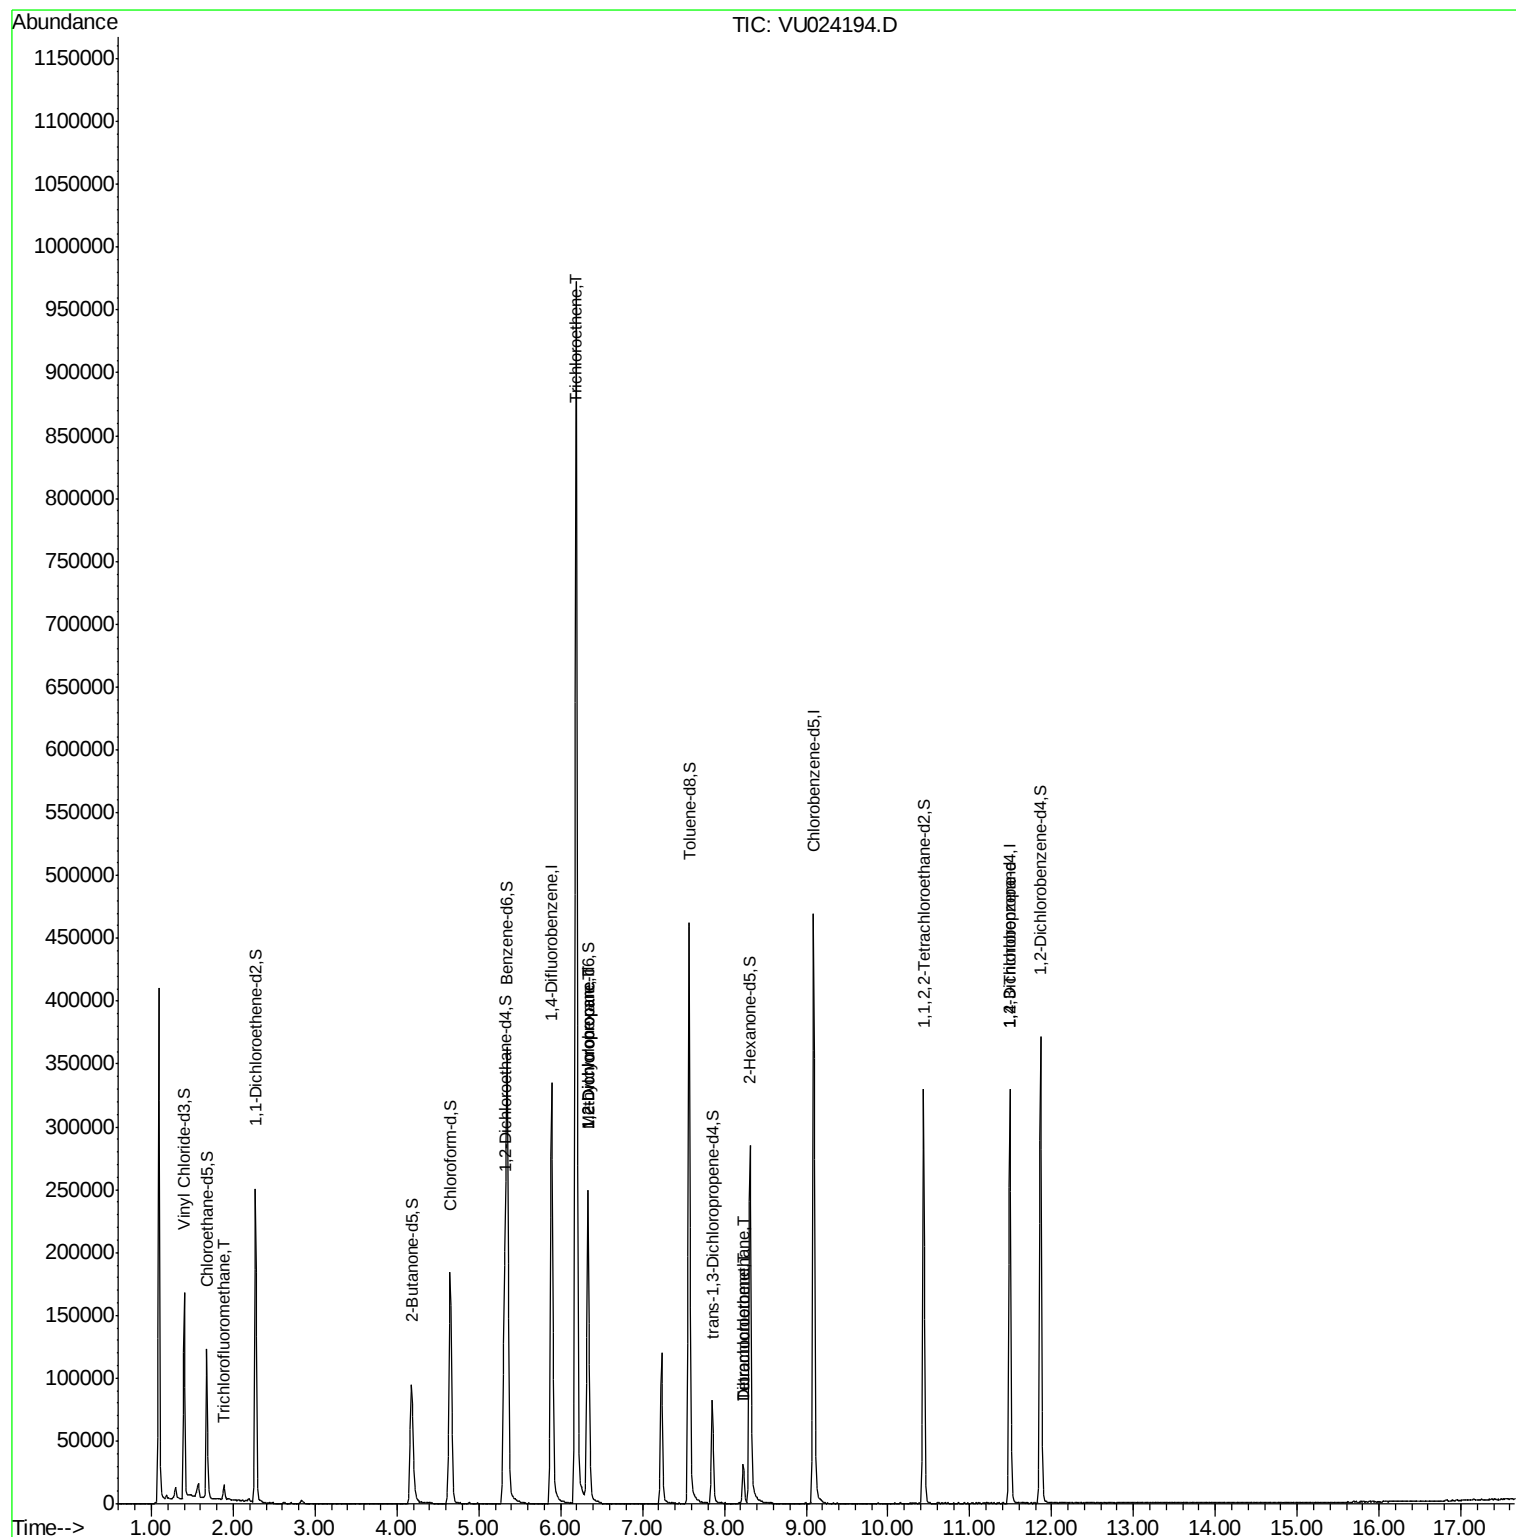

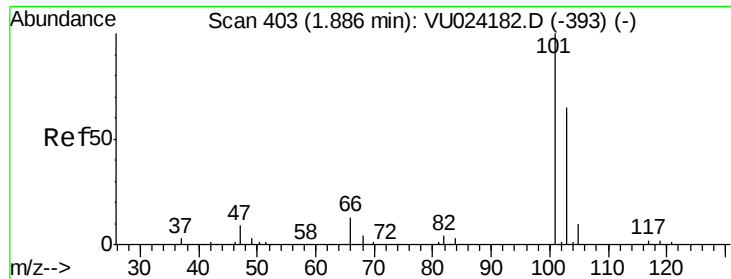




#9
 Trichlorofluoromethane
 Concen: 1.55 ug/L
 RT: 1.89 min Scan# 403
 Delta R.T. 0.00 min
 Lab File: VU024194.D
 Acq: 27 May 2018 17:33


Tgt Ion: 101 Resp: 5480
 Ion Ratio Lower Upper
 101 100
 103 62.8 52.1 78.1

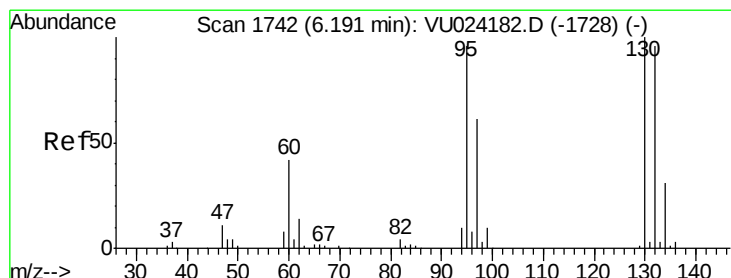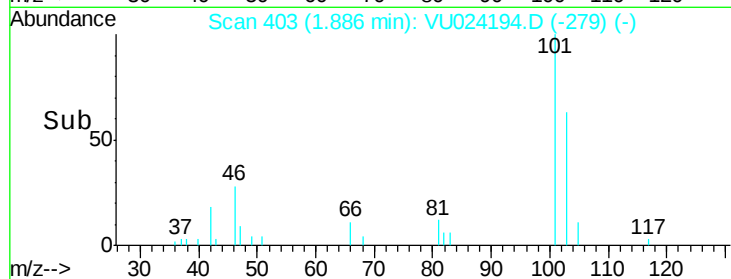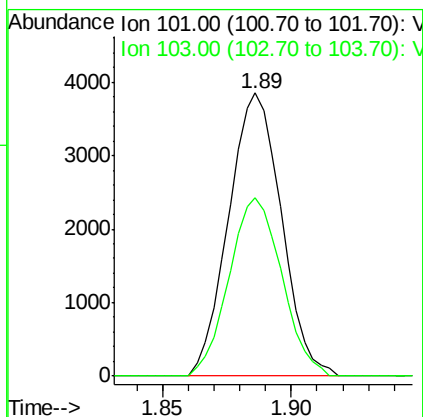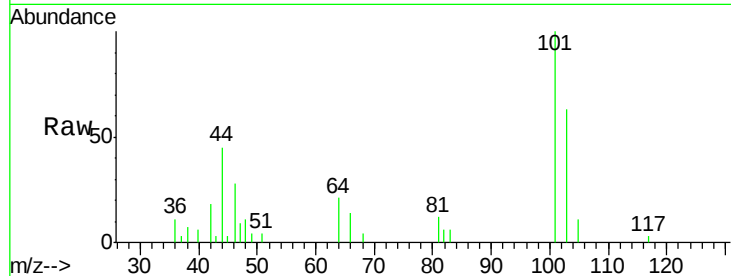

#34
 Trichloroethene
 Concen: 135.20 ug/L
 RT: 6.19 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: VU024194.D
 Acq: 27 May 2018 17:33


Tgt Ion: 95 Resp: 340959
 Ion Ratio Lower Upper
 95 100
 97 64.8 44.5 82.7
 132 97.3 69.0 128.2
 130 102.4 70.6 131.0

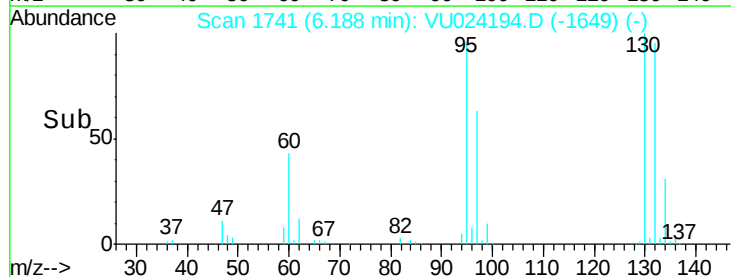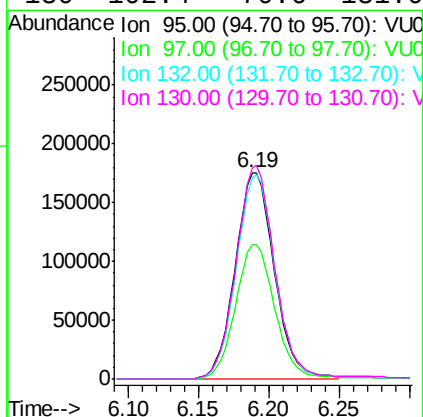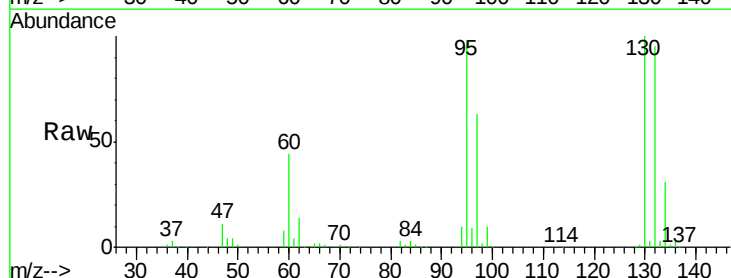



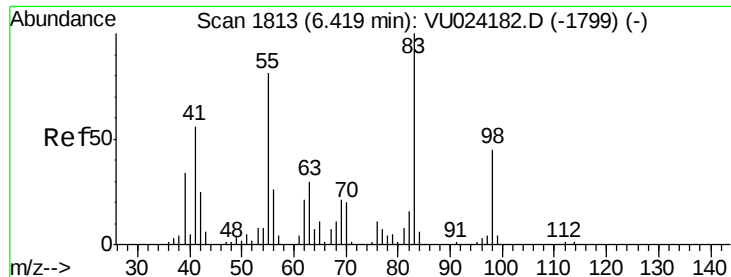


#35
Methylcyclohexane
Concen: 8.00 ug/L
RT: 6.34 min Scan# 1787
Delta R.T. -0.08 min
Lab File: VU024194.D
Acq: 27 May 2018 17:33

Tgt Ion	Ratio	Lower	Upper
83	100		
55	0.0	64.1	96.1#
98	1.3	35.8	53.8#

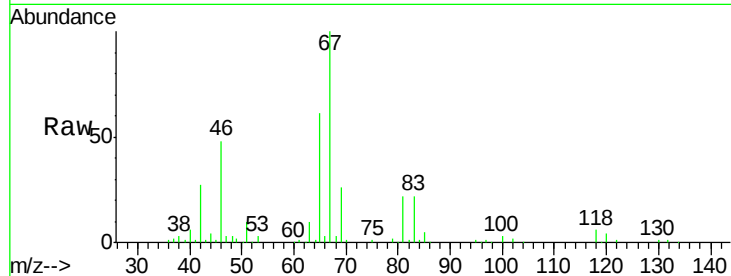


Abundance Ion 83.00 (82.70 to 83.70): VU0
Ion 55.00 (54.70 to 55.70): VU0
Ion 98.00 (97.70 to 98.70): VU0

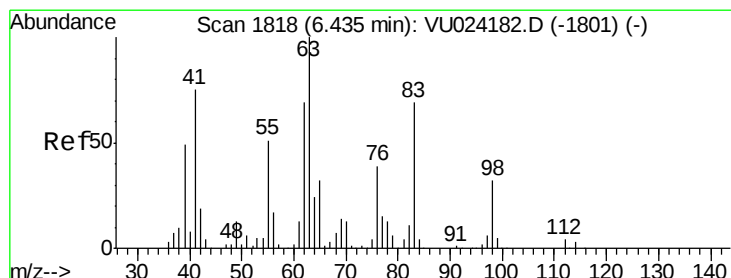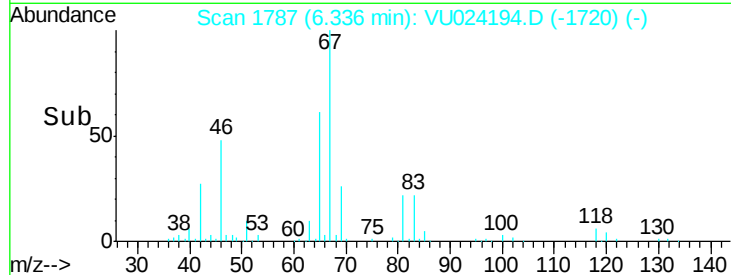
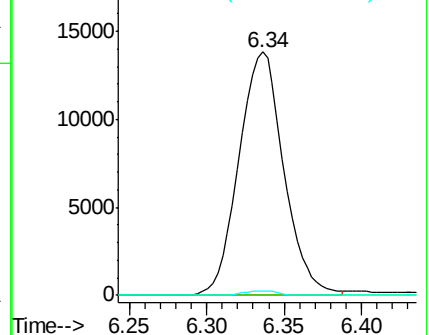



#37
1,2-Dichloropropane
Concen: 5.27 ug/L
RT: 6.33 min Scan# 1786
Delta R.T. -0.10 min
Lab File: VU024194.D
Acq: 27 May 2018 17:33

Tgt Ion	Ratio	Lower	Upper
63	100		
112	0.0	2.9	4.3#

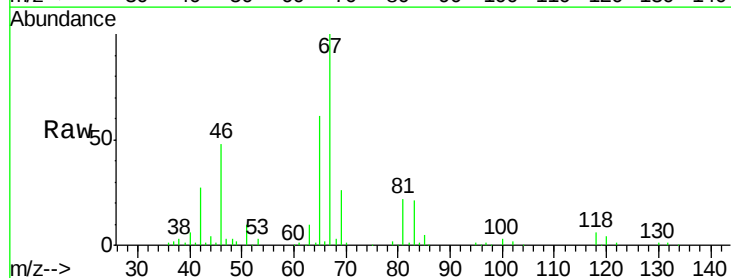

Abundance Ion 63.00 (62.70 to 63.70): VU0
Ion 112.00 (111.70 to 112.70): V

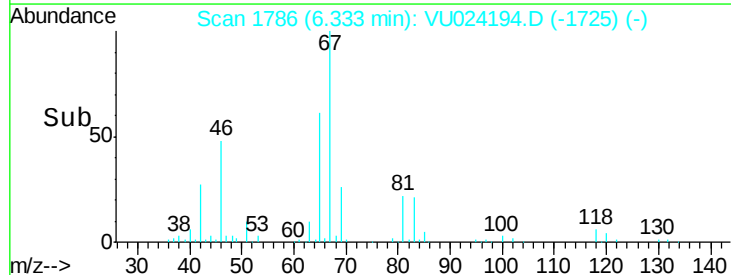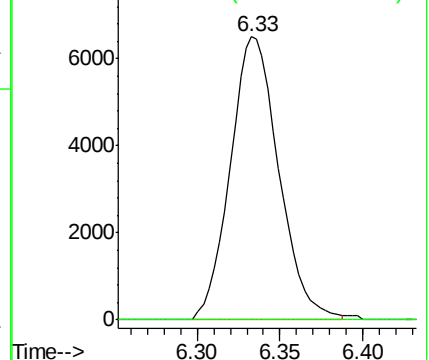

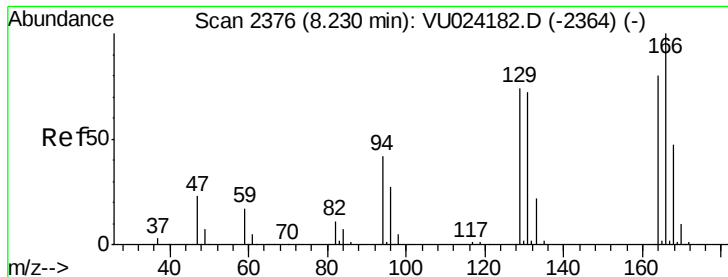

#46

Tetrachloroethene

Concen: 4.47 ug/L

RT: 8.23 min Scan# 2377

Delta R.T. 0.00 min

Lab File: VU024194.D

Acq: 27 May 2018 17:33

Tgt Ion:164 Resp: 7882


Ion Ratio Lower Upper

164 100

129 93.6 66.6 123.6

131 93.7 64.5 119.9

166 131.3 89.3 165.9



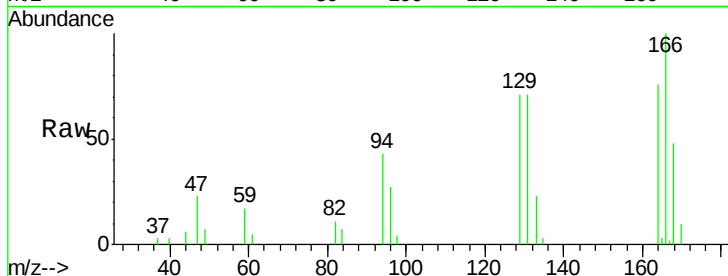


Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

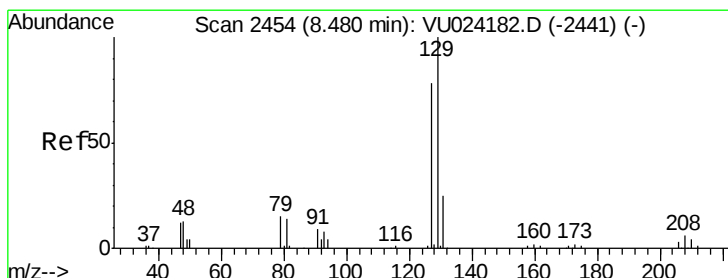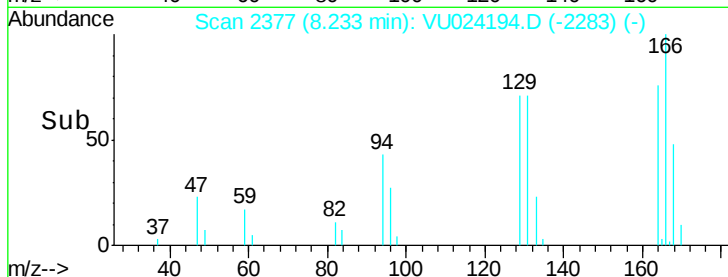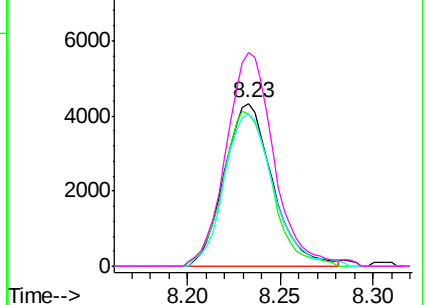

#49

Dibromochloromethane

Concen: 3.18 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. -0.25 min

Lab File: VU024194.D


Acq: 27 May 2018 17:33

Tgt Ion:129 Resp: 7481

Ion Ratio Lower Upper



129 100


127 0.0 54.2 100.6#

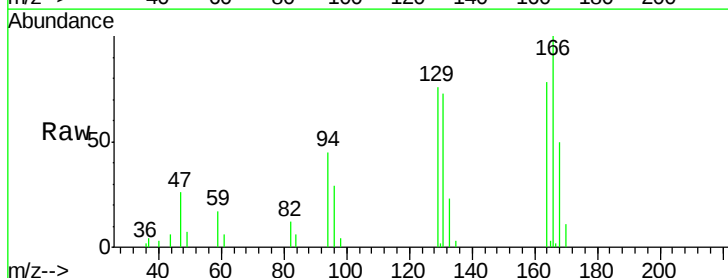

Abundance Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

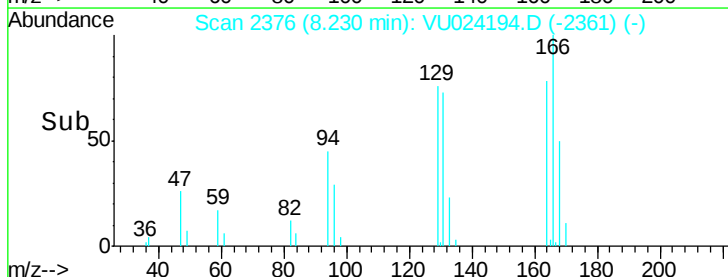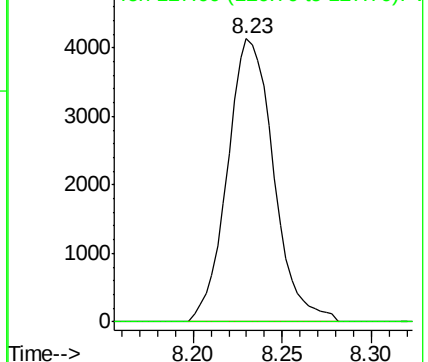

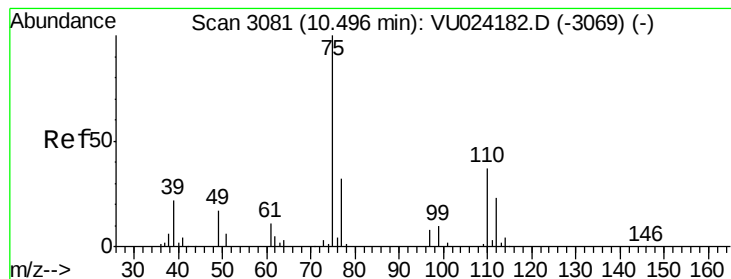

#59
 1,2,3-Trichloropropane
 Concen: 3.37 ug/L
 RT: 11.49 min Scan# 3389
 Delta R.T. 0.99 min
 Lab File: VU024194.D
 Acq: 27 May 2018 17:33

Tgt Ion: 75 Resp: 10630
 Ion Ratio Lower Upper
 75 100
 77 37.9 25.5 38.3

