

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
 Data File : VU024186.D
 Acq On : 27 May 2018 14:11
 Operator : MD/SY
 Sample : J3043-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 28 04:29:53 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 04:17:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	310917	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	292136	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	102889	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	127032	53.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.48%
7) Chloroethane-d5	1.68	69	103782	55.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.58%
11) 1,1-Dichloroethene-d2	2.27	63	174643	39.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.44%
21) 2-Butanone-d5	4.18	46	172853	91.99	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.99%
24) Chloroform-d	4.65	84	214332	50.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.31	65	140765	52.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.92%
32) Benzene-d6	5.35	84	442169	54.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.38%
36) 1,2-Dichloropropane-d6	6.34	67	147651	53.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.56%
41) Toluene-d8	7.57	98	384296	51.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.58%
43) trans-1,3-Dichloropropene-	7.85	79	54730	49.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.34%
47) 2-Hexanone-d5	8.31	63	116013	87.76	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.76%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	190494	47.13	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.26%
64) 1,2-Dichlorobenzene-d4	11.87	152	129235	57.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.58%


Target Compounds					Ovalue
13) Acetone	2.32	43	6586	4.02 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
Data File : VU024186.D
Acq On : 27 May 2018 14:11
Operator : MD/SY
Sample : J3043-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 28 04:29:53 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 04:17:49 2018
Response via : Initial Calibration

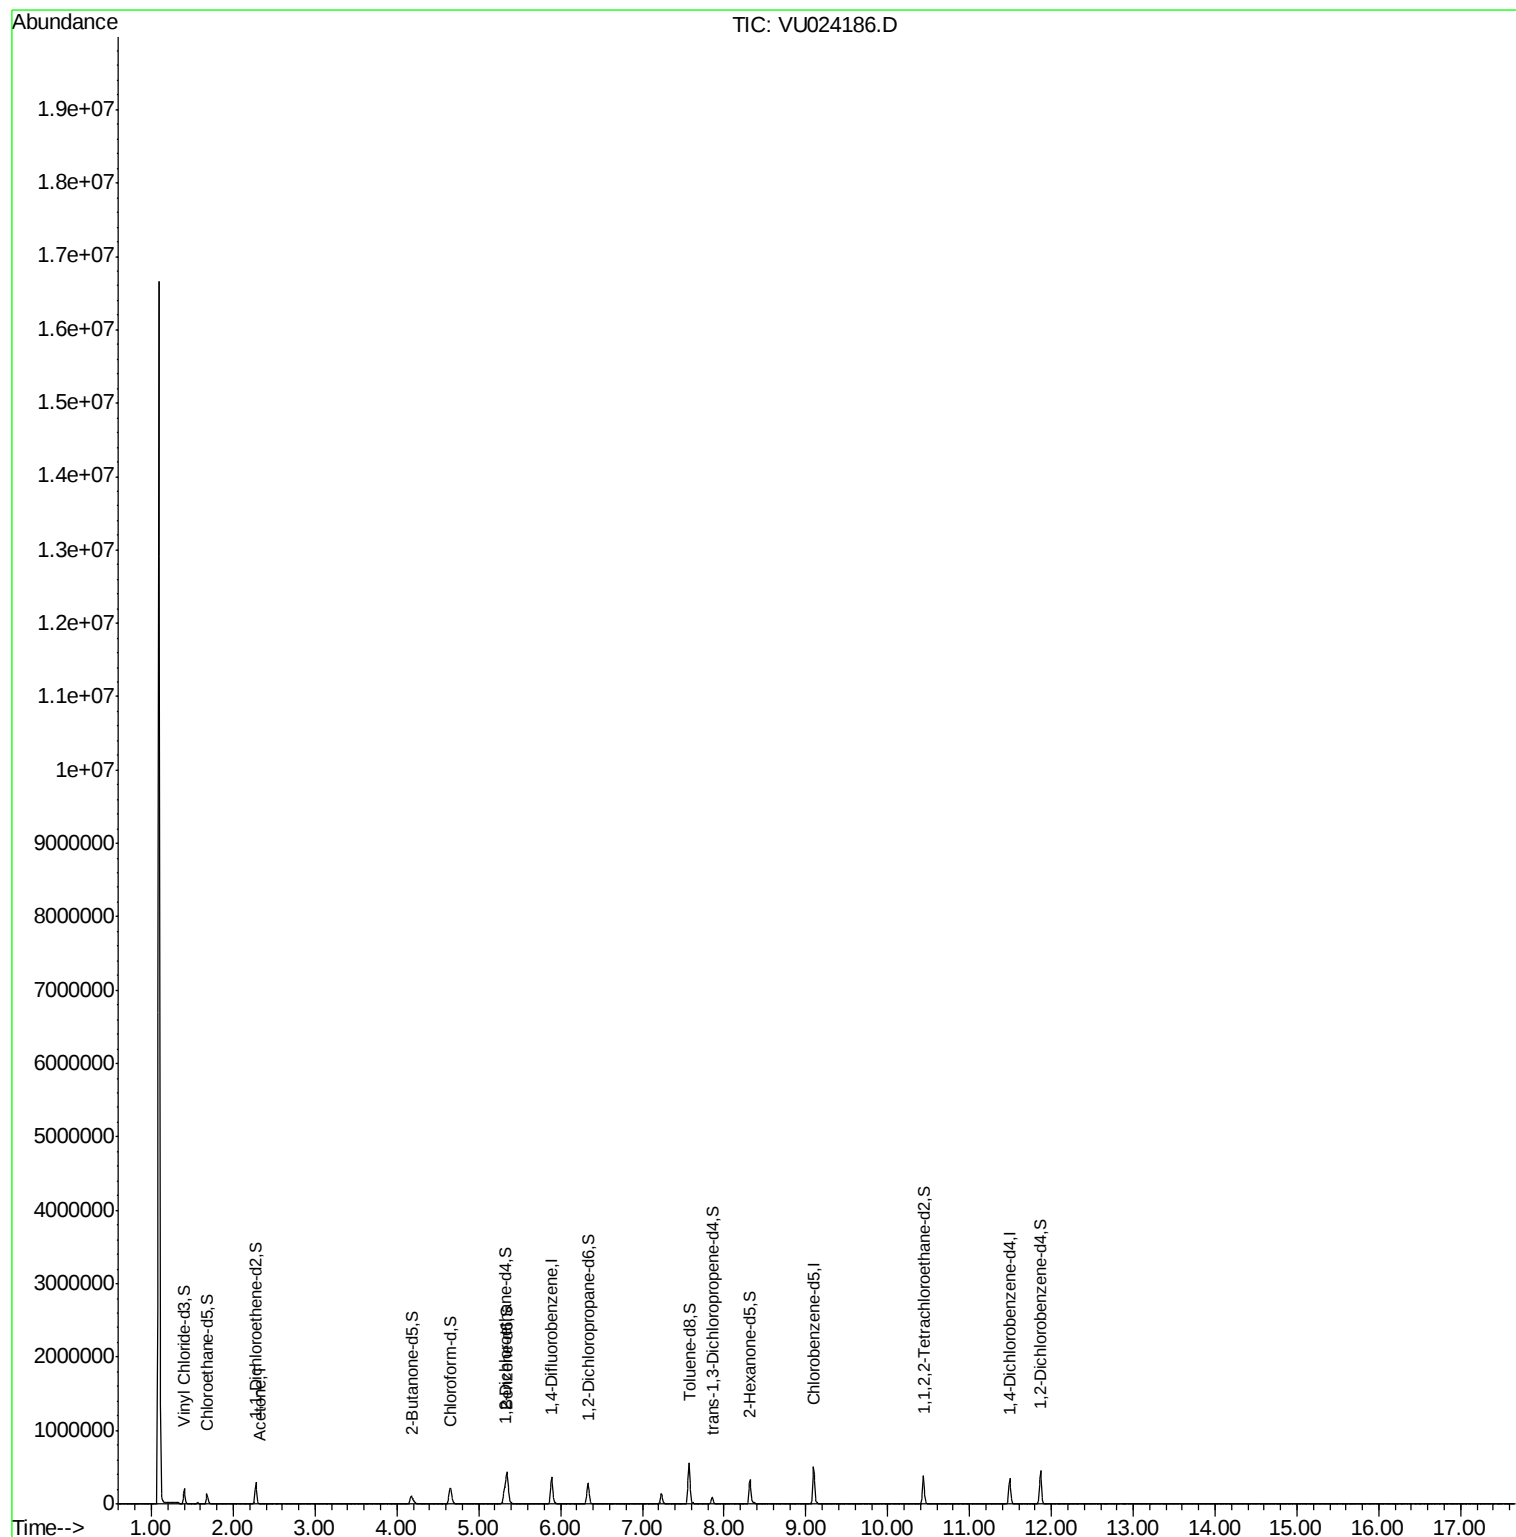

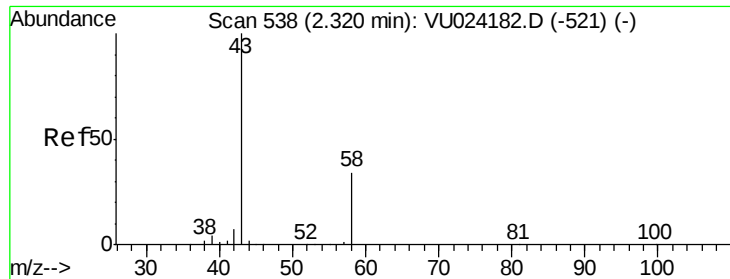

#13

Acetone

Concen: 4.02 ug/L

RT: 2.32 min Scan# 539

Delta R.T. 0.00 min

Lab File: VU024186.D

Acq: 27 May 2018 14:11

Tot Ion: 43 Resp: 6586

Ion Ratio Lower Upper

43 100

58 33.5 0.0 64.4

