

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
 Data File : VU024194.D
 Acq On : 27 May 2018 17:33
 Operator : MD/SY
 Sample : J3092-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 28 04:50:27 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 04:17:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	291411	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	269692	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	92626	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	105782	47.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.50%
7) Chloroethane-d5	1.68	69	88214	50.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.28%
11) 1,1-Dichloroethene-d2	2.27	63	146327	35.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.02%
21) 2-Butanone-d5	4.18	46	150937	85.70	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.70%
24) Chloroform-d	4.65	84	183713	46.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.56%
26) 1,2-Dichloroethane-d4	5.31	65	121117	48.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.32%
32) Benzene-d6	5.35	84	372994	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
36) 1,2-Dichloropropane-d6	6.34	67	127335	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.56%
41) Toluene-d8	7.57	98	323555	46.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.56%
43) trans-1,3-Dichloropropene-	7.85	79	46472	45.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.38%
47) 2-Hexanone-d5	8.31	63	100234	82.13	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.13%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	164923	44.20	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.40%
64) 1,2-Dichlorobenzene-d4	11.87	152	107539	52.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.90%


Target Compounds						Ovalue
9) Trichlorofluoromethane	1.89	101	5480	1.55	ug/L	97
34) Trichloroethene	6.19	95	340959	135.20	ug/L	99
46) Tetrachloroethene	8.23	164	7882	4.47	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
Data File : VU024194.D
Acq On : 27 May 2018 17:33
Operator : MD/SY
Sample : J3092-12 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 28 04:50:27 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 04:17:49 2018
Response via : Initial Calibration

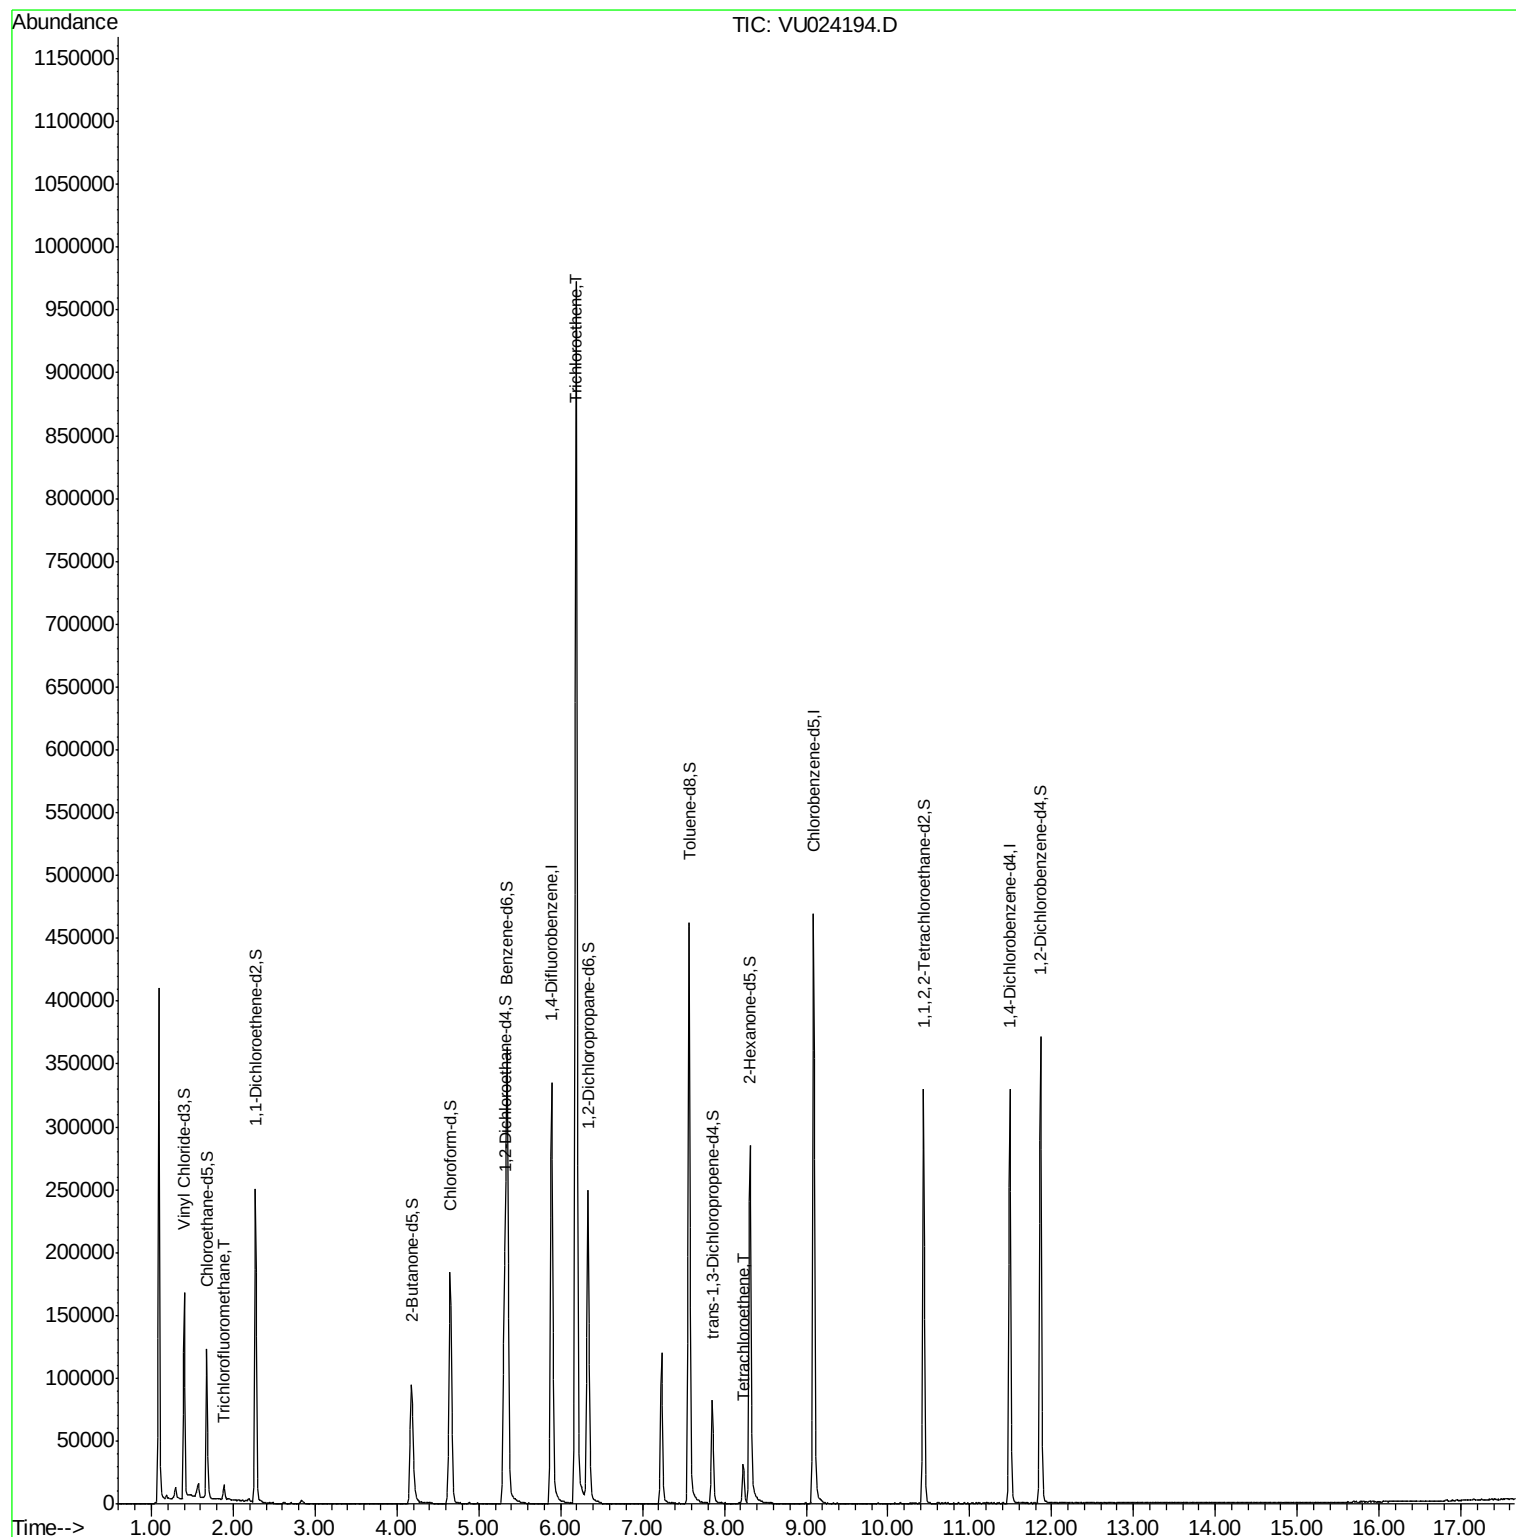

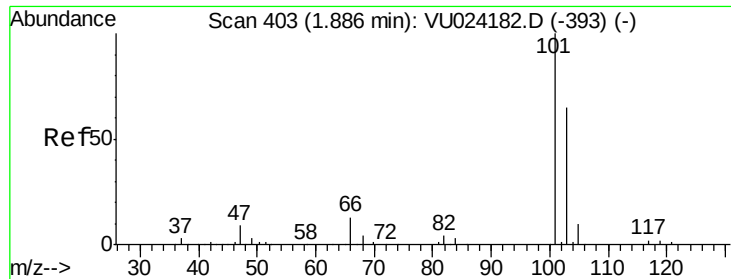

#9

Trichlorofluoromethane

Concen: 1.55 ug/L

RT: 1.89 min Scan# 403

Delta R.T. 0.00 min

Lab File: VU024194.D


Acq: 27 May 2018 17:33

Tot Ion:101 Resp: 5480

Ion Ratio Lower Upper




101 100

103 62.8 52.1 78.1

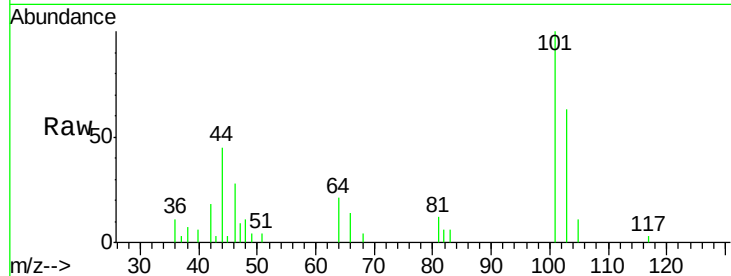

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

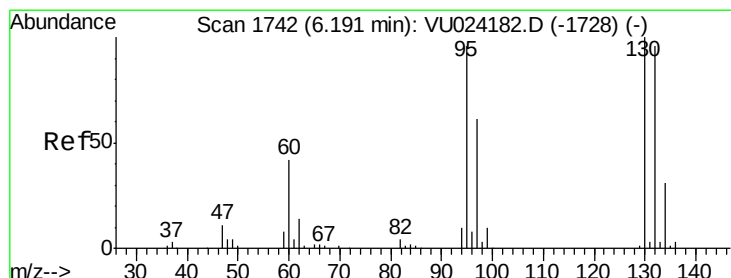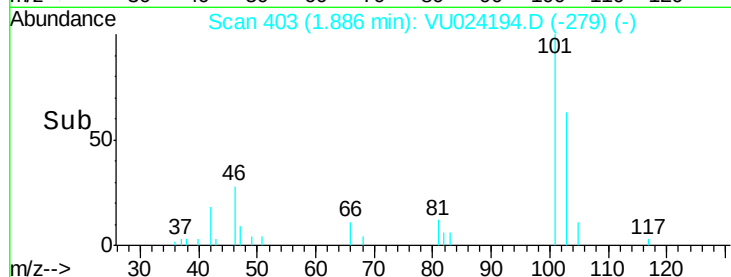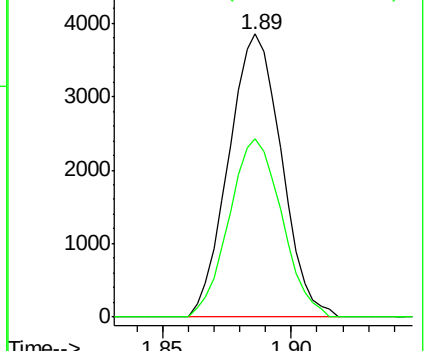

#34

Trichloroethene

Concen: 135.20 ug/L

RT: 6.19 min Scan# 1741

Delta R.T. -0.00 min

Lab File: VU024194.D

Acq: 27 May 2018 17:33

Tgt Ion: 95 Resp: 340959


Ion Ratio Lower Upper

95 100

97 64.8 44.5 82.7

132 97.3 69.0 128.2

130 102.4 70.6 131.0


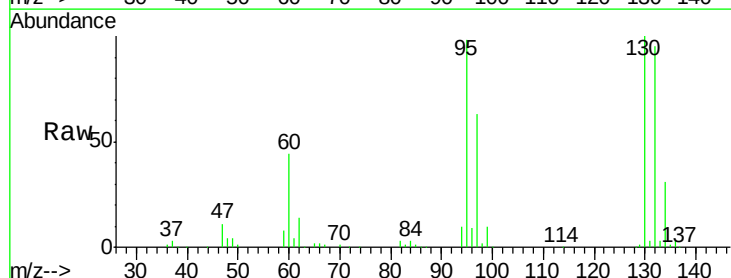



Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

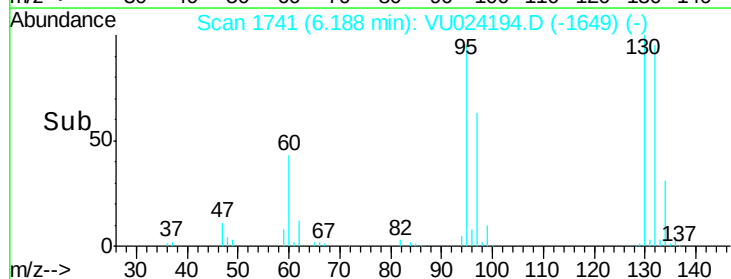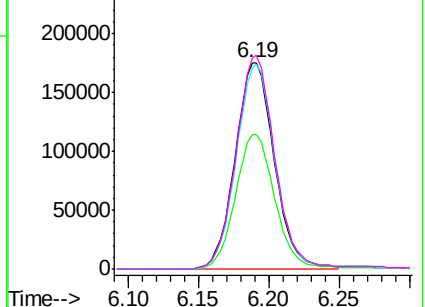

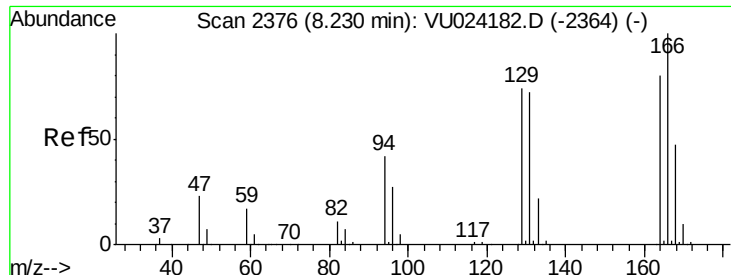

#46

Tetrachloroethene

Concen: 4.47 ug/L

RT: 8.23 min Scan# 2377

Delta R.T. 0.00 min

Lab File: VU024194.D

Acq: 27 May 2018 17:33

Tot Ion:164 Resp: 7882



Ion Ratio Lower Upper

164 100

129 93.6 66.6 123.6

131 93.7 64.5 119.9

166 131.3 89.3 165.9

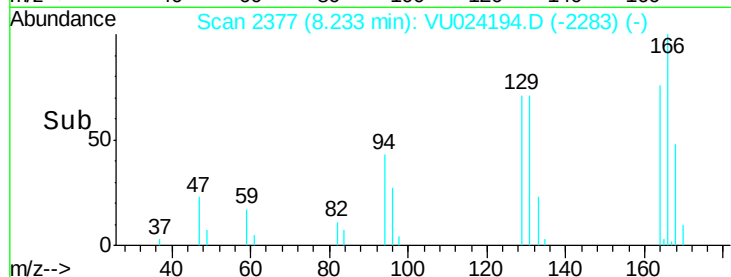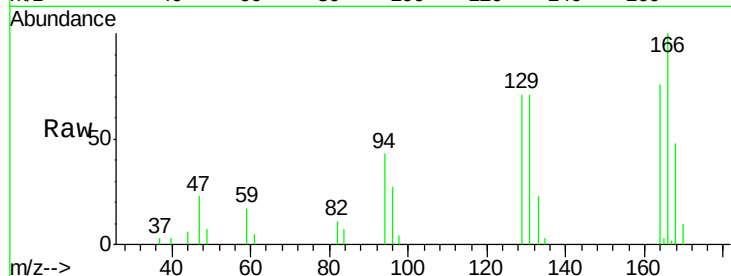

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

