

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
 Data File : VU024203.D
 Acq On : 27 May 2018 21:20
 Operator : MD/SY
 Sample : J3091-06 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: May 28 05:10:32 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 04:17:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	303473	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	287942	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	99506	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	108580	47.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.12%
7) Chloroethane-d5	1.68	69	91266	49.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.64%
11) 1,1-Dichloroethene-d2	2.27	63	151950	35.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.82%
21) 2-Butanone-d5	4.18	46	165812	90.40	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.40%
24) Chloroform-d	4.65	84	191296	46.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.54%
26) 1,2-Dichloroethane-d4	5.31	65	128382	49.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.04%
32) Benzene-d6	5.35	84	392233	49.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.44%
36) 1,2-Dichloropropane-d6	6.34	67	135152	49.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.96%
41) Toluene-d8	7.57	98	337984	45.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.52%
43) trans-1,3-Dichloropropene-	7.85	79	47210	43.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.94%
47) 2-Hexanone-d5	8.31	63	110751	85.00	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.00%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	176356	44.26	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.52%
64) 1,2-Dichlorobenzene-d4	11.86	152	114370	52.42	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.84%


Target Compounds					Ovalue
9) Trichlorofluoromethane	1.89	101	5938	1.61 ug/L	100
34) Trichloroethene	6.19	95	290367	107.84 ug/L	98
46) Tetrachloroethene	8.23	164	4869	2.58 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
Data File : VU024203.D
Acq On : 27 May 2018 21:20
Operator : MD/SY
Sample : J3091-06 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: May 28 05:10:32 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 04:17:49 2018
Response via : Initial Calibration

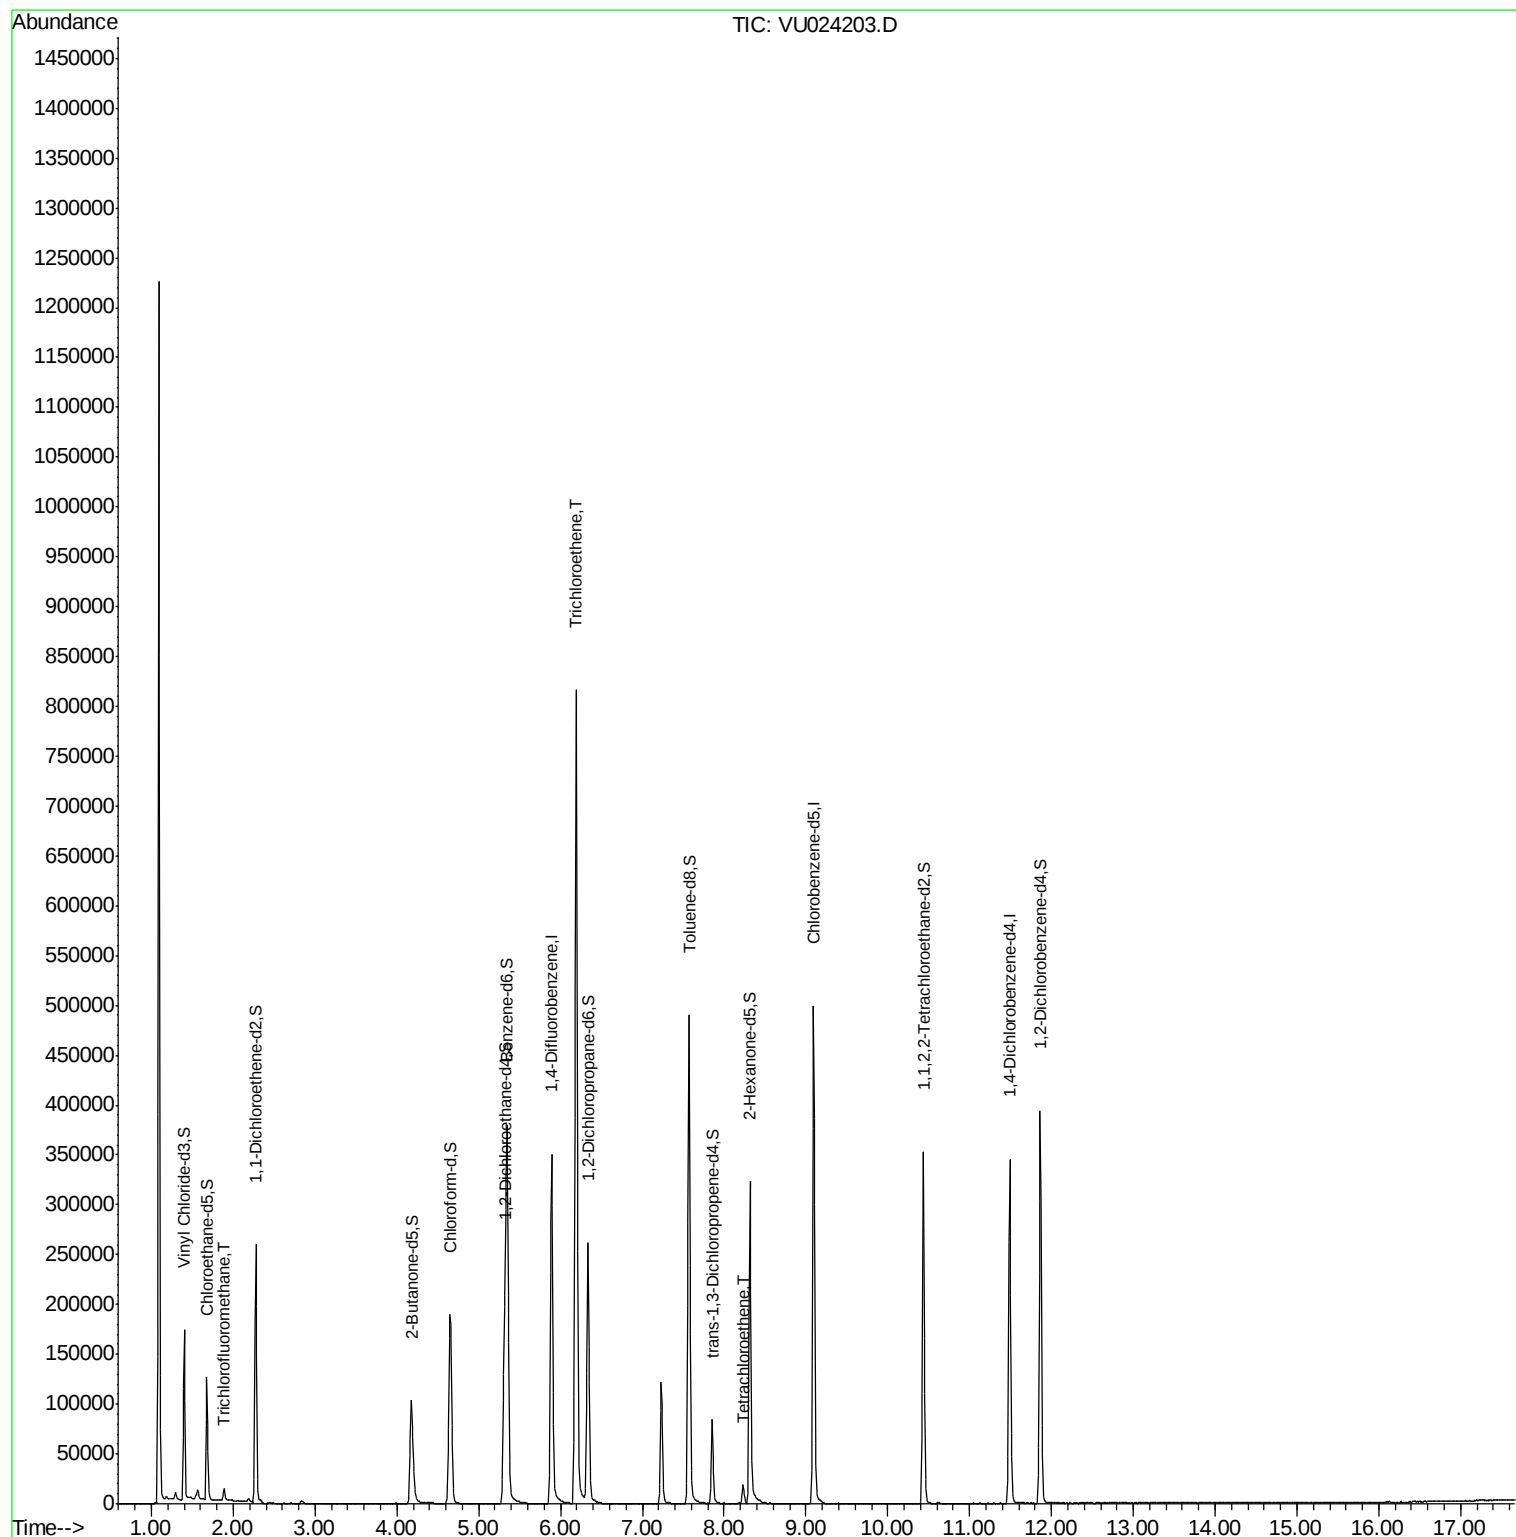

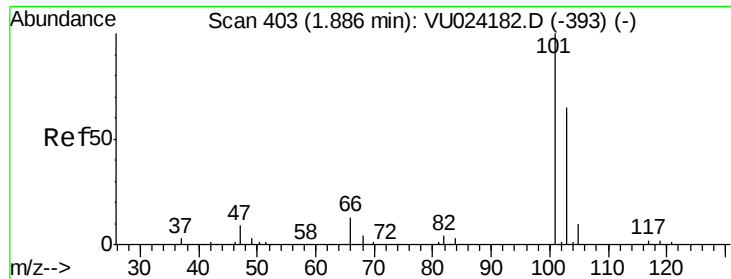

#9

Trichlorofluoromethane

Concen: 1.61 ug/L

RT: 1.89 min Scan# 403

Delta R.T. -0.00 min

Lab File: VU024203.D


Acq: 27 May 2018 21:20

Tot Ion: 101 Resp: 5938

Ion Ratio Lower Upper




101 100

103 65.1 52.1 78.1

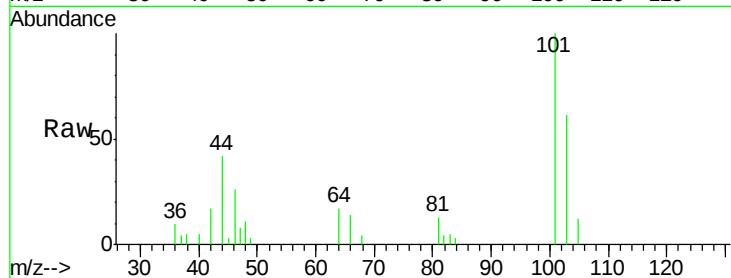

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

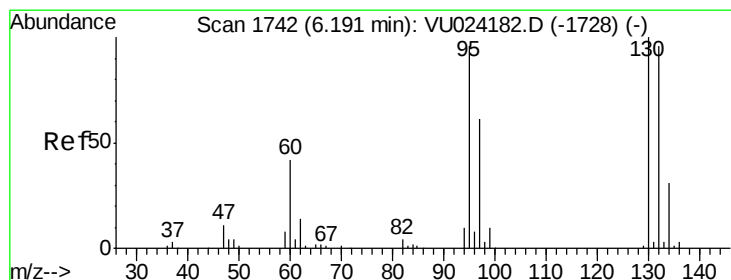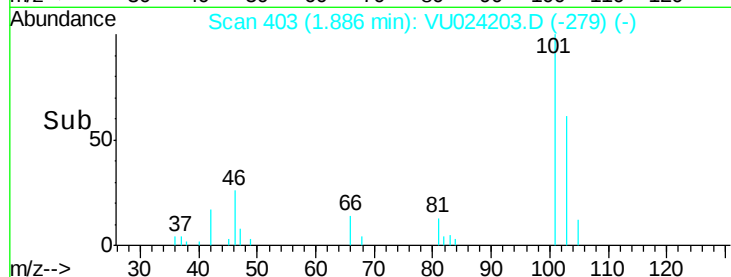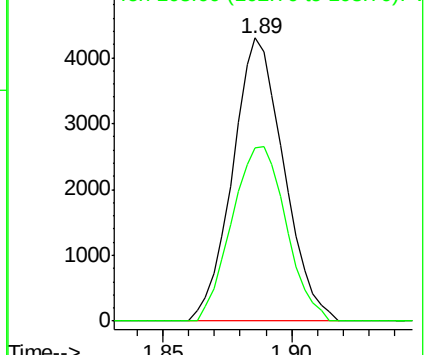

#34

Trichloroethene

Concen: 107.84 ug/L

RT: 6.19 min Scan# 1742

Delta R.T. -0.00 min

Lab File: VU024203.D

Acq: 27 May 2018 21:20

Tgt Ion: 95 Resp: 290367


Ion Ratio Lower Upper

95 100

97 65.5 44.5 82.7

132 99.2 69.0 128.2

130 103.0 70.6 131.0


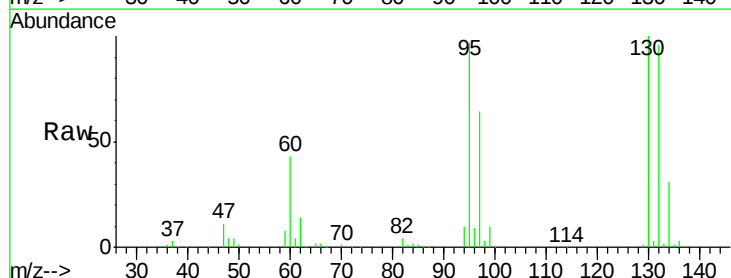



Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

Ion 132.00 (131.70 to 132.70): VU0

Ion 130.00 (129.70 to 130.70): VU0

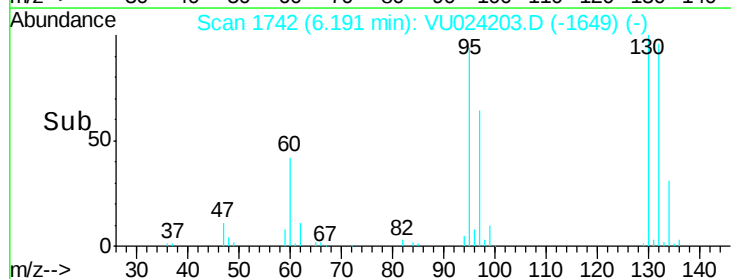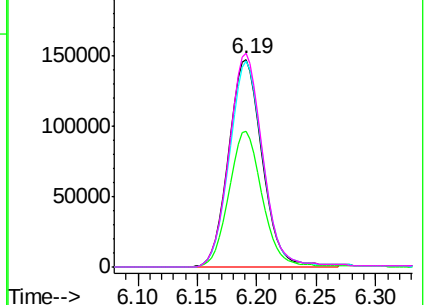

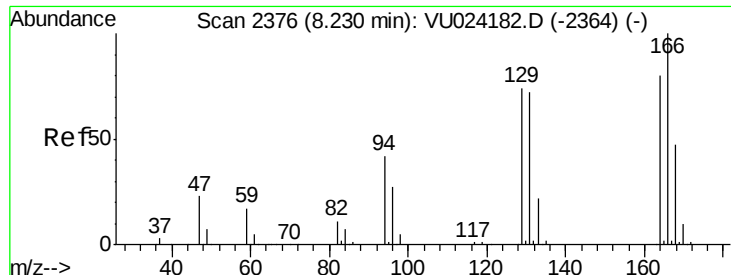

#46

Tetrachloroethene


Concen: 2.58 ug/L

RT: 8.23 min Scan# 2377

Delta R.T. 0.00 min

Lab File: VU024203.D

Acq: 27 May 2018 21:20

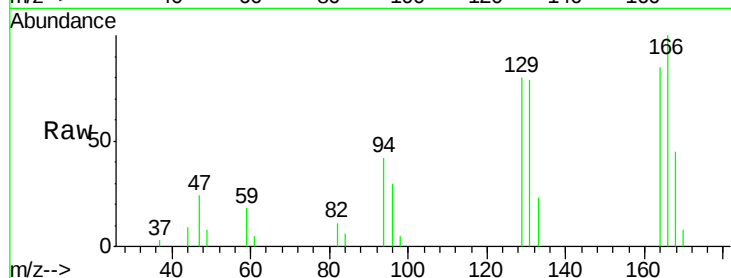

Tot Ion:164 Resp: 4869

Ion Ratio Lower Upper

164 100

129 94.7 66.6 123.6

131 92.7 64.5 119.9

166 118.0 89.3 165.9

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

