


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU052718\
Data File : VU024181.D
Acq On : 27 May 2018 11:21
Operator : MD/SY
Sample : BFB60
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
Title : VOC Analysis
Last Update : Mon May 28 05:15:39 2018

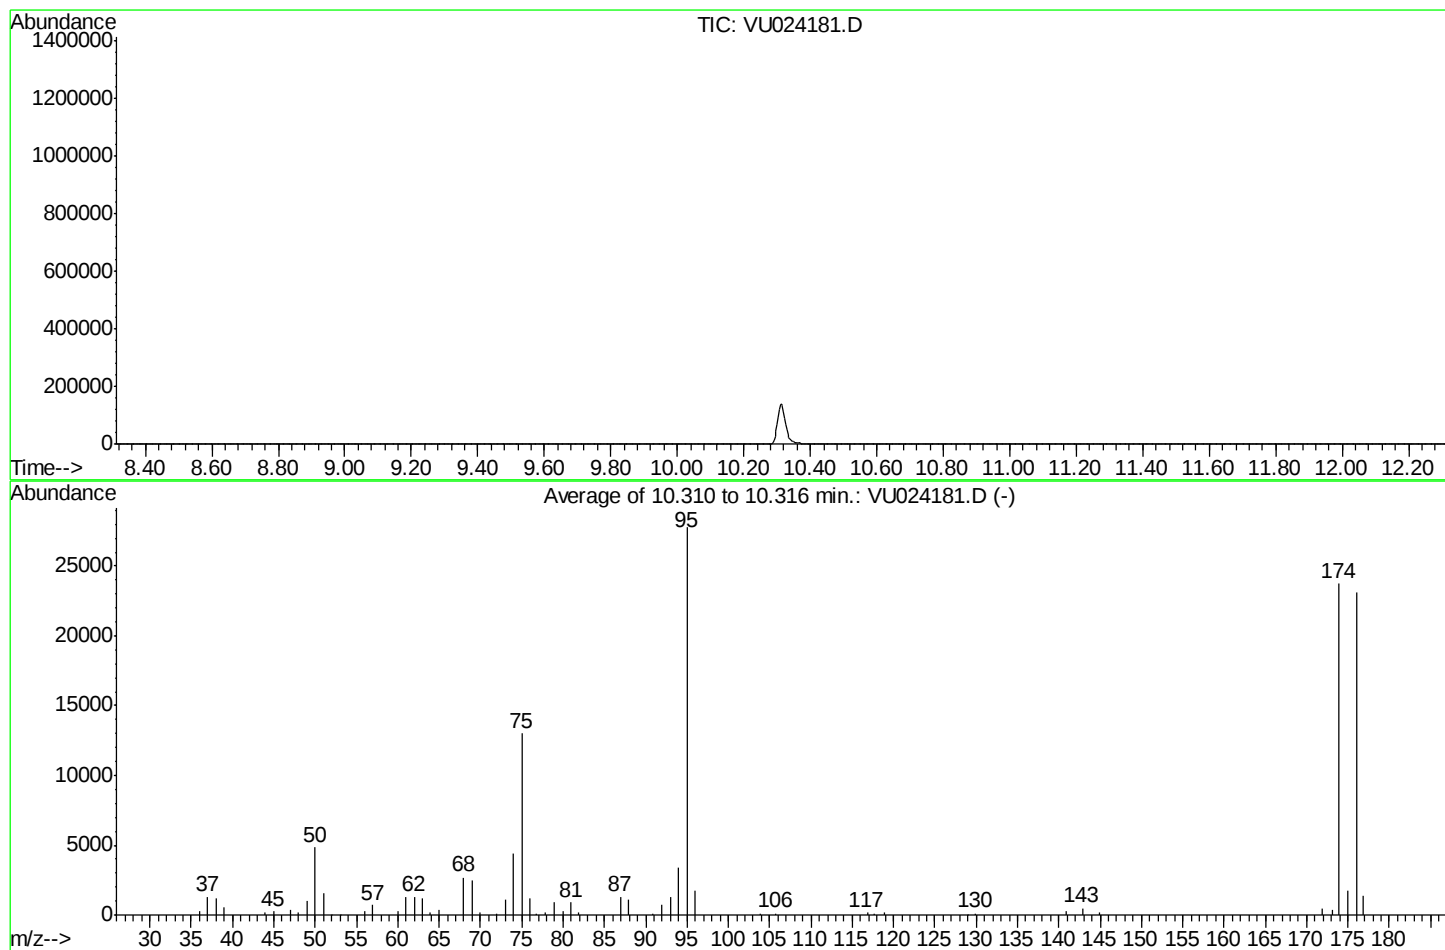

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4853	PASS
75	95	30	80	46.8	13000	PASS
95	95	100	100	100.0	27778	PASS
96	95	5	9	6.2	1722	PASS
173	174	0.00	2	1.4	327	PASS
174	95	50	120	85.4	23717	PASS
175	174	5	9	7.2	1706	PASS
176	174	95	101	97.3	23077	PASS
177	176	5	9	6.0	1390	PASS

Scan 3012 (10.275 min): VU024181.D
BFB60

m/z	Abundance
39.90	114.0
43.90	398.0

Scan 3023 (10.310 min): VU024181.D
BFB60

m/z	Abundance
35.90	246.0
37.00	1323.0
38.00	1343.0
39.00	561.0
39.90	146.0
43.90	519.0
45.00	252.0
47.00	395.0
48.00	190.0
49.00	1062.0
50.00	4882.0
51.00	1565.0
52.00	101.0
56.00	276.0
57.00	737.0
59.90	248.0
61.00	1291.0
62.00	1335.0
63.00	1176.0
63.90	163.0
65.00	344.0
68.00	2683.0
69.00	2519.0
70.00	165.0
71.90	129.0
73.00	1074.0
74.00	4494.0
75.00	13449.0
76.00	1198.0
76.80	175.0
77.80	163.0
78.90	936.0
80.00	238.0
80.90	908.0
81.80	182.0
87.00	1299.0
87.90	1046.0
90.80	107.0
92.00	719.0
93.00	1259.0
94.00	3279.0
95.00	28280.0
96.00	1727.0
103.80	111.0
105.80	130.0
116.90	181.0
117.70	100.0
118.80	148.0
128.90	104.0
129.80	123.0
140.90	255.0
142.90	482.0
144.80	229.0
171.90	432.0
173.10	325.0
173.90	23336.0
175.00	1649.0
176.00	22488.0
176.90	1360.0

m/z	Abundance
36.00	249.0
37.00	1343.0
38.00	1315.0
39.00	583.0
39.90	116.0
44.00	534.0
45.00	248.0
47.00	395.0
48.00	181.0
49.00	1058.0
50.00	4943.0
51.00	1612.0
53.00	105.0
56.00	288.0
57.00	733.0
60.00	262.0
61.00	1271.0
62.00	1356.0
63.00	1264.0
63.90	216.0
65.00	356.0
68.00	2783.0
69.00	2614.0
70.00	180.0
71.90	115.0
73.00	1173.0
74.00	4541.0
75.00	13295.0
76.00	1275.0
76.80	138.0
77.80	174.0
78.90	930.0
80.00	287.0
80.90	902.0
81.80	182.0
87.00	1346.0
87.90	1179.0
90.80	114.0
92.00	721.0
93.00	1273.0
94.00	3496.0
95.00	28592.0
96.00	1747.0
103.80	117.0
105.80	134.0
116.80	182.0
117.70	114.0
118.90	161.0
129.90	120.0
140.90	267.0
142.90	526.0
144.90	236.0
171.90	534.0
173.00	338.0
174.00	24416.0
175.00	1747.0
176.00	23864.0
176.90	1442.0

Scan 3025 (10.316 min): VU024181.D
BFB60

m/z	Abundance
36.00	223.0
37.00	1206.0
38.00	1053.0
39.00	531.0
44.00	575.0
45.00	220.0
47.00	373.0
47.90	135.0
49.00	995.0
50.00	4736.0
51.00	1552.0
55.90	289.0
57.00	625.0
60.00	261.0
61.00	1247.0
62.00	1291.0
63.00	1237.0
63.90	227.0
65.10	316.0
68.00	2649.0
69.00	2386.0
70.00	177.0
71.90	102.0
73.00	1162.0
74.00	4290.0
75.00	12256.0
76.00	1178.0
77.80	166.0
78.90	845.0
80.00	293.0
81.00	853.0
81.90	196.0
86.90	1258.0
87.90	1216.0
90.80	105.0
92.00	655.0
93.00	1223.0
94.00	3314.0
95.00	26464.0
96.00	1693.0
105.80	107.0
116.80	158.0
118.90	154.0
130.00	117.0
140.90	249.0
142.90	469.0
144.90	213.0
171.90	535.0
173.00	320.0
174.00	23400.0
175.00	1723.0
176.00	22880.0
176.90	1368.0