


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU052720\
 Data File : VU038309.D
 Acq On : 27 May 2020 08:56
 Operator : JC/MD
 Sample : BFB01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 28 04:16:01 2020

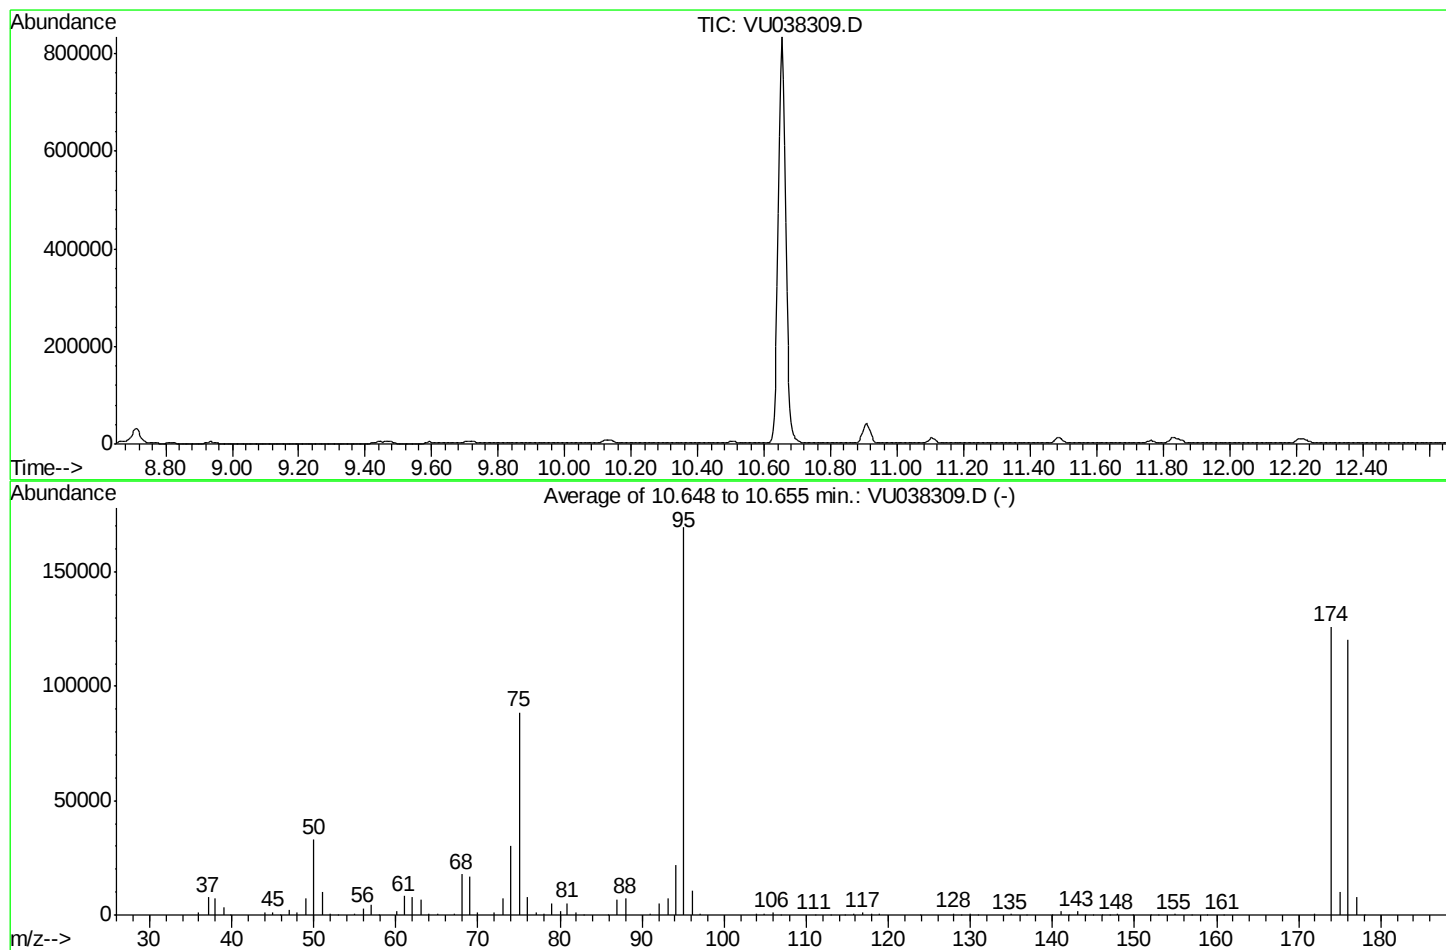

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	32914	PASS
75	95	30	80	52.2	88610	PASS
95	95	100	100	100.0	169600	PASS
96	95	5	9	6.4	10878	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.4	126162	PASS
175	174	5	9	8.0	10050	PASS
176	174	95	101	95.3	120240	PASS
177	176	5	9	6.4	7714	PASS

m/z	Abundance
36.00	1940.0
37.10	7621.0
38.00	7379.0
39.00	2938.0
39.90	302.0
44.00	1847.0
45.00	1368.0
47.00	2071.0
47.90	1001.0
49.00	6974.0
50.00	31456.0
51.00	9804.0
52.00	400.0
53.00	146.0
55.00	417.0
56.00	2583.0
57.00	4632.0
58.10	198.0
60.10	1656.0
61.00	7532.0
62.00	7747.0
63.00	6068.0
64.00	716.0
65.00	567.0
67.10	558.0
68.00	16992.0
69.10	16301.0
70.00	1239.0
72.00	877.0
73.10	7177.0
74.00	29088.0
75.00	85384.0
76.00	7379.0
77.00	1146.0
78.00	849.0
78.90	4813.0
80.00	1517.0
80.90	4833.0
81.90	1197.0
85.90	177.0
87.00	6431.0
88.00	6899.0
91.00	564.0
92.00	4513.0
93.10	7071.0
94.10	20688.0
95.10	159872.0
96.10	10235.0
97.10	383.0
104.00	645.0
104.90	351.0
105.90	831.0
106.90	190.0
111.00	154.0
113.00	170.0
114.70	118.0
115.90	438.0
116.90	931.0
117.90	590.0
119.00	721.0
128.00	707.0
129.00	310.0
129.90	606.0
130.90	298.0
134.90	288.0
136.90	238.0
139.90	116.0
141.00	1479.0
141.90	182.0
143.00	1584.0
144.10	140.0
144.90	177.0
146.00	124.0
146.90	110.0
147.90	323.0
151.90	100.0
152.90	117.0
154.90	532.0
156.90	202.0
158.80	132.0
160.80	187.0
172.00	676.0
174.00	115384.0
175.10	9431.0
176.00	109840.0
177.10	7379.0
178.00	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	2064.0
37.10	8062.0
38.00	7841.0
39.00	3265.0
39.80	348.0
44.00	1840.0
45.00	1344.0
45.90	101.0
47.00	2441.0
48.00	1074.0
49.00	7694.0
50.00	34008.0
51.00	10779.0
52.10	370.0
53.00	151.0
55.00	436.0
56.00	3006.0
57.00	4748.0
57.90	259.0
60.10	1774.0
61.00	8511.0
62.00	8241.0
63.00	6941.0
64.00	866.0
65.10	606.0
67.00	585.0
68.00	18472.0
69.00	17552.0
70.00	1435.0
72.00	1067.0
73.00	7615.0
74.00	31520.0
75.00	90928.0
76.00	7896.0
77.10	1089.0
78.00	864.0
78.90	5116.0
80.00	1718.0
80.90	5260.0
81.90	1279.0
82.90	161.0
85.90	208.0
87.00	7023.0
88.00	7447.0
90.90	617.0
92.00	5022.0
93.10	7529.0
94.10	22496.0
95.10	174848.0
96.10	11140.0
97.10	384.0
104.00	777.0
104.90	345.0
105.90	959.0
106.90	201.0
111.10	168.0
113.00	132.0
114.80	101.0
115.80	520.0
116.90	1144.0
117.90	614.0
118.90	787.0
128.00	690.0
129.00	296.0
130.00	663.0
130.90	312.0
134.90	367.0
136.90	251.0
139.90	122.0
141.00	1625.0
142.00	177.0
143.00	1729.0
144.00	157.0
145.00	178.0
146.00	131.0
147.00	130.0
147.90	327.0
151.90	136.0
154.90	530.0
156.90	302.0
158.90	140.0
160.80	254.0
172.00	646.0
174.00	130432.0
175.00	10371.0
176.00	124464.0
177.10	7891.0
178.00	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	2134.0
37.10	7734.0
38.00	7710.0
39.00	3180.0
39.90	393.0
44.00	1856.0
45.00	1355.0
47.00	2505.0
48.00	985.0
49.00	7539.0
50.00	33280.0
51.00	10533.0
52.00	325.0
52.90	120.0
55.00	415.0
56.00	2942.0
57.00	4673.0
57.90	270.0
60.10	1694.0
61.00	8880.0
62.00	8093.0
63.00	7070.0
64.10	848.0
65.10	631.0
67.00	567.0
68.00	18080.0
69.00	17216.0
70.00	1382.0
72.00	1070.0
73.00	7492.0
74.00	30896.0
75.00	89520.0
76.00	7638.0
77.00	1142.0
78.00	837.0
78.90	5095.0
80.00	1602.0
80.90	5290.0
81.90	1226.0
83.00	220.0
85.90	196.0
87.00	6741.0
88.00	7264.0
90.90	688.0
92.00	5088.0
93.10	7454.0
94.10	21928.0
95.10	174080.0
96.10	11261.0
97.00	310.0
104.00	813.0
104.90	306.0
105.90	877.0
106.80	145.0
111.10	132.0
115.80	585.0
116.90	1192.0
117.90	618.0
118.90	874.0
123.90	101.0
128.00	627.0
128.90	243.0
130.00	571.0
130.90	272.0
134.90	382.0
136.90	226.0
139.90	156.0
141.00	1645.0
142.00	182.0
143.00	1685.0
144.00	167.0
145.10	189.0
146.00	178.0
147.00	140.0
147.90	341.0
149.80	129.0
151.90	123.0
154.90	479.0
156.90	355.0
158.80	160.0
160.90	261.0
172.00	716.0
174.00	132672.0
175.00	10348.0
176.00	126416.0
177.10	7874.0
178.00	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Scan 2881 (10.603 min): VU038309.D
BFB01

m/z	Abundance
35.90	891.0
37.90	351.0
39.90	301.0
44.10	716.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01