

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052722\
 Data File : VU048685.D
 Acq On : 27 May 2022 11:56
 Operator : SY/MD
 Sample : N3064-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TRIP-BLANK

Quant Time: May 28 00:16:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 27 06:42:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.375	168	197210	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.250	114	329140	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	341391	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	193663	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	148399	50.106	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 100.220%			
35) Dibromofluoromethane	5.292	113	126585	53.908	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 107.820%			
50) Toluene-d8	7.899	98	370681	44.038	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 88.080%#			
62) 4-Bromofluorobenzene	10.632	95	167589	52.645	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 105.300%			
Target Compounds						Qvalue
3) Chloromethane	1.520	50	596	0.205	ug/l #	71
5) Bromomethane	1.790	94	54	Below Cal	#	3
6) Chloroethane	1.941	64	42	Below Cal	#	43
11) Tert butyl alcohol	3.182	59	1494	1.990	ug/l #	28
13) Acrolein	2.498	56	43	Below Cal	#	1
16) Acetone	2.649	43	4820	3.193	ug/l #	87
17) Carbon Disulfide	2.797	76	1395	0.238	ug/l #	88
20) Methylene Chloride	3.047	84	1084	0.422	ug/l #	79
29) Tetrahydrofuran	5.076	42	1085	0.794	ug/l #	54
31) Cyclohexane	5.375	56	4203	1.126	ug/l #	1
36) 1,1-Dichloropropene	5.372	75	15585	4.548	ug/l #	50
38) Carbon Tetrachloride	5.372	117	20647	5.251	ug/l #	17
49) 1,4-Dioxane	7.012	88	134	2.123	ug/l #	24
51) 4-Methyl-2-Pentanone	7.796	43	4134	1.012	ug/l	94
56) Ethyl methacrylate	8.349	69	407	2.705	ug/l #	76
59) 2-Hexanone	8.693	43	5223	1.558	ug/l	93
64) Tetrachloroethene	8.549	164	295	Below Cal	#	66
74) N-amyl acetate	10.327	43	1662	2.717	ug/l #	70
76) 1,2,3-Trichloropropane	10.632	75	86958	13.926	ug/l #	48
81) trans-1,4-Dichloro-2-b...	10.632	75	86958	50.565	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.475	105	1867	1.342	ug/l	79
87) 1,3-Dichlorobenzene	11.748	146	1855	0.282	ug/l	89
88) 1,4-Dichlorobenzene	11.748	146	1855	0.273	ug/l	88
89) n-Butylbenzene	12.217	91	4879	2.601	ug/l	96
91) 1,2-Dichlorobenzene	12.217	146	1746	0.263	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	12.999	75	462	0.314	ug/l	87
93) 1,2,4-Trichlorobenzene	13.841	180	3492	0.800	ug/l	95
94) Hexachlorobutadiene	14.024	225	945	0.452	ug/l	93
95) Naphthalene	14.092	128	25019	4.091	ug/l	98
96) 1,2,3-Trichlorobenzene	14.330	180	4159	0.962	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052722\
Data File : VU048685.D
Acq On : 27 May 2022 11:56
Operator : SY/MD
Sample : N3064-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK

Quant Time: May 28 00:16:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260
QLast Update : Fri May 27 06:42:31 2022
Response via : Initial Calibration




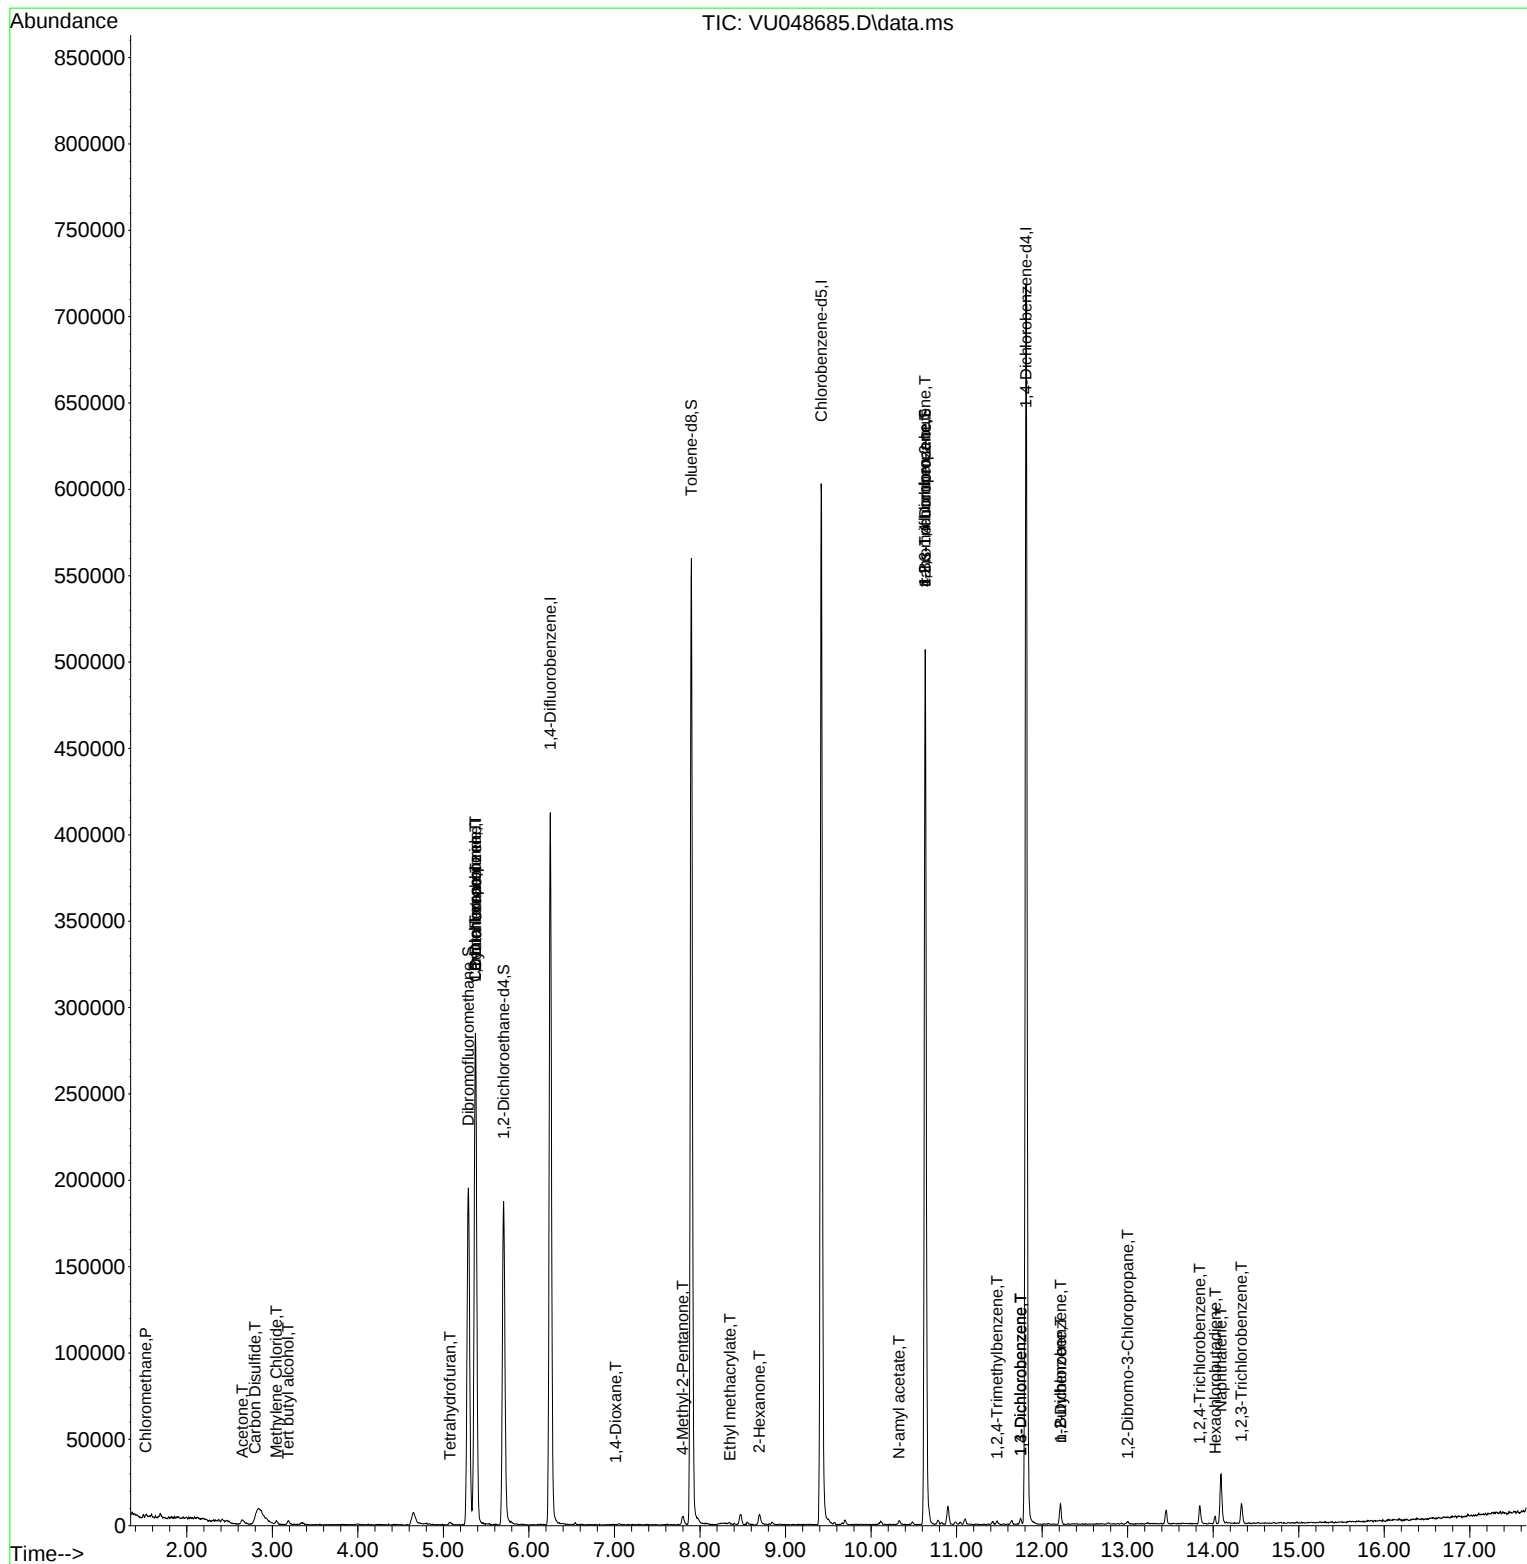




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 197210
Ion Ratio Lower Upper
168 100
99 60.1 49.3 73.9

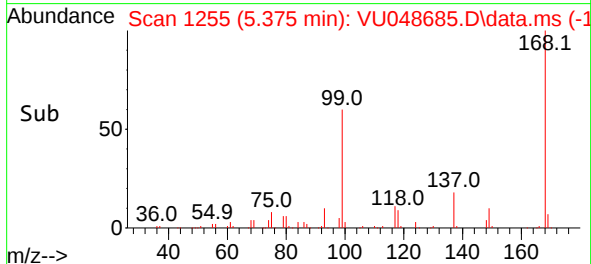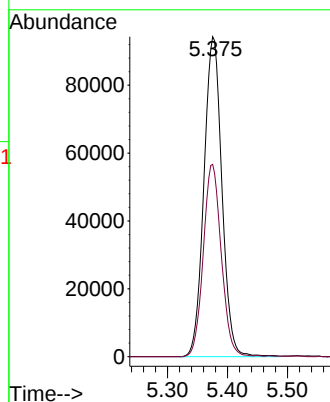

#3
Chloromethane
Concen: 0.205 ug/l
RT: 1.520 min Scan# 56
Delta R.T. -0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 50 Resp: 596
Ion Ratio Lower Upper
50 100
52 48.6 25.7 38.5#


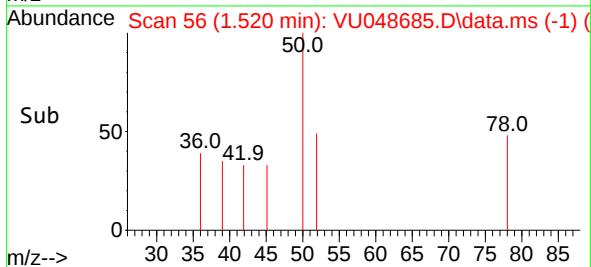
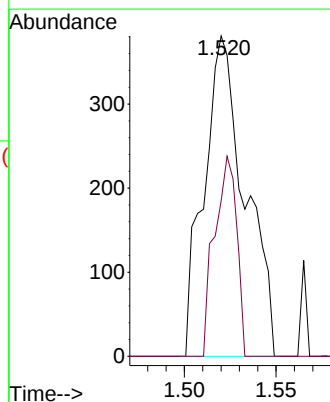
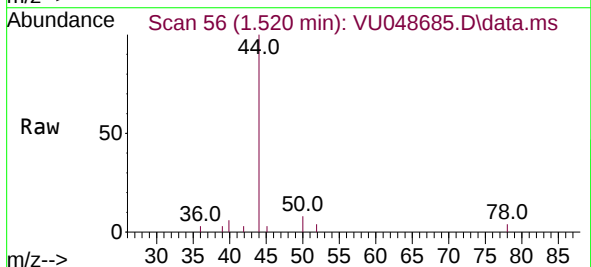




#5
Bromomethane
Concen: Below Cal
RT: 1.790 min Scan# 14
Delta R.T. -0.061 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK

Tgt Ion: 94 Resp: 54
Ion Ratio Lower Upper
94 100
96 0.0 75.1 112.7#

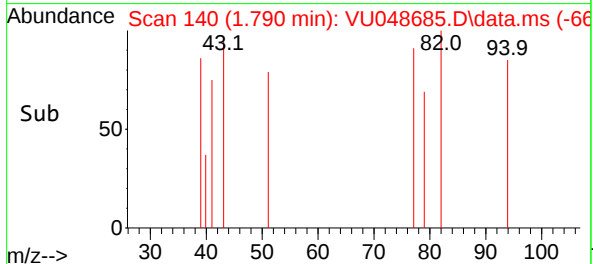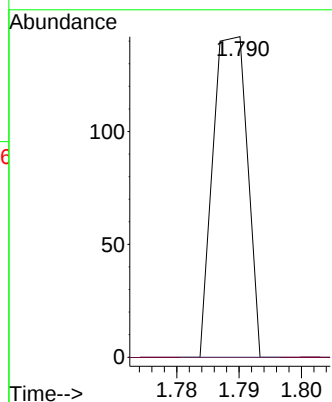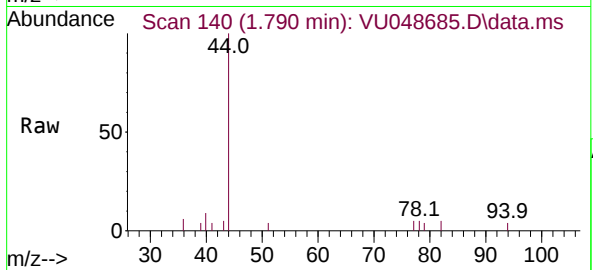

#6
Chloroethane
Concen: Below Cal
RT: 1.941 min Scan# 187
Delta R.T. 0.009 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 64 Resp: 42
Ion Ratio Lower Upper
64 100
66 0.0 25.2 37.8#


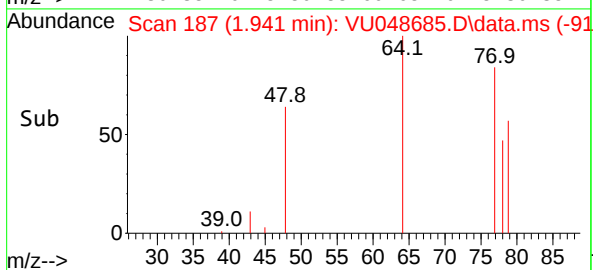
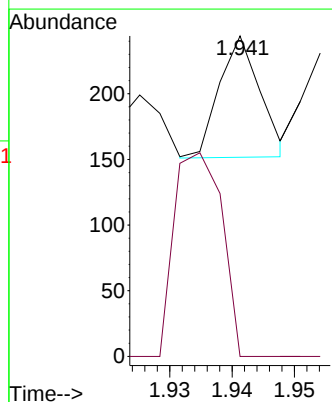
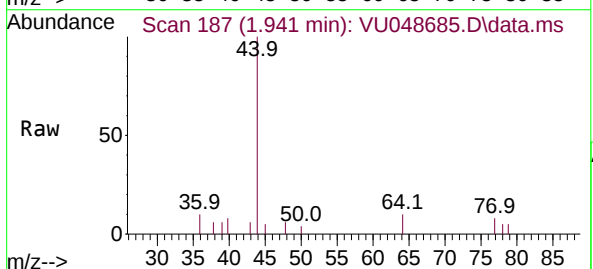




#11
Tert butyl alcohol
Concen: 1.990 ug/l
RT: 3.182 min Scan# 51
Delta R.T. -0.007 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion: 59 Resp: 1494
Ion Ratio Lower Upper
59 100
57 0.0 39.7 59.5#

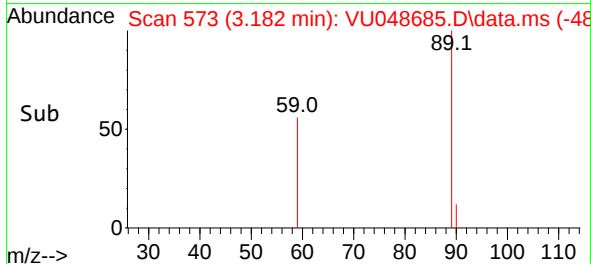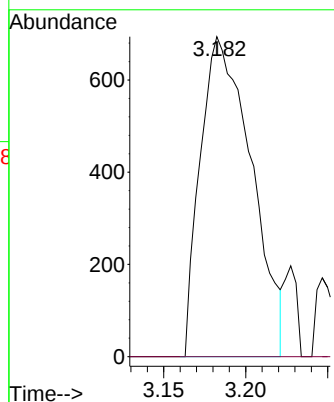

#13
Acrolein
Concen: Below Cal
RT: 2.498 min Scan# 360
Delta R.T. 0.010 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 56 Resp: 43
Ion Ratio Lower Upper
56 100
55 390.7 57.7 86.5#

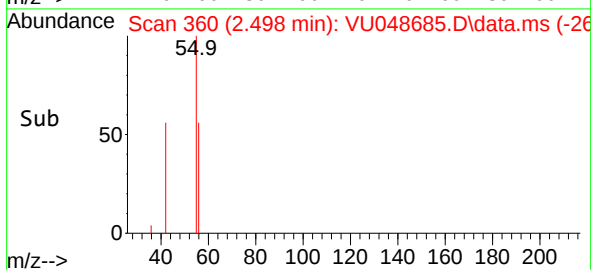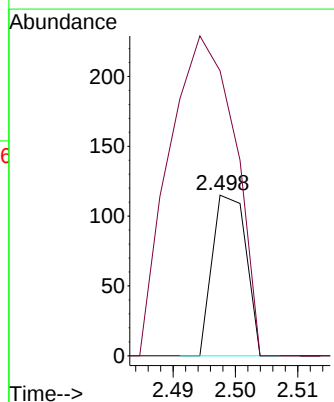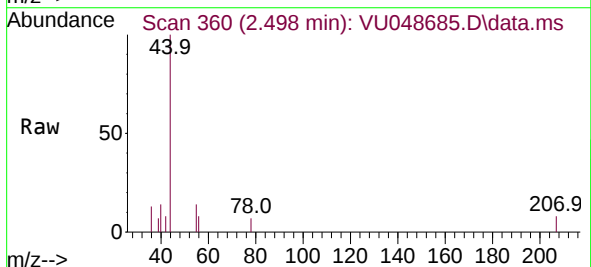

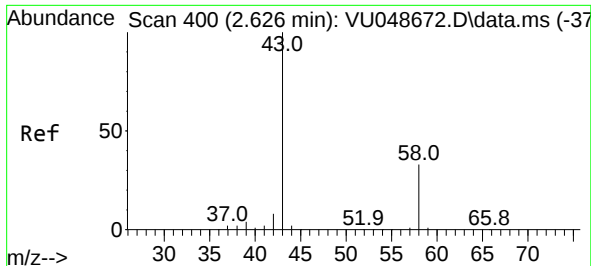

#16

Acetone

Concen: 3.193 ug/l

RT: 2.649 min Scan# 400

Delta R.T. 0.022 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :





TRIP-BLANK

Tgt Ion: 43 Resp: 4820

Ion Ratio Lower Upper

43 100

58 25.6 26.3 39.5#

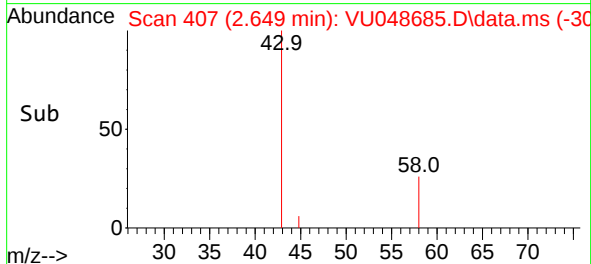

#17

Carbon Disulfide

Concen: 0.238 ug/l

RT: 2.797 min Scan# 453

Delta R.T. 0.003 min

Lab File: VU048685.D




Acq: 27 May 2022 11:56


Tgt Ion: 76 Resp: 1395

Ion Ratio Lower Upper

76 100

78 13.6 7.3 10.9#


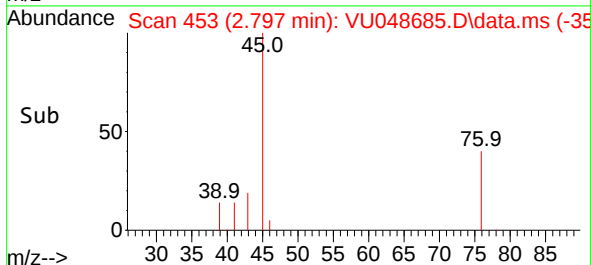

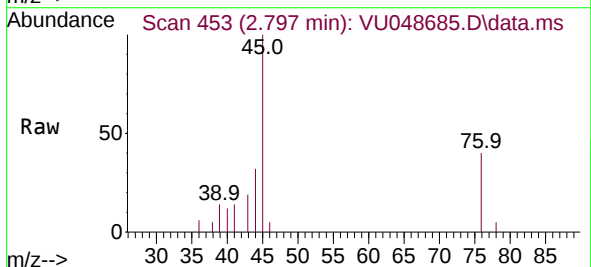


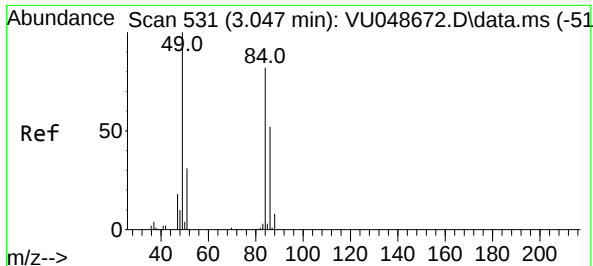

#20
Methylene Chloride
Concen: 0.422 ug/l
RT: 3.047 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:	84	Resp:	1084
Ion	Ratio	Lower	Upper
84	100		
49	98.1	97.0	145.4
51	29.4	29.8	44.8#
86	42.0	50.9	76.3#

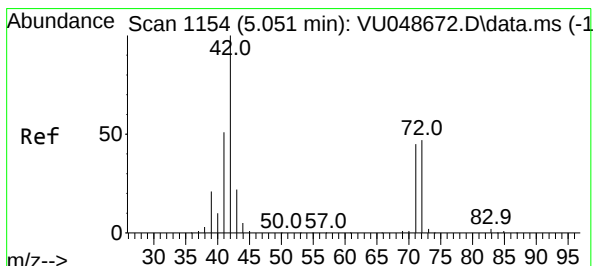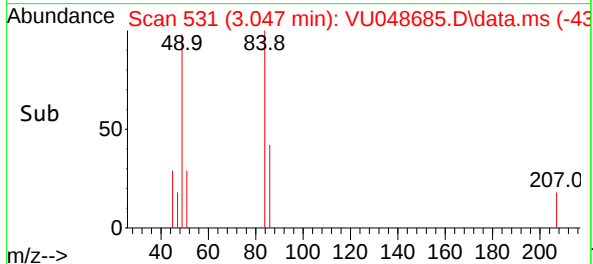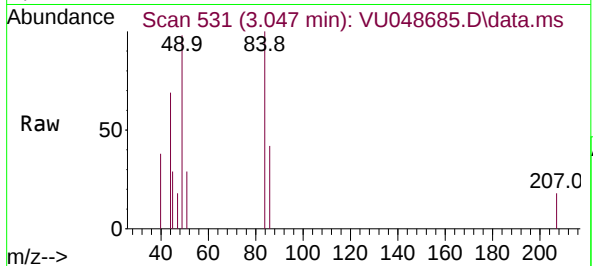

#29
Tetrahydrofuran
Concen: 0.794 ug/l
RT: 5.076 min Scan# 1162
Delta R.T. 0.026 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion:	42	Resp:	1085
Ion	Ratio	Lower	Upper
42	100		
72	8.9	37.6	56.4#
71	21.4	35.0	52.4#


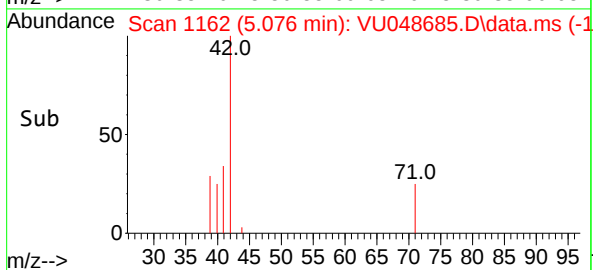

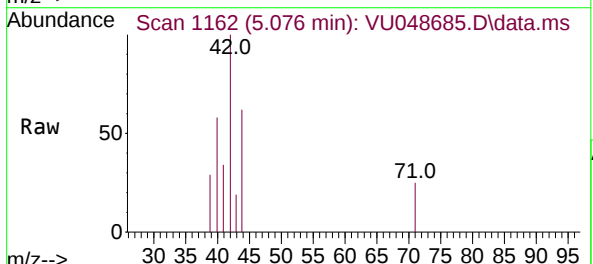


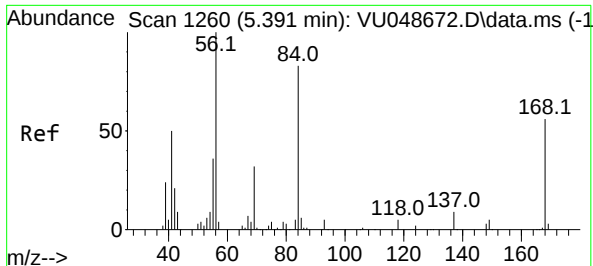

#31
Cyclohexane
Concen: 1.126 ug/l
RT: 5.375 min Scan# 11
Delta R.T. -0.016 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion: 56 Resp: 4203
Ion Ratio Lower Upper
56 100
69 169.8 25.6 38.4#
84 136.4 66.2 99.4#

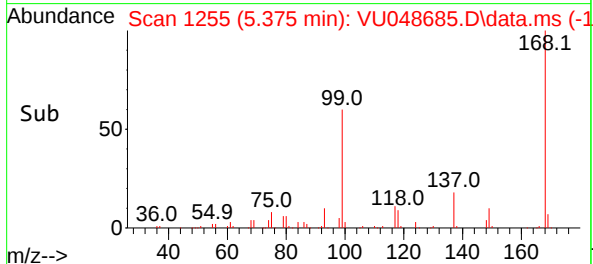

#33
1,2-Dichloroethane-d4
Concen: 50.106 ug/l
RT: 5.703 min Scan# 1357
Delta R.T. 0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 65 Resp: 148399
Ion Ratio Lower Upper
65 100
67 52.0 0.0 103.0

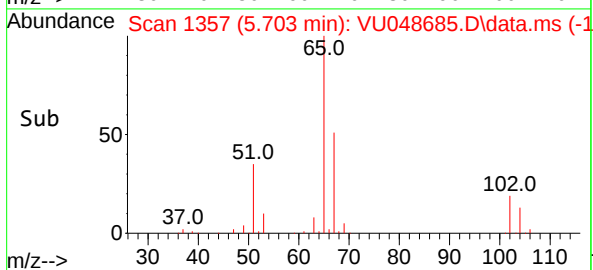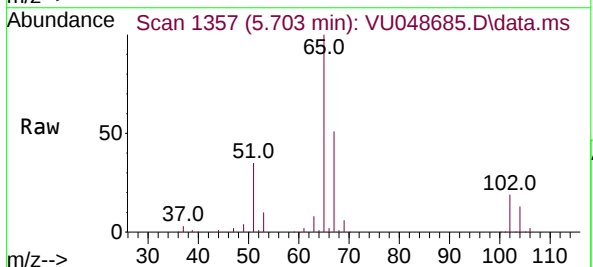

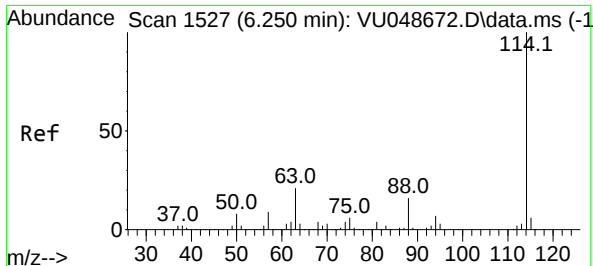

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :

TRIP-BLANK





Tgt Ion:114 Resp: 329140

Ion Ratio Lower Upper

114 100

63 21.2 0.0 42.6

88 16.2 0.0 32.2

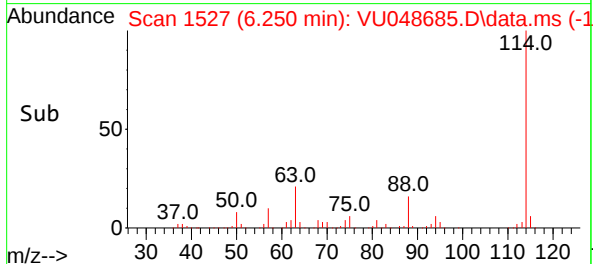

#35

Dibromofluoromethane

Concen: 53.908 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. -0.000 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56




Tgt Ion:113 Resp: 126585


Ion Ratio Lower Upper

113 100

111 104.4 80.7 121.1

192 19.8 15.9 23.9

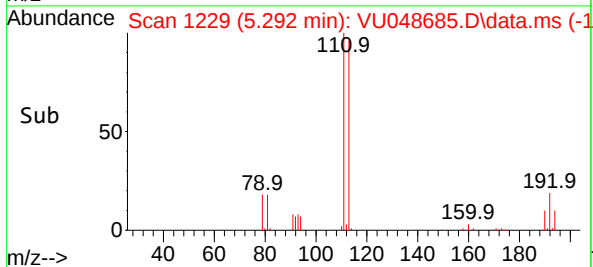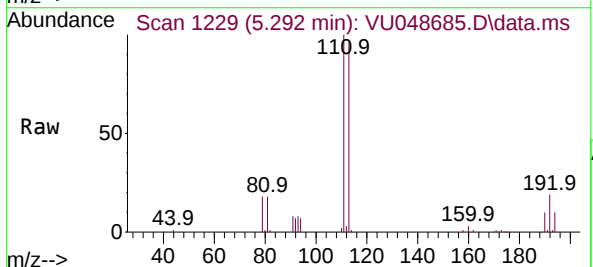

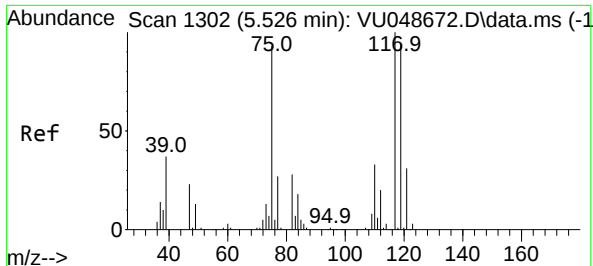

#36

1,1-Dichloropropene

Concen: 4.548 ug/l

RT: 5.372 min Scan# 11

Delta R.T. -0.154 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :

TRIP-BLANK





Tgt Ion: 75 Resp: 15585

Ion Ratio Lower Upper

75 100

110 9.0 17.4 52.3#

77 0.0 24.8 37.2#

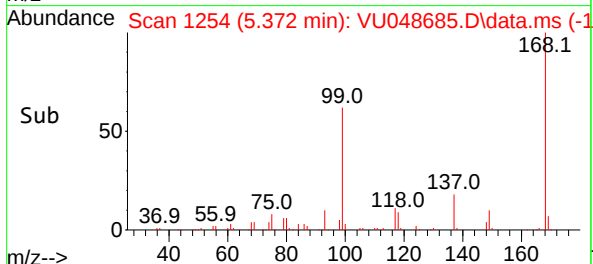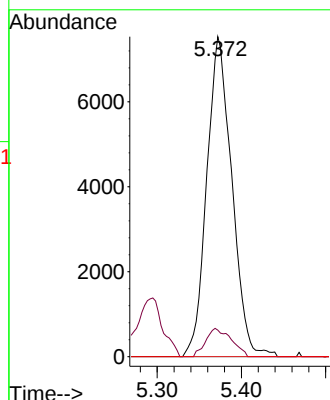

#38

Carbon Tetrachloride

Concen: 5.251 ug/l

RT: 5.372 min Scan# 1254

Delta R.T. -0.154 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56




Tgt Ion:117 Resp: 20647


Ion Ratio Lower Upper

117 100

119 6.1 75.4 113.2#

121 0.0 24.6 36.8#

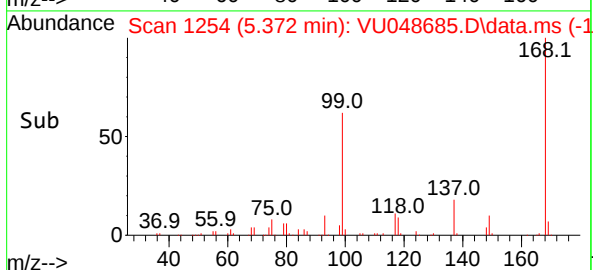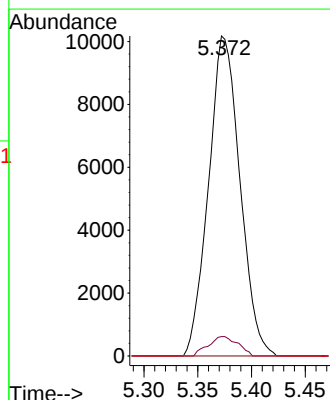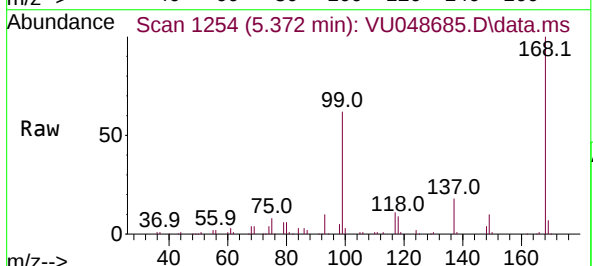

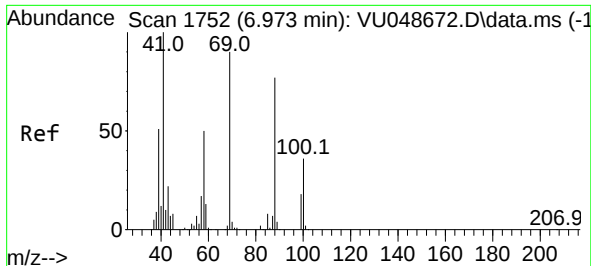

#49

1,4-Dioxane

Concen: 2.123 ug/l

RT: 7.012 min Scan# 1

Delta R.T. 0.038 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :

TRIP-BLANK





Tgt Ion: 88 Resp: 134

Ion Ratio Lower Upper

88 100

43 0.0 24.6 36.8#

58 0.0 54.7 82.1#

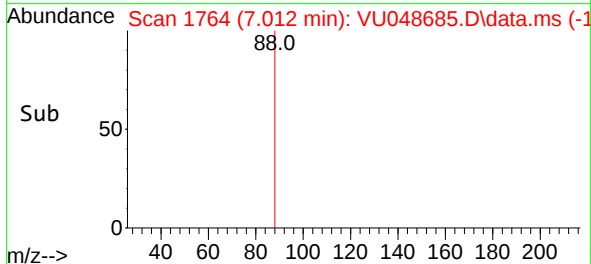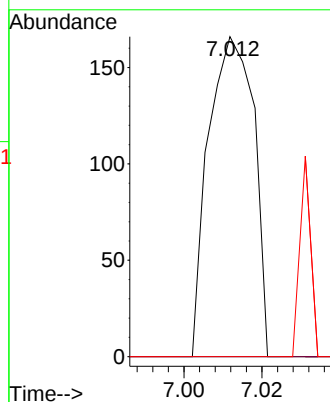

#50

Toluene-d8

Concen: 44.038 ug/l

RT: 7.899 min Scan# 2040

Delta R.T. -0.000 min

Lab File: VU048685.D




Acq: 27 May 2022 11:56


Tgt Ion: 98 Resp: 370681

Ion Ratio Lower Upper

98 100

100 65.8 52.2 78.4

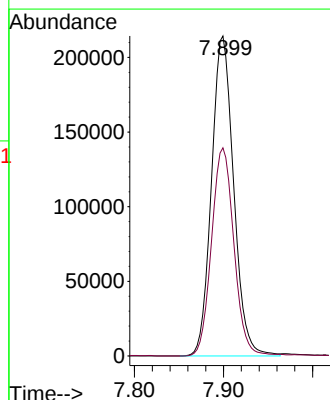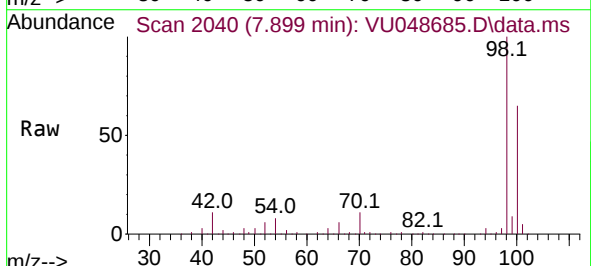

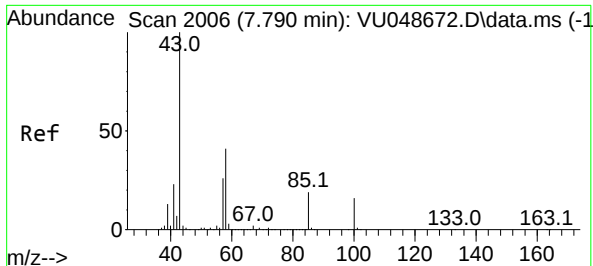

#51

4-Methyl-2-Pentanone

Concen: 1.012 ug/l

RT: 7.796 min Scan# 2006

Delta R.T. 0.006 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :





TRIP-BLANK

Tgt Ion: 43 Resp: 4134

Ion Ratio Lower Upper

43 100

58 37.2 32.7 49.1

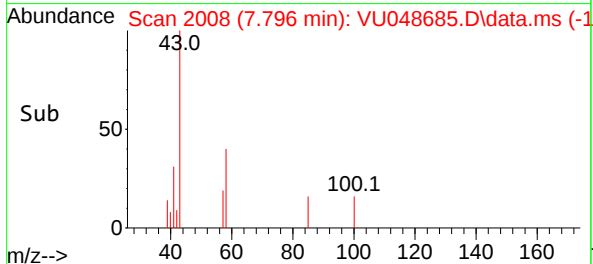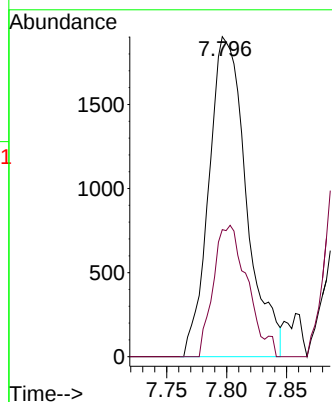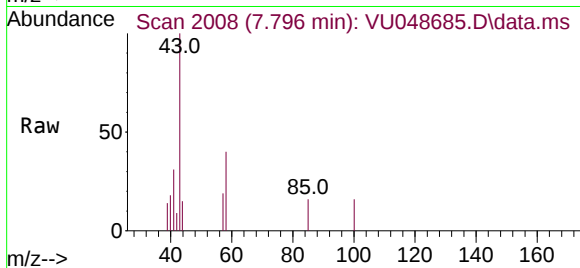

#56

Ethyl methacrylate

Concen: 2.705 ug/l

RT: 8.349 min Scan# 2180

Delta R.T. 0.016 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56




Tgt Ion: 69 Resp: 407


Ion Ratio Lower Upper

69 100

41 82.3 50.6 76.0#

39 45.7 26.6 40.0#

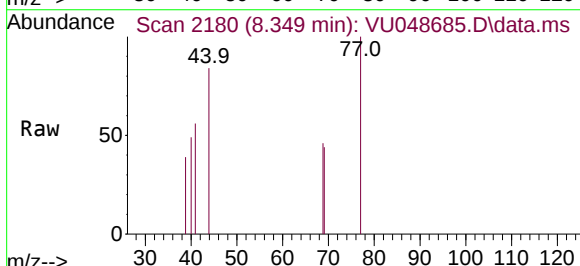

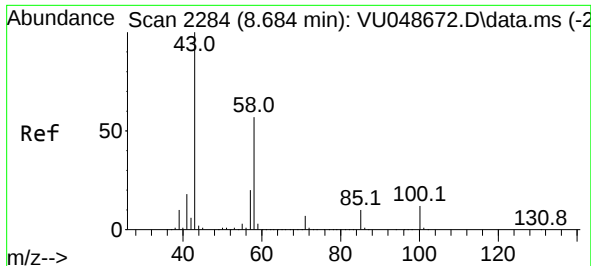

#59

2-Hexanone

Concen: 1.558 ug/l

RT: 8.693 min Scan# 21

Delta R.T. 0.010 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56

Instrument :

MSVOA_U

ClientSampleId :





TRIP-BLANK

Tgt Ion: 43 Resp: 5223

Ion Ratio Lower Upper

43 100

58 51.6 28.2 84.6

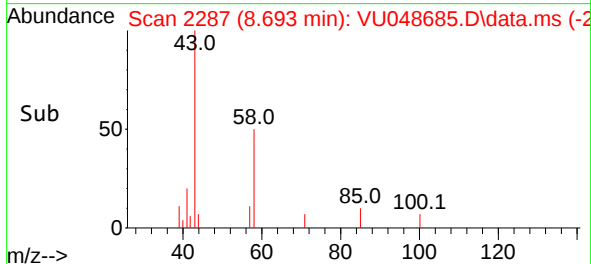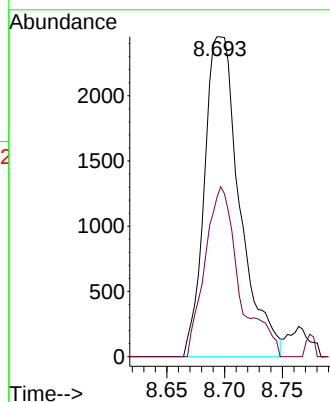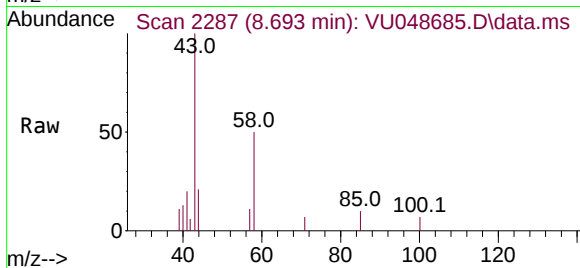

#62

4-Bromofluorobenzene

Concen: 52.645 ug/l

RT: 10.632 min Scan# 2890

Delta R.T. -0.000 min

Lab File: VU048685.D

Acq: 27 May 2022 11:56




Tgt Ion: 95 Resp: 167589


Ion Ratio Lower Upper

95 100

174 83.5 0.0 159.4

176 78.4 0.0 152.4


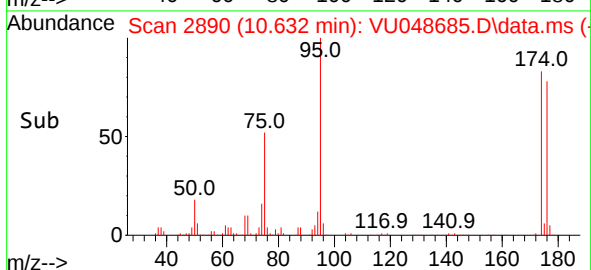
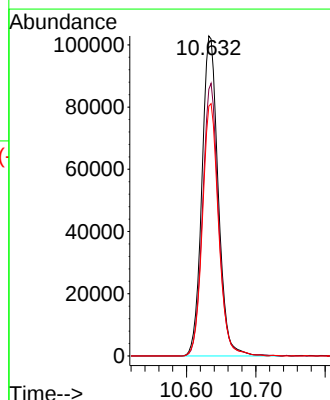
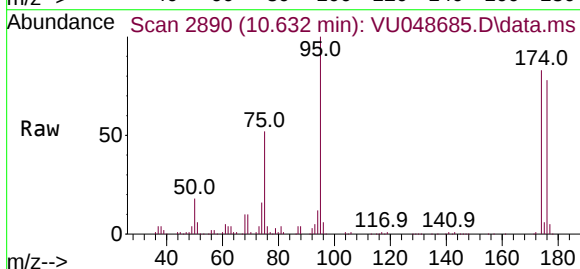


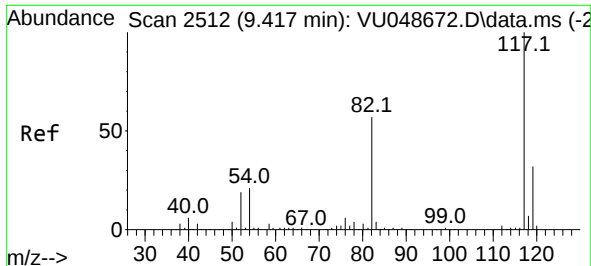

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:117 Resp: 341391
Ion Ratio Lower Upper
117 100
82 56.0 45.3 67.9
119 31.4 25.4 38.2

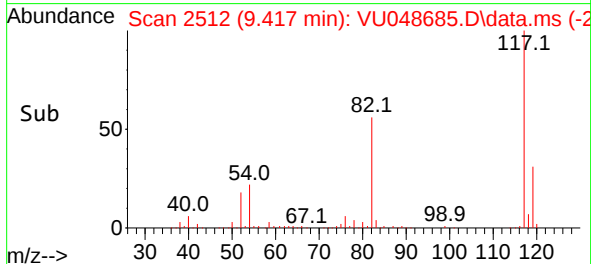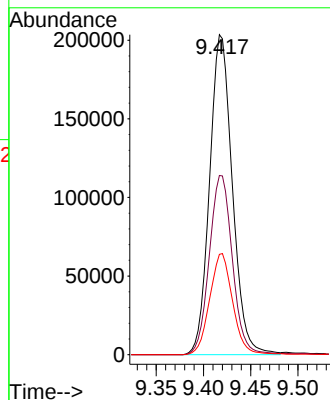

#64
Tetrachloroethene
Concen: Below Cal
RT: 8.549 min Scan# 2242
Delta R.T. -0.006 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion:164 Resp: 295
Ion Ratio Lower Upper
164 100
166 94.0 105.0 157.4#
129 51.8 76.5 114.7#
131 69.0 73.8 110.6#


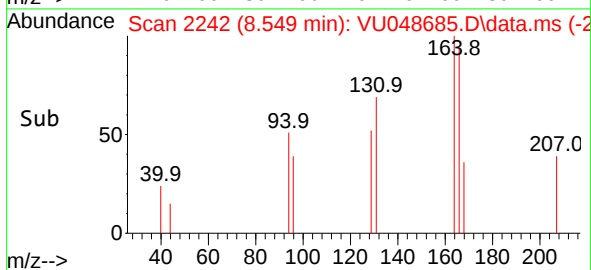
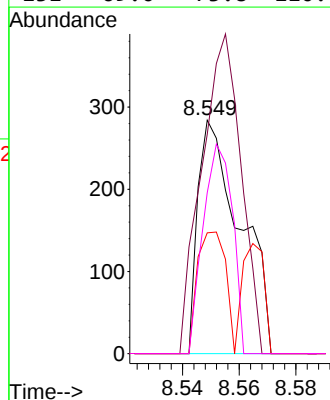
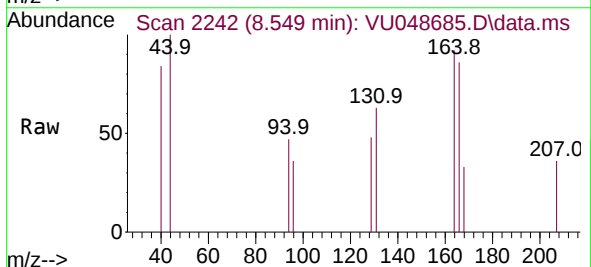


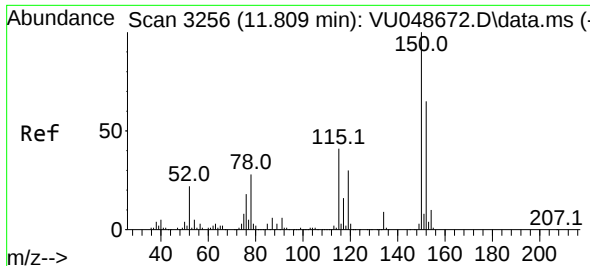

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:152 Resp: 193663
Ion Ratio Lower Upper
152 100
115 59.2 41.8 125.4
150 155.9 0.0 341.0

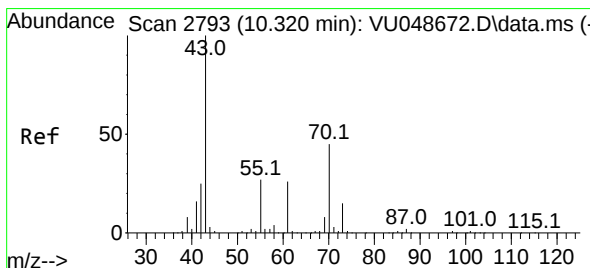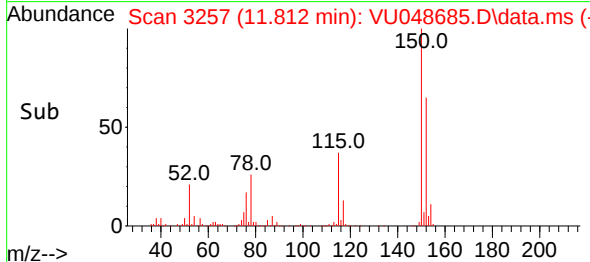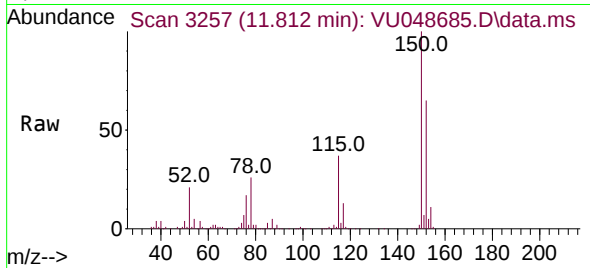

#74
N-ethyl acetate
Concen: 2.717 ug/l
RT: 10.327 min Scan# 2795
Delta R.T. 0.007 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 43 Resp: 1662
Ion Ratio Lower Upper
43 100
70 29.4 35.8 53.6#
55 0.0 21.1 31.7#
61 16.1 20.2 30.4#


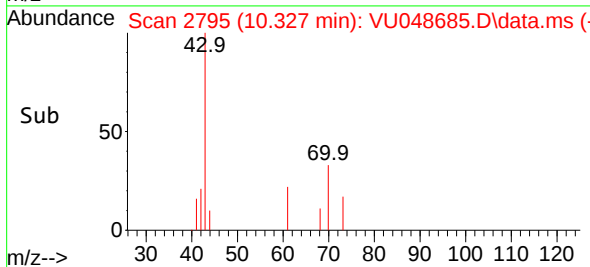

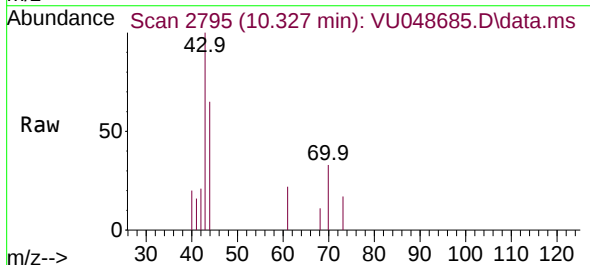


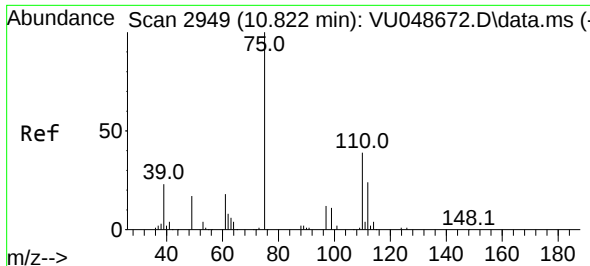

#76
1,2,3-Trichloropropane
Concen: 13.926 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.190 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion: 75 Resp: 86958
Ion Ratio Lower Upper
75 100
77 1.3 14.8 44.3#

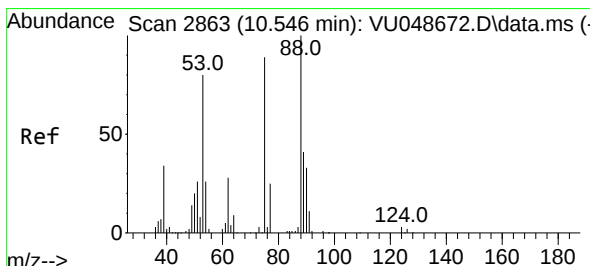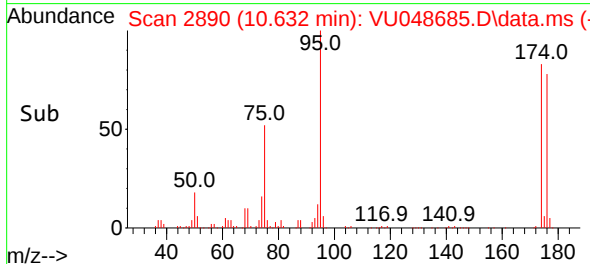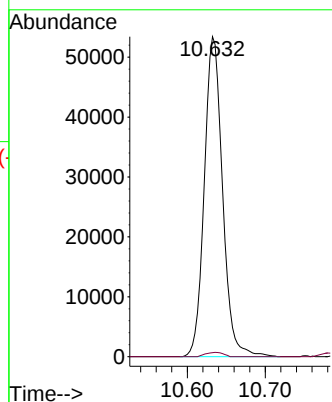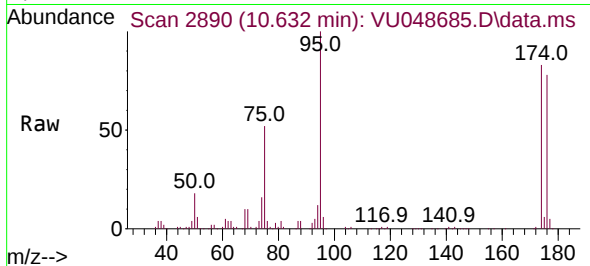

#81
trans-1,4-Dichloro-2-butene
Concen: 50.565 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.087 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 75 Resp: 86958
Ion Ratio Lower Upper
75 100
53 0.1 72.5 108.7#
89 0.0 37.0 55.4#


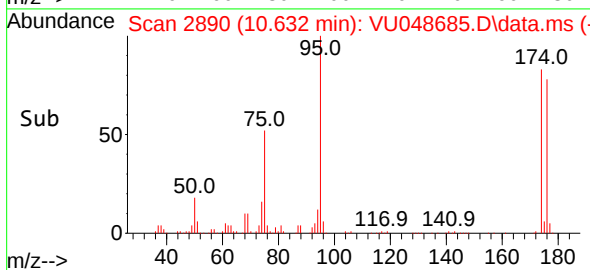

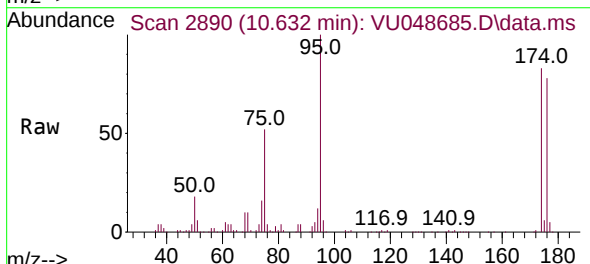


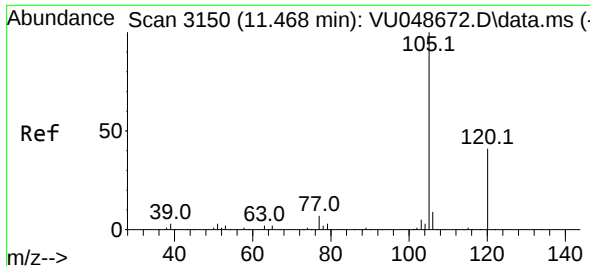

#84
1,2,4-Trimethylbenzene
Concen: 1.342 ug/l
RT: 11.475 min Scan# 3150
Delta R.T. 0.007 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:105 Resp: 1867
Ion Ratio Lower Upper
105 100
120 31.4 22.5 67.5

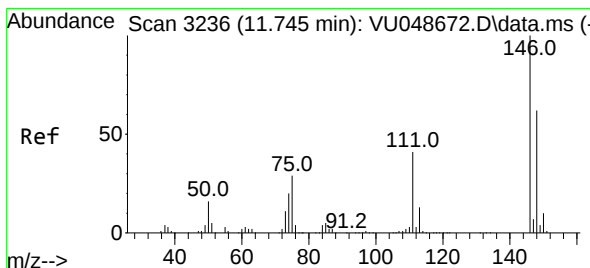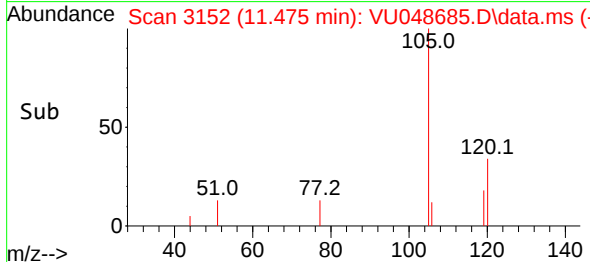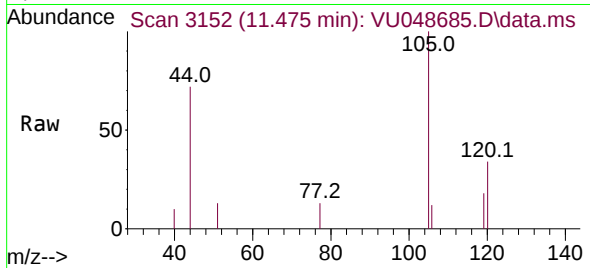

#87
1,3-Dichlorobenzene
Concen: 0.282 ug/l
RT: 11.748 min Scan# 3237
Delta R.T. 0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion:146 Resp: 1855
Ion Ratio Lower Upper
146 100
111 27.9 20.6 61.9
148 59.5 31.6 95.0


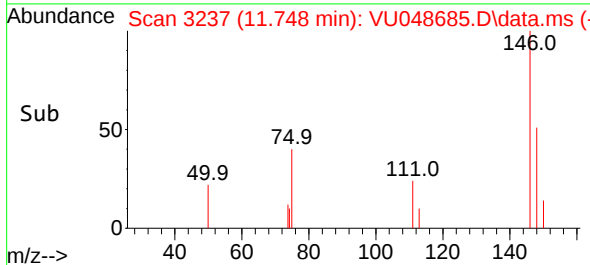

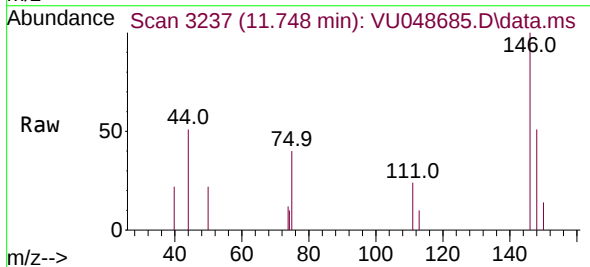


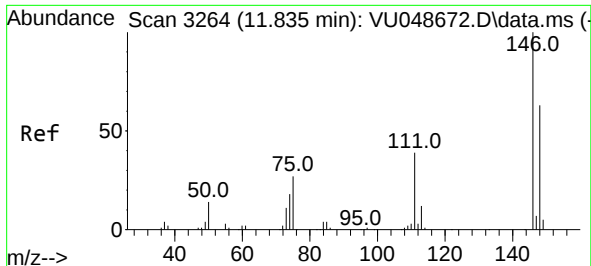

#88
1,4-Dichlorobenzene
Concen: 0.273 ug/l
RT: 11.748 min Scan# 31
Delta R.T. -0.087 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:146 Resp: 1855
Ion Ratio Lower Upper
146 100
111 27.9 20.2 60.6
148 59.5 32.4 97.0

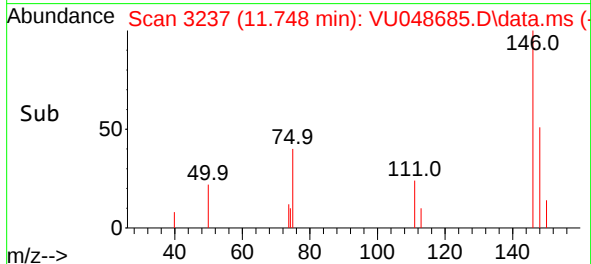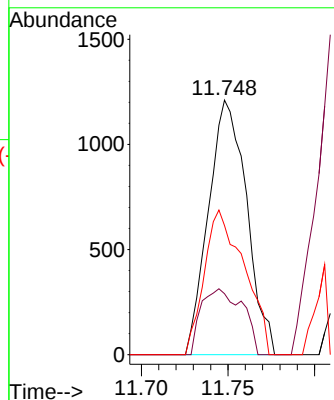

#89
n-Butylbenzene
Concen: 2.601 ug/l
RT: 12.217 min Scan# 3383
Delta R.T. 0.009 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion: 91 Resp: 4879
Ion Ratio Lower Upper
91 100
92 49.5 25.9 77.8
134 21.8 12.5 37.5


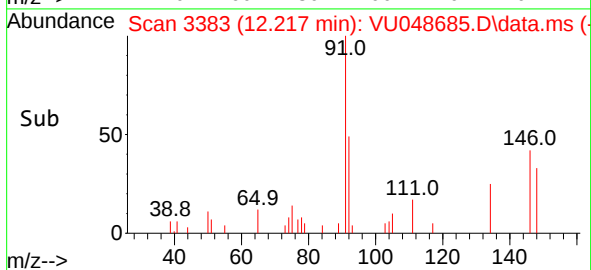
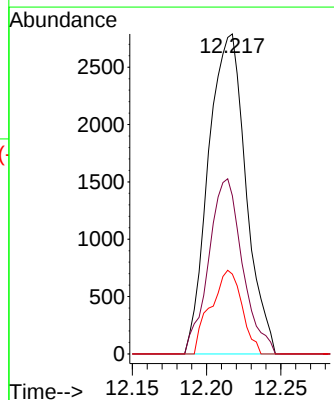
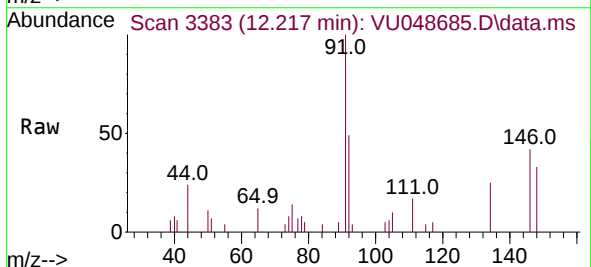




#91
 1,2-Dichlorobenzene
 Concen: 0.263 ug/l
 RT: 12.217 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VU048685.D
 Acq: 27 May 2022 11:56




Instrument :
 MSVOA_U
 ClientSampleId :
 TRIP-BLANK


Tgt Ion:146 Resp: 1746
 Ion Ratio Lower Upper
 146 100
 111 41.5 21.4 64.3
 148 66.2 32.0 96.2

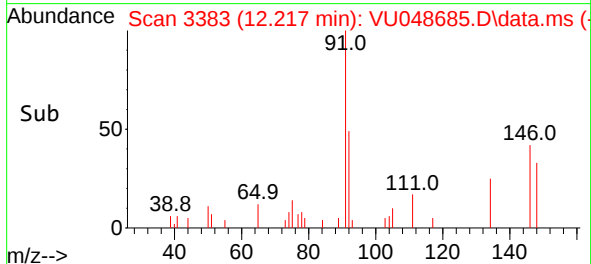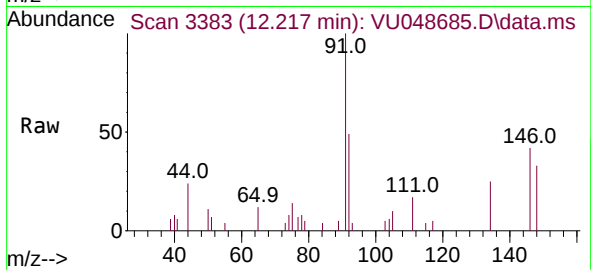

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.314 ug/l
 RT: 12.999 min Scan# 3626
 Delta R.T. 0.003 min
 Lab File: VU048685.D
 Acq: 27 May 2022 11:56

Tgt Ion: 75 Resp: 462
 Ion Ratio Lower Upper
 75 100
 155 56.1 40.3 120.8
 157 100.6 50.0 150.0


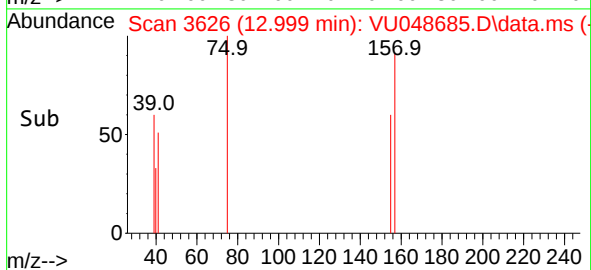

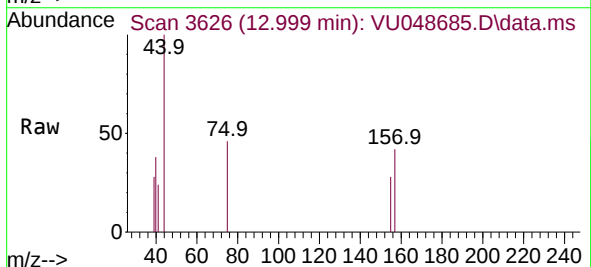




#93
1,2,4-Trichlorobenzene
Concen: 0.800 ug/l
RT: 13.841 min Scan# 3888
Delta R.T. 0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:180 Resp: 3492
Ion Ratio Lower Upper
180 100
182 103.0 48.3 144.9
145 31.3 15.6 46.7

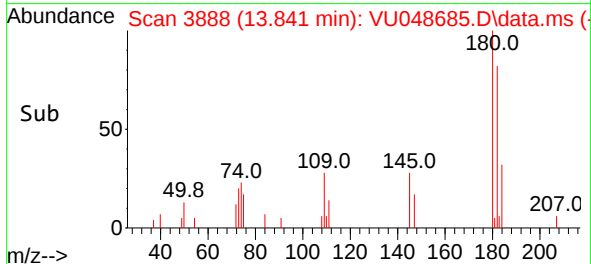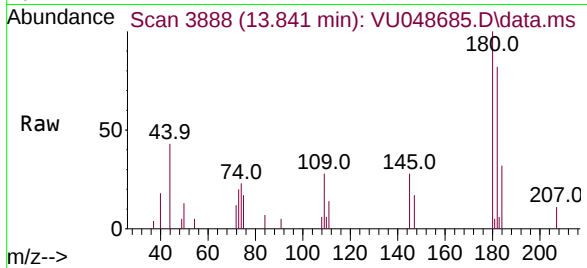

#94
Hexachlorobutadiene
Concen: 0.452 ug/l
RT: 14.024 min Scan# 3945
Delta R.T. 0.006 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion:225 Resp: 945
Ion Ratio Lower Upper
225 100
223 54.2 30.9 92.8
227 59.2 31.1 93.5


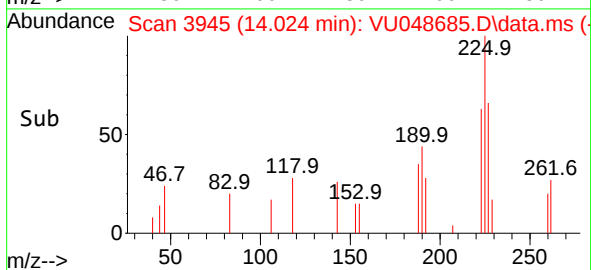

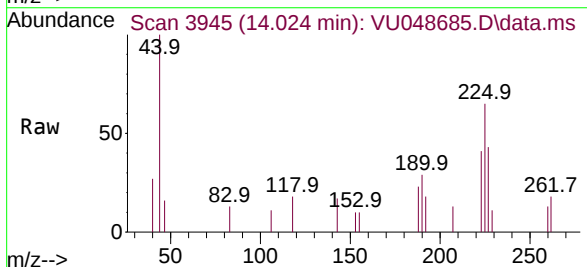


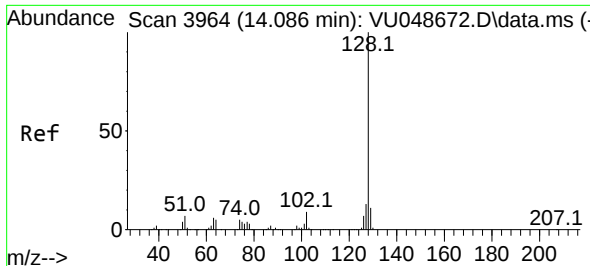

#95
Naphthalene
Concen: 4.091 ug/l
RT: 14.092 min Scan# 3964
Delta R.T. 0.006 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK

Tgt Ion:	128	Resp:	25019
Ion Ratio	Lower	Upper	
128	100		
127	14.1	10.2	15.4
129	11.2	8.7	13.1

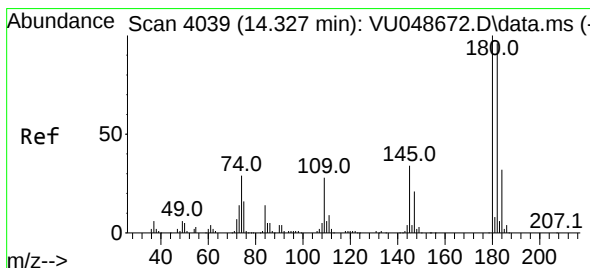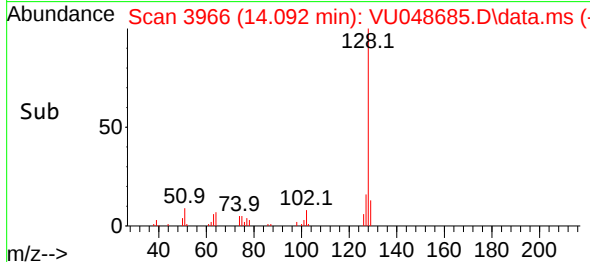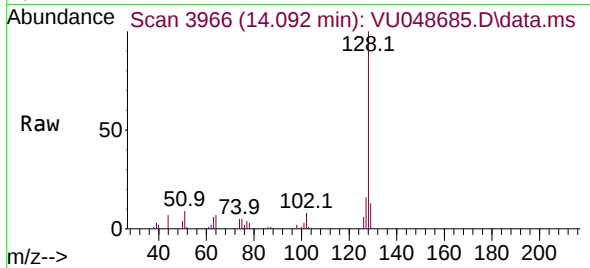

#96
1,2,3-Trichlorobenzene
Concen: 0.962 ug/l
RT: 14.330 min Scan# 4040
Delta R.T. 0.003 min
Lab File: VU048685.D
Acq: 27 May 2022 11:56

Tgt Ion:	180	Resp:	4159
Ion Ratio	Lower	Upper	
180	100		
182	89.2	47.4	142.2
145	33.2	16.6	49.8

