


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052722\
 Data File : VU048680.D
 Acq On : 27 May 2022 09:02
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Title : SW846 8260
 Last Update : Fri May 27 06:42:31 2022

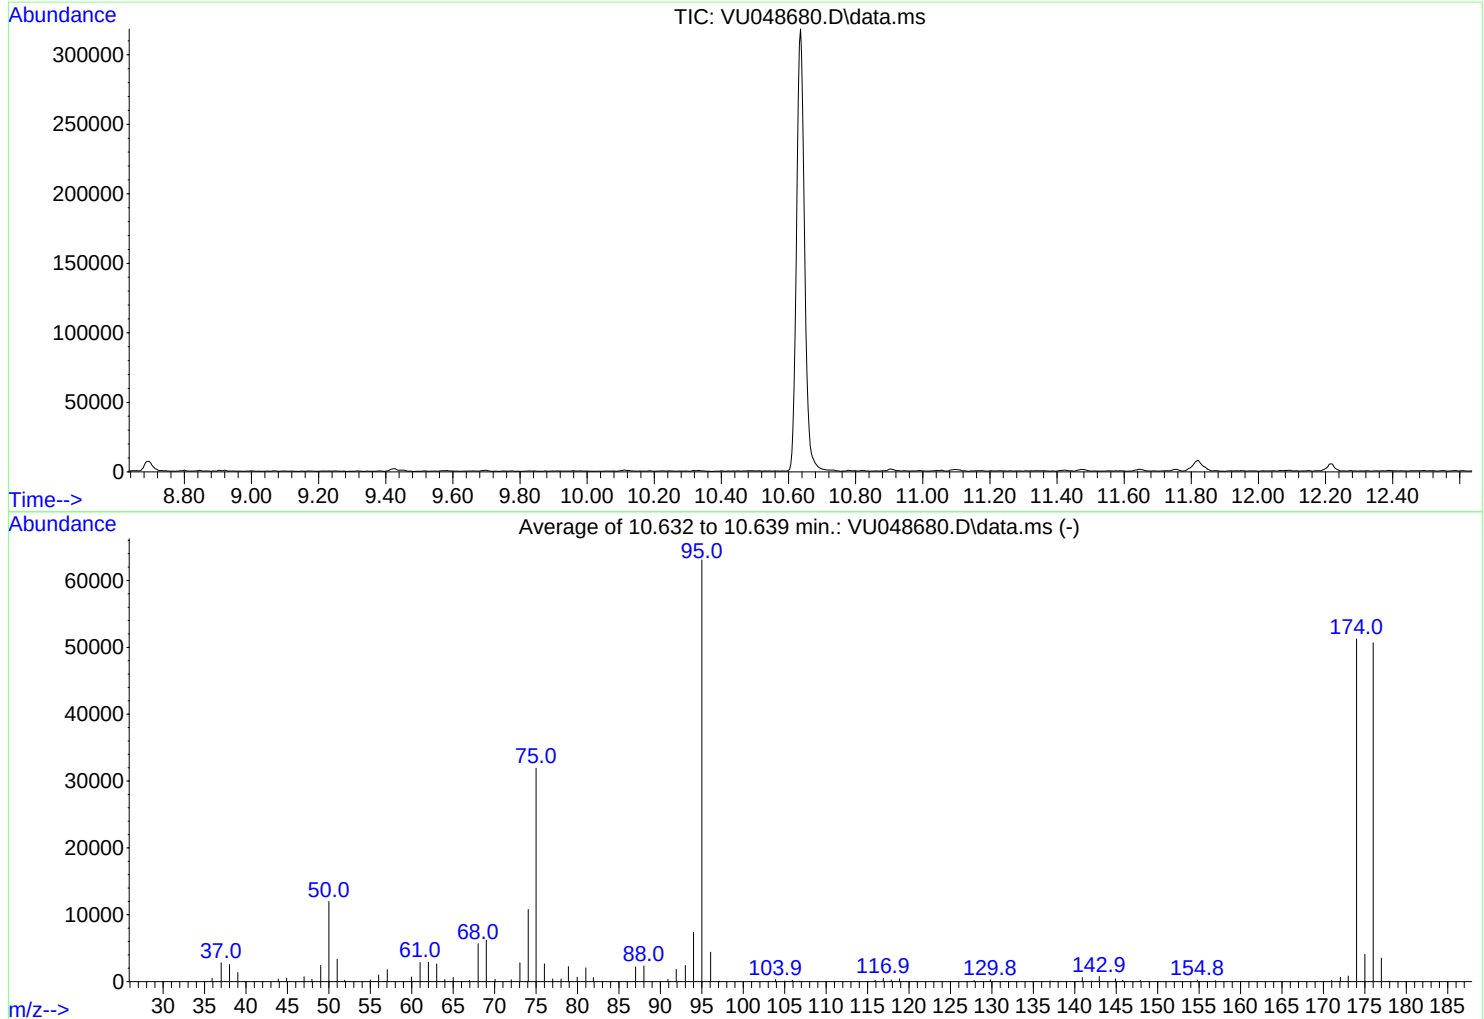

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	11983	PASS
75	95	30	60	50.6	31920	PASS
95	95	100	100	100.0	63085	PASS
96	95	5	9	7.0	4409	PASS
173	174	0.00	2	1.6	838	PASS
174	95	50	100	81.2	51253	PASS
175	174	5	9	8.0	4115	PASS
176	174	95	101	98.9	50683	PASS
177	176	5	9	7.0	3527	PASS