


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052820\
Data File : VU038354.D
Acq On : 28 May 2020 18:28
Operator : JC/MD
Sample : L2751-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y24

Manual Integrations
APPROVED

MMDadoda
6/1/2020 12:26:43 PM

Quant Time: Mav 29 05:54:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 29 04:31:03 2020
Response via : Initial Calibration

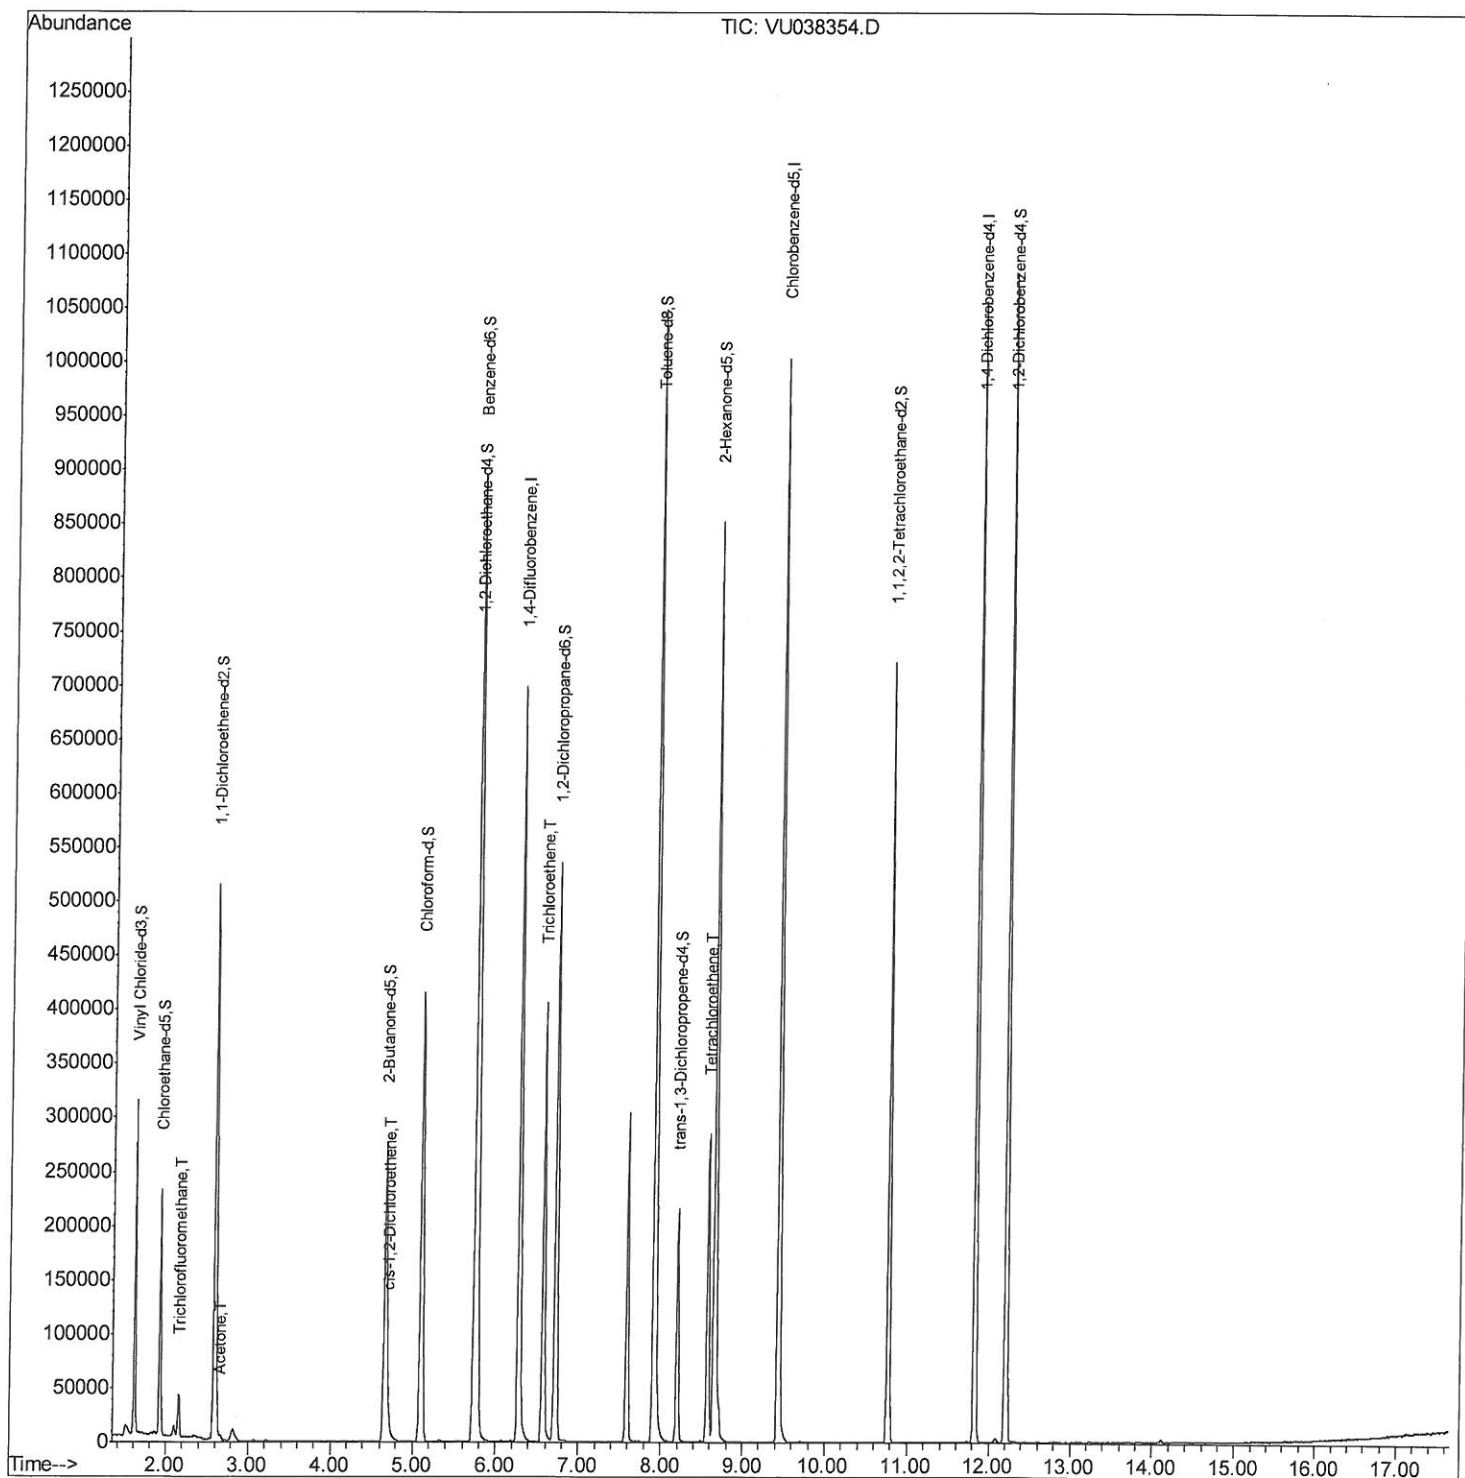

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052820\
 Data File : VU038354.D
 Acq On : 28 May 2020 18:28
 Operator : JC/MD
 Sample : L2751-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y24

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 12:26:43 PM

Quant Time: May 29 04:34:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 29 04:31:03 2020
 Response via : Initial Calibration

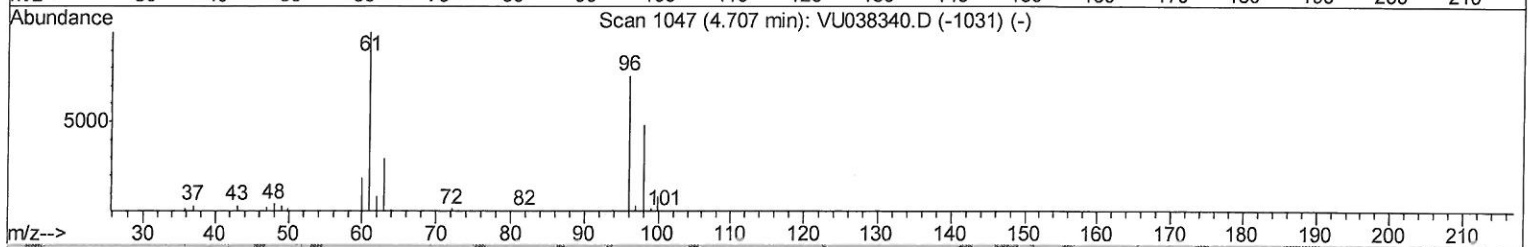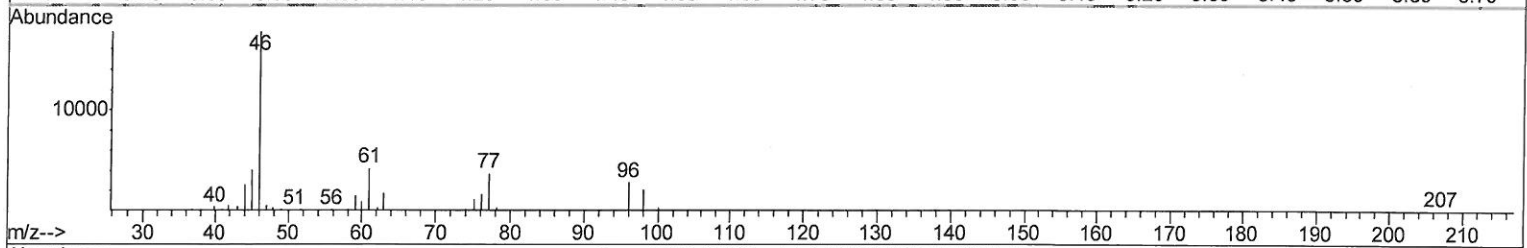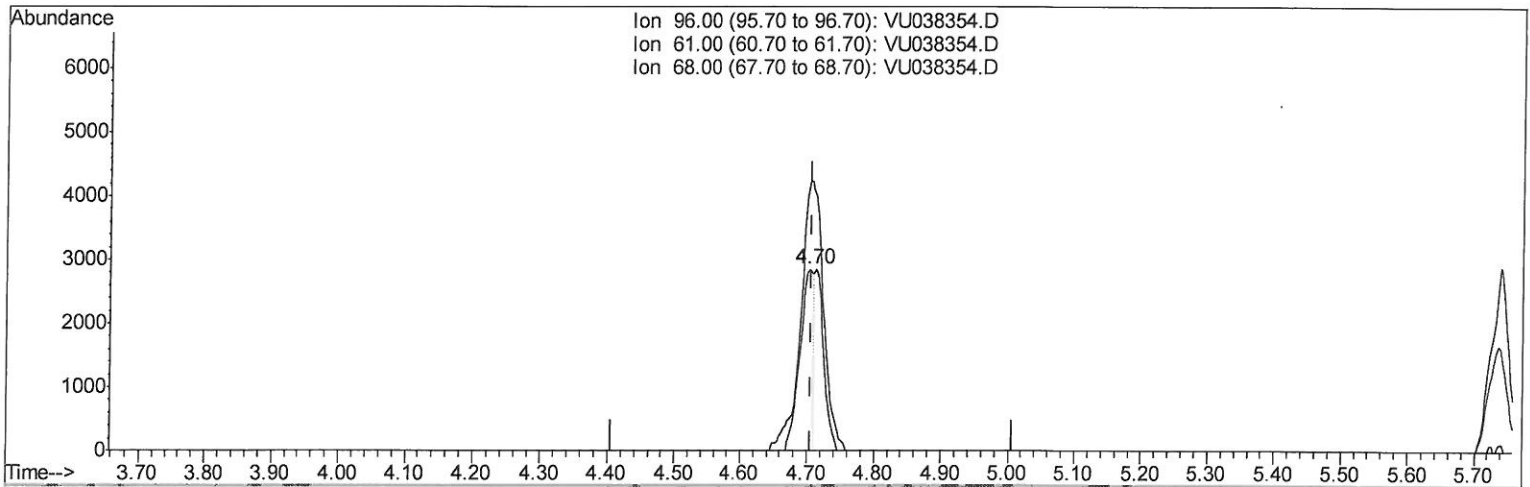

TIC: VU038354.D

(20) cis-1,2-Dichloroethene (T)

4.703min (-0.004) 0.98ug/L

response 4058

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	148.11
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052820\
 Data File : VU038354.D
 Acq On : 28 May 2020 18:28
 Operator : JC/MD
 Sample : L2751-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y24

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 12:26:43 PM

Quant Time: May 29 04:34:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 29 04:31:03 2020
 Response via : Initial Calibration

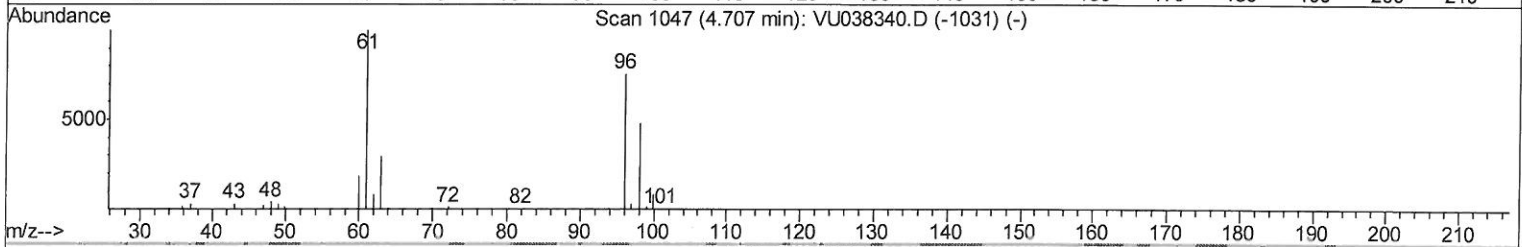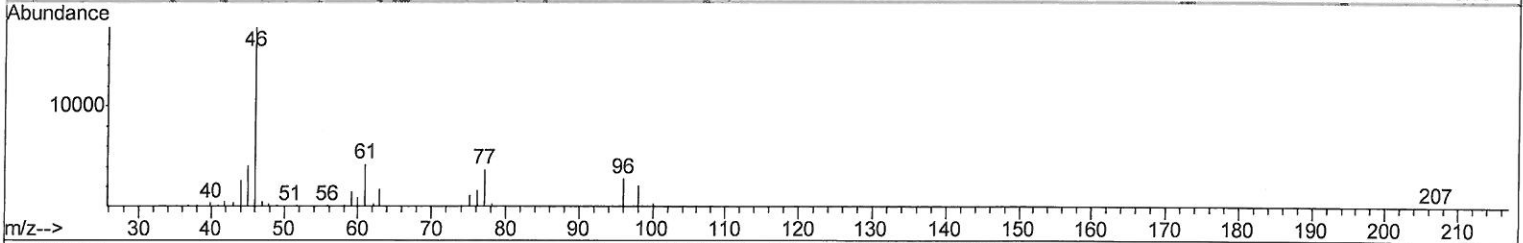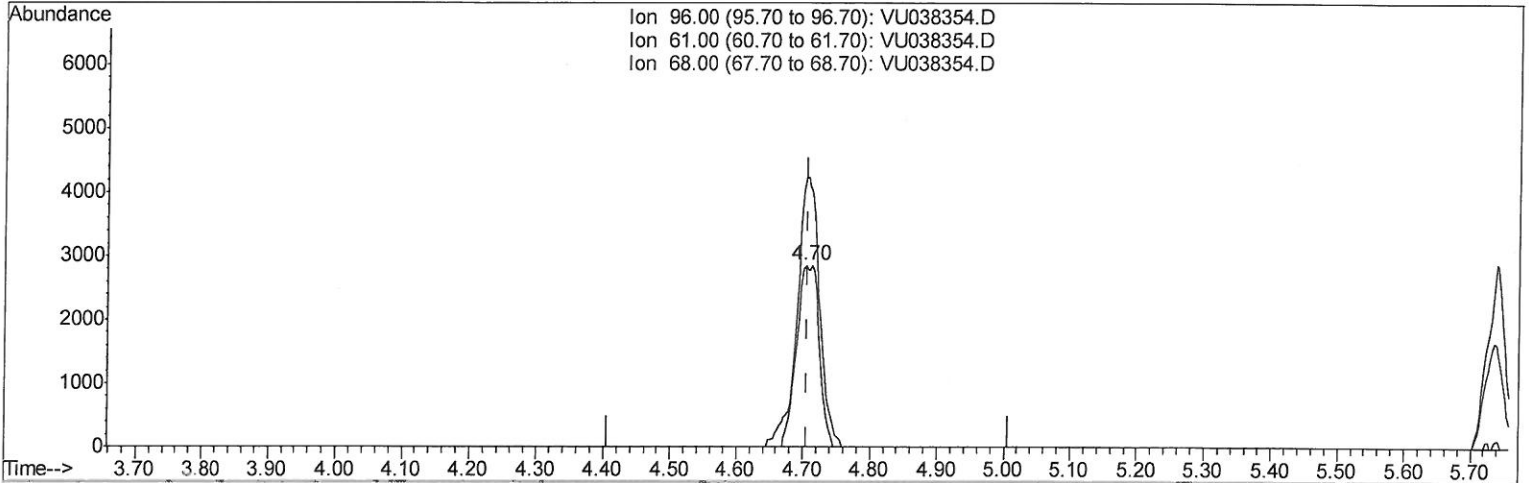

TIC: VU038354.D

(20) cis-1,2-Dichloroethene (T)

4.703min (-0.004) 1.60ug/L m

response 6654

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	148.11
68.00	0.00	0.00
0.00	0.00	0.00

Handwritten signature: 505/29/2024

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052820\
 Data File : VU038354.D
 Acq On : 28 May 2020 18:28
 Operator : JC/MD
 Sample : L2751-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y24

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 12:26:43 PM

Quant Time: May 29 05:54:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 29 04:31:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	581660	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	565934	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	264090	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	205291	56.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	112.44%
7) Chloroethane-d5	1.93	69	161585	57.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.56%
11) 1,1-Dichloroethene-d2	2.59	63	306687	41.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.18%
21) 2-Butanone-d5	4.66	46	404585	116.62	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.62%
24) Chloroform-d	5.10	84	384190	53.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.16%
26) 1,2-Dichloroethane-d4	5.74	65	264753	53.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.76%
32) Benzene-d6	5.76	84	815551	55.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.92%
36) 1,2-Dichloropropane-d6	6.72	67	251618	55.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.40%
41) Toluene-d8	7.92	98	707264	54.41	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.82%
43) trans-1,3-Dichloropropene-	8.20	79	118265	52.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.22%
47) 2-Hexanone-d5	8.65	63	295308	123.05	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.05%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	352806	52.30	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.60%
64) 1,2-Dichlorobenzene-d4	12.20	152	272425	55.65	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.30%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
9) Trichlorofluoromethane	2.16	101	24581	4.115	ug/L	97
13) Acetone	2.66	43	5681	1.971	ug/L	97
20) cis-1,2-Dichloroethene	4.70	96	6654m	1.603	ug/L	98
34) Trichloroethene	6.57	95	135469	33.311	ug/L	98
46) Tetrachloroethene	8.57	164	64159	21.580	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed