


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052820\
 Data File : VU038333.D
 Acq On : 28 May 2020 08:41
 Operator : JC/MD
 Sample : BFB48
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Title : VOC Analysis
 Last Update : Sat May 30 07:49:50 2020

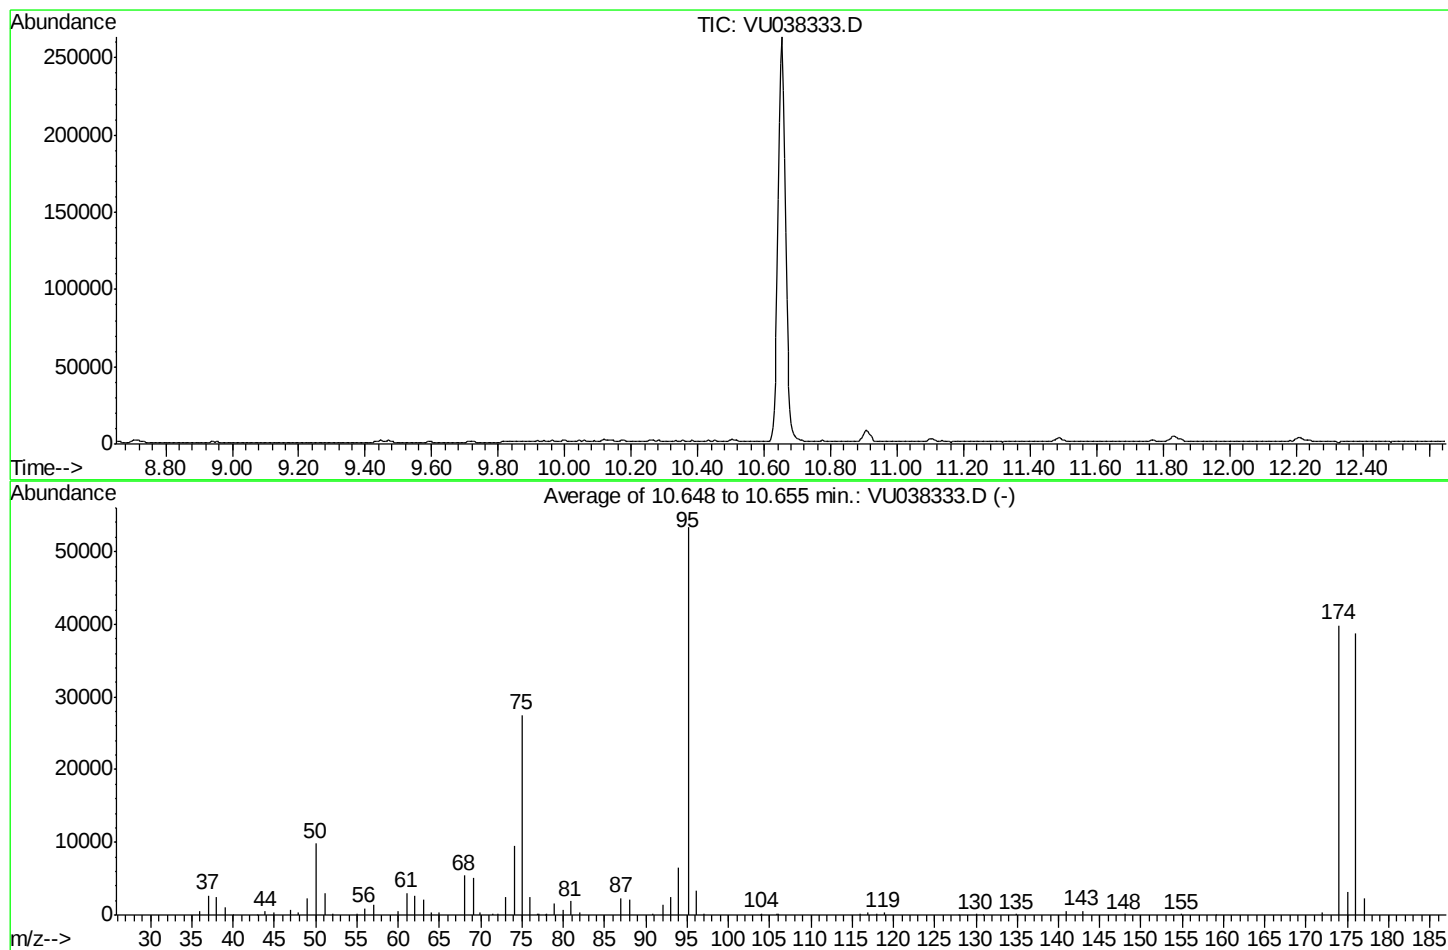

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	9847	PASS
75	95	30	80	51.7	27565	PASS
95	95	100	100	100.0	53344	PASS
96	95	5	9	6.4	3394	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.7	39872	PASS
175	174	5	9	8.0	3183	PASS
176	174	95	101	97.1	38712	PASS
177	176	5	9	6.1	2363	PASS