


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052820\
 Data File : VU038333.D
 Acq On : 28 May 2020 08:41
 Operator : JC/MD
 Sample : BFB48
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Title : VOC Analysis
 Last Update : Sat May 30 07:49:50 2020

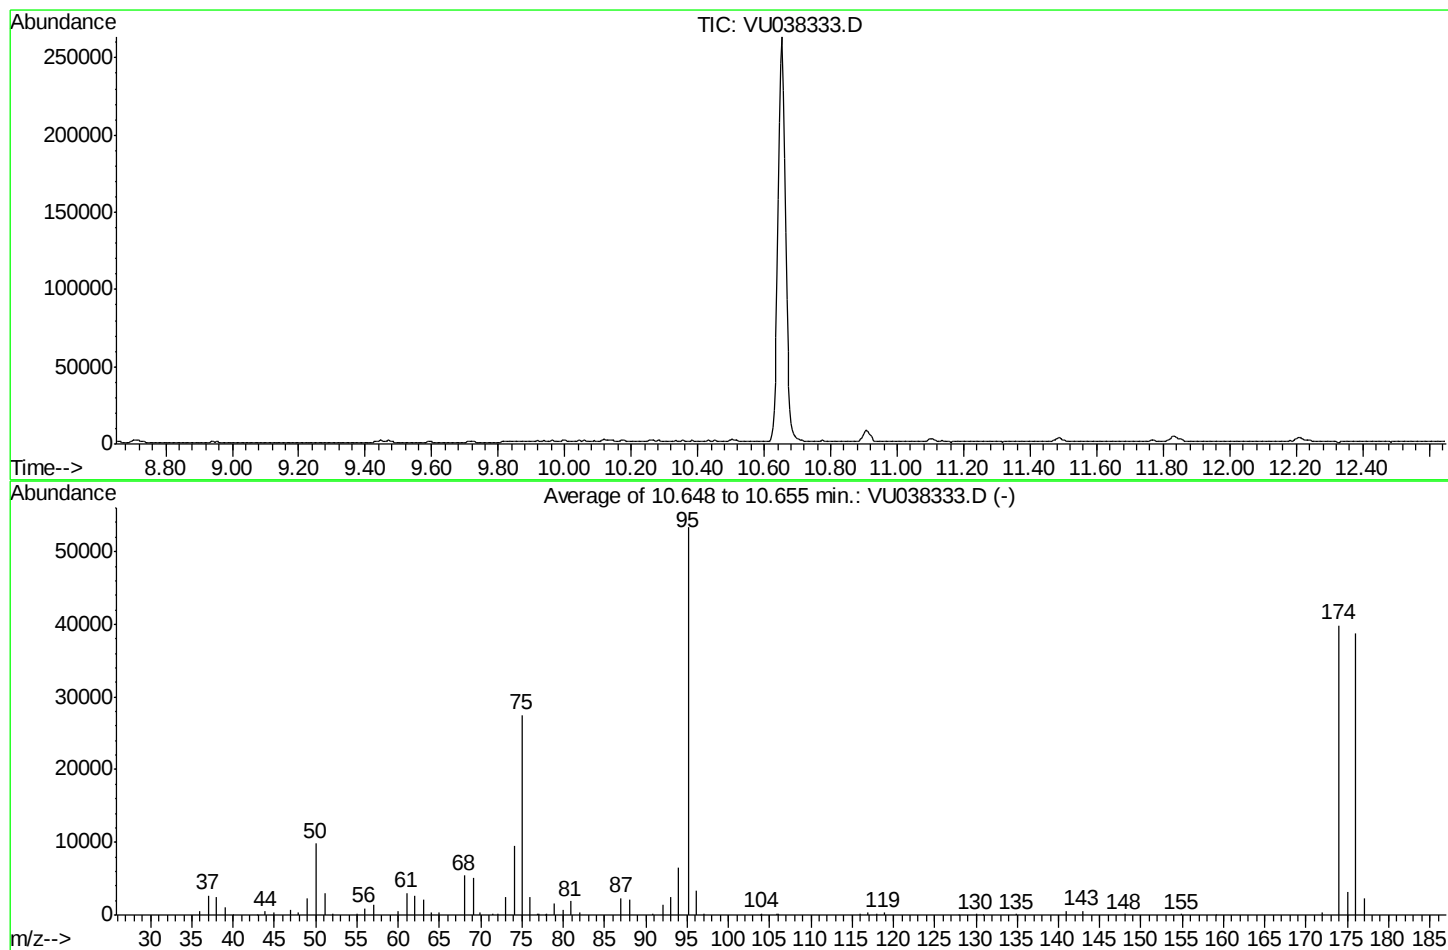

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	9847	PASS
75	95	30	80	51.7	27565	PASS
95	95	100	100	100.0	53344	PASS
96	95	5	9	6.4	3394	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.7	39872	PASS
175	174	5	9	8.0	3183	PASS
176	174	95	101	97.1	38712	PASS
177	176	5	9	6.1	2363	PASS

m/z	Abundance
35.90	1047.0
37.00	2514.0
38.00	2610.0
39.00	1012.0
39.90	214.0
42.90	121.0
44.00	1306.0
45.00	415.0
47.00	765.0
47.90	246.0
49.00	2277.0
50.00	9878.0
51.10	2966.0
52.10	132.0
54.90	213.0
55.90	804.0
56.90	1411.0
60.00	576.0
61.00	2947.0
62.00	2511.0
63.10	2269.0
64.00	255.0
64.90	393.0
68.00	5212.0
69.00	5249.0
69.90	336.0
72.00	232.0
73.10	2393.0
74.10	9181.0
75.00	26640.0
76.00	2509.0
76.80	312.0
77.80	229.0
78.90	1533.0
79.90	613.0
80.90	1821.0
81.90	400.0
87.00	2336.0
88.00	2059.0
90.80	217.0
92.00	1419.0
93.00	2455.0
94.00	6508.0
95.10	51304.0
96.10	3237.0
97.10	106.0
103.80	194.0
104.00	198.0
105.80	141.0
106.00	143.0
115.90	165.0
116.90	293.0
118.10	210.0
118.80	347.0
127.90	132.0
130.00	184.0
130.80	101.0
135.00	112.0
141.00	467.0
143.00	516.0
148.00	136.0
154.90	176.0
159.00	117.0
172.00	388.0
174.00	37048.0
175.00	3025.0
176.00	36448.0
177.00	2252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	1094.0
37.00	2796.0
38.00	2817.0
39.00	1006.0
39.90	211.0
44.00	1170.0
44.90	442.0
47.00	710.0
47.90	242.0
49.00	2380.0
50.00	10145.0
51.00	3079.0
52.00	109.0
54.90	243.0
55.90	957.0
57.00	1374.0
59.90	616.0
61.00	3147.0
62.00	2814.0
63.10	2222.0
64.00	310.0
64.90	460.0
68.00	5564.0
69.10	5250.0
69.90	343.0
71.50	162.0
72.00	226.0
73.00	2592.0
74.10	9769.0
75.00	28192.0
76.00	2688.0
76.80	296.0
78.90	1701.0
80.00	660.0
80.90	1937.0
82.00	403.0
87.00	2473.0
88.00	2185.0
90.80	238.0
92.00	1533.0
93.00	2600.0
94.00	6678.0
95.10	55160.0
96.10	3470.0
97.10	115.0
104.10	243.0
105.80	196.0
106.00	197.0
115.90	211.0
117.00	315.0
118.10	195.0
118.90	334.0
127.80	120.0
130.00	171.0
135.00	110.0
141.00	546.0
142.90	615.0
148.00	168.0
155.00	147.0
159.00	112.0
172.00	397.0
174.00	41312.0
175.00	3288.0
176.00	39848.0
177.00	2452.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	1024.0
37.00	2741.0
38.00	2709.0
39.00	977.0
39.90	172.0
43.90	1100.0
44.90	434.0
47.00	715.0
47.90	350.0
49.00	2306.0
50.00	9518.0
51.00	3027.0
52.00	126.0
55.00	239.0
55.90	981.0
57.00	1292.0
59.90	531.0
61.00	2964.0
62.00	2709.0
63.10	1993.0
64.00	309.0
64.90	418.0
68.00	5508.0
69.10	5025.0
70.00	319.0
71.50	128.0
72.00	180.0
73.00	2507.0
74.10	9354.0
75.00	27864.0
76.00	2413.0
77.10	290.0
78.00	331.0
78.90	1656.0
80.00	647.0
80.90	1871.0
82.00	370.0
87.00	2231.0
88.00	2085.0
90.80	201.0
92.00	1477.0
93.00	2523.0
94.00	6354.0
95.10	53568.0
96.10	3475.0
97.10	114.0
104.10	258.0
105.80	254.0
115.90	227.0
116.90	262.0
118.00	160.0
118.80	247.0
129.90	115.0
130.80	106.0
134.90	100.0
141.00	545.0
142.90	666.0
148.00	152.0
155.00	128.0
172.00	396.0
174.00	41256.0
175.00	3236.0
176.00	39840.0
177.00	2387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

Scan 2883 (10.610 min): VU038333.D
BFB48

m/z	Abundance
36.00	570.0
36.70	102.0
37.90	232.0
40.00	184.0
43.90	701.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48