

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052821\
 Data File : VU044003.D
 Acq On : 28 May 2021 12:50
 Operator : SY/MD
 Sample : VU0528WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 29 02:05:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 29 02:01:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	15258	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	13736	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.741	152	6333	0.50	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	3450	0.37	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	74.00%
4) 1,2-Dichloroethane-d4	5.679	65	6248	0.45	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	90.00%
7) 1,2-Dichloropropane-d6	6.658	67	7163	0.54	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.00%
8) Toluene-d8	7.845	98	13894	0.51	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.00%
10) 1,1,2,2-Tetrachloroeth...	10.696	84	6873	0.55	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.00%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.924	75	24	0.01	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052821\
Data File : VU044003.D
Acq On : 28 May 2021 12:50
Operator : SY/MD
Sample : VU0528WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 29 02:05:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 29 02:01:06 2021
Response via : Initial Calibration

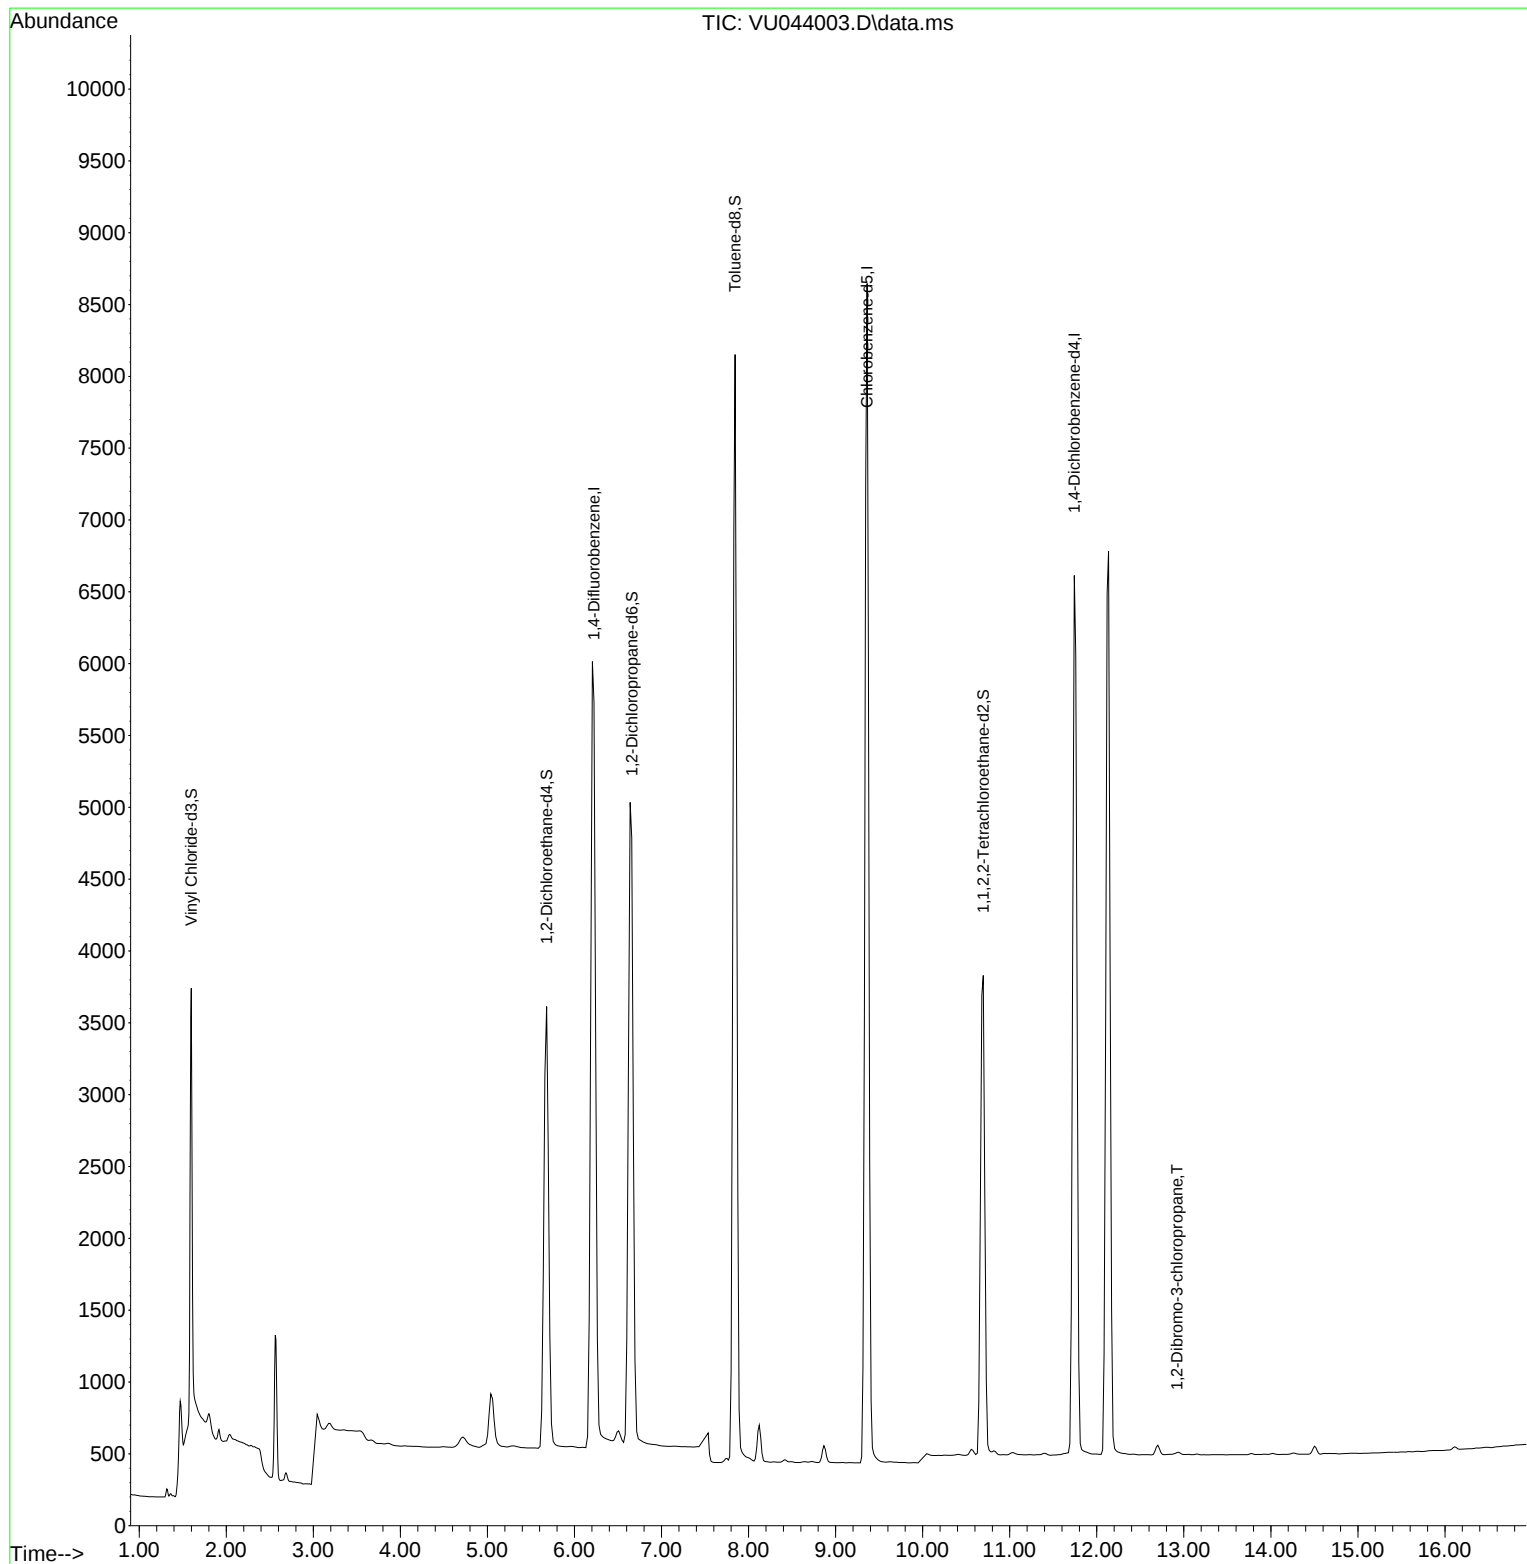

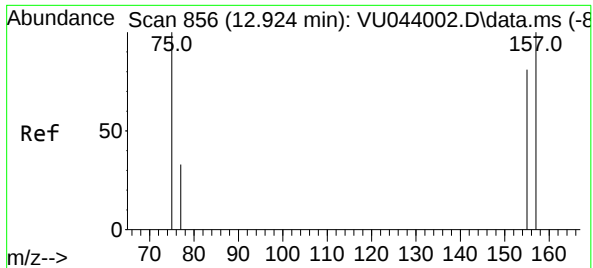

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.01 ug/L
 RT: 12.924 min Scan# 856
 Delta R.T. -0.000 min
 Lab File: VU044003.D
 Acq: 28 May 2021 12:50

Instrument :
 MSVOA_U
 ClientSampleId :

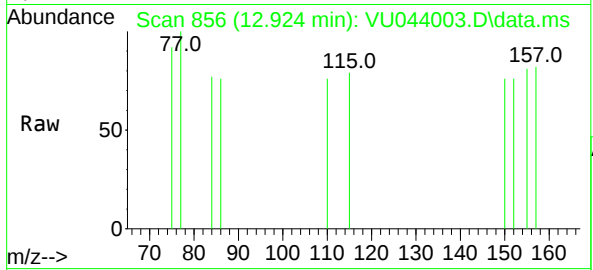

Tgt Ion: 75	Resp: 24
Ion Ratio	Lower Upper
75	100
157	89.5 71.8 107.8
155	87.7 61.2 91.8

