
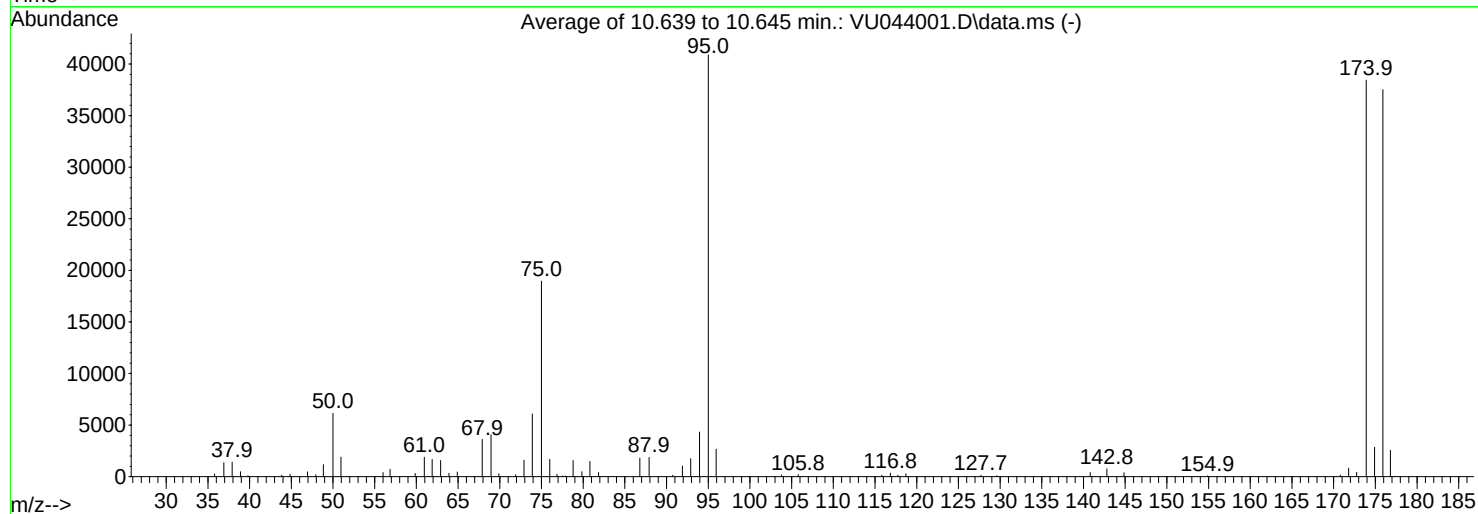


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052821\
 Data File : VU044001.D
 Acq On : 28 May 2021 11:50
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB137

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052621.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat May 29 02:01:06 2021

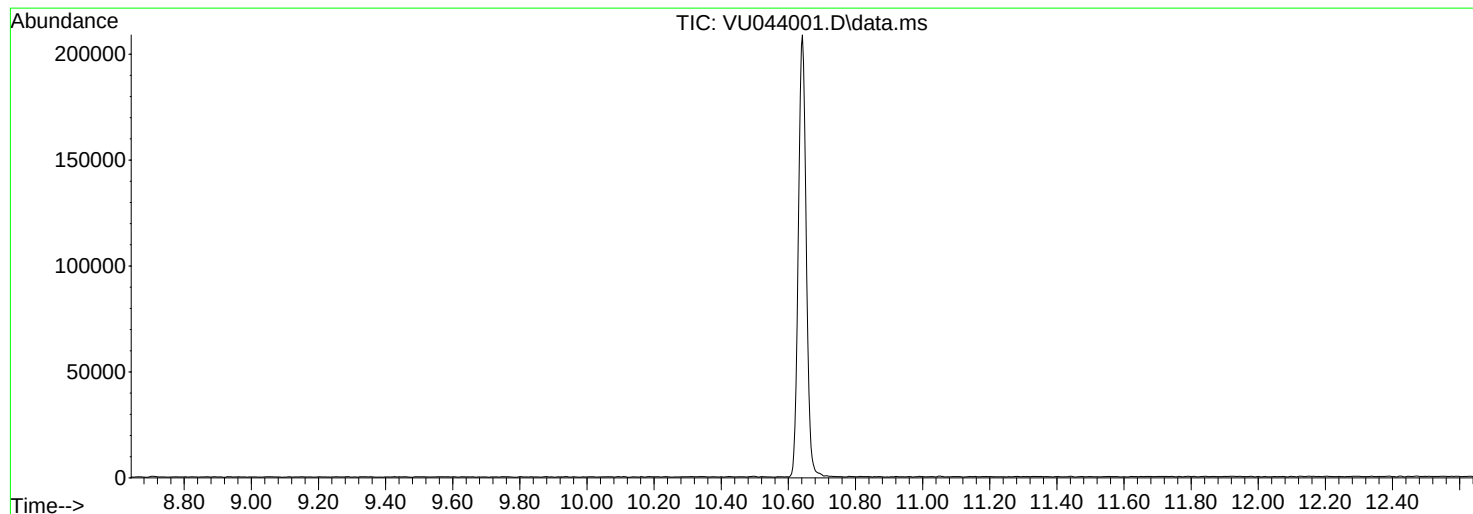

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	6151	PASS
75	95	30	80	46.4	18957	PASS
95	95	100	100	100.0	40893	PASS
96	95	5	9	6.5	2666	PASS
173	174	0.00	2	1.1	418	PASS
174	95	50	120	94.0	38435	PASS
175	174	5	9	7.4	2847	PASS
176	174	95	101	97.7	37533	PASS
177	176	5	9	6.8	2567	PASS

m/z	Abundance
35.80	284.0
36.90	1359.0
37.90	1408.0
38.90	470.0
39.80	209.0
43.90	646.0
44.90	242.0
46.90	503.0
47.90	188.0
48.80	1153.0
50.00	6293.0
50.90	2045.0
56.00	403.0
56.90	728.0
59.90	313.0
61.00	1930.0
61.90	1865.0
62.90	1544.0
63.90	359.0
64.90	512.0
67.90	3756.0
68.90	3995.0
69.90	342.0
71.90	176.0
72.90	1604.0
73.90	6167.0
75.00	19168.0
76.00	1662.0
76.80	247.0
77.90	176.0
78.80	1579.0
79.90	460.0
80.80	1489.0
81.80	353.0
86.80	1855.0
87.90	1847.0
90.80	157.0
91.90	1056.0
92.90	1688.0
94.00	4529.0
95.00	41080.0
96.00	2736.0
103.80	177.0
105.80	177.0
115.80	158.0
116.90	314.0
117.80	142.0
118.70	301.0
127.70	135.0
129.60	141.0
140.80	433.0
142.80	654.0
144.80	390.0
154.90	111.0
170.80	173.0
171.80	867.0
172.70	460.0
173.90	38040.0
174.90	2908.0
175.90	37040.0
176.80	2616.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.80	274.0
36.90	1385.0
37.90	1466.0
38.90	499.0
39.80	214.0
43.90	605.0
44.90	213.0
47.00	476.0
47.90	205.0
48.90	1173.0
50.00	6339.0
51.00	1913.0
56.00	390.0
56.90	725.0
59.80	306.0
61.00	1936.0
61.90	1697.0
62.90	1631.0
63.90	337.0
64.90	471.0
66.90	101.0
67.90	3705.0
69.00	4171.0
69.90	279.0
71.90	187.0
72.90	1672.0
73.90	6224.0
75.00	19528.0
76.00	1727.0
76.90	222.0
77.60	107.0
78.80	1605.0
79.80	501.0
80.80	1525.0
81.80	409.0
86.80	1874.0
87.90	1970.0
90.70	154.0
91.90	1051.0
92.90	1781.0
93.90	4418.0
95.00	42104.0
96.00	2708.0
103.80	178.0
105.80	208.0
115.80	161.0
116.80	359.0
117.70	154.0
118.70	283.0
127.70	141.0
129.60	124.0
140.80	420.0
142.80	804.0
144.90	393.0
154.90	110.0
170.80	167.0
171.80	848.0
172.70	425.0
173.90	39600.0
174.90	2893.0
175.90	38776.0
176.80	2681.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.80	274.0
36.90	1385.0
37.90	1466.0
38.90	499.0
39.80	214.0
43.90	605.0
44.90	213.0
47.00	476.0
47.90	205.0
48.90	1173.0
50.00	6339.0
51.00	1913.0
56.00	390.0
56.90	725.0
59.80	306.0
61.00	1936.0
61.90	1697.0
62.90	1631.0
63.90	337.0
64.90	471.0
66.90	101.0
67.90	3705.0
69.00	4171.0
69.90	279.0
71.90	187.0
72.90	1672.0
73.90	6224.0
75.00	19528.0
76.00	1727.0
76.90	222.0
77.60	107.0
78.80	1605.0
79.80	501.0
80.80	1525.0
81.80	409.0
86.80	1874.0
87.90	1970.0
90.70	154.0
91.90	1051.0
92.90	1781.0
93.90	4418.0
95.00	42104.0
96.00	2708.0
103.80	178.0
105.80	208.0
115.80	161.0
116.80	359.0
117.70	154.0
118.70	283.0
127.70	141.0
129.60	124.0
140.80	420.0
142.80	804.0
144.90	393.0
154.90	110.0
170.80	167.0
171.80	848.0
172.70	425.0
173.90	39600.0
174.90	2893.0
175.90	38776.0
176.80	2681.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

Scan 2879 (10.597 min): VU044001.D\data.ms
BFB37

m/z	Abundance
39.80	107.0
43.80	459.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137