

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059040.D
 Acq On : 28 May 2024 19:22
 Operator : MD/SY
 Sample : P2570-14ME
 Misc : 6.42g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 29 02:46:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 29 02:38:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	189007	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	181636	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	67404	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	73252	36.644	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.280%
7) Chloroethane-d5	1.872	69	63546	38.250	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	76.500%
11) 1,1-Dichloroethene-d2	2.531	63	94885	31.068	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.140%
21) 2-Butanone-d5	4.624	46	133259	97.048	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.050%
24) Chloroform-d	5.049	84	129616	37.802	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.600%
26) 1,2-Dichloroethane-d4	5.692	65	89711	42.781	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.560%
32) Benzene-d6	5.711	84	267207	43.151	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.300%
36) 1,2-Dichloropropane-d6	6.682	67	93002	45.471	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.940%
41) Toluene-d8	7.891	98	212150	38.222	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.440%#
43) trans-1,3-Dichloroprop...	8.174	79	36291	39.515	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.040%
47) 2-Hexanone-d5	8.640	63	77659	91.805	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.810%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	128012	41.603	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	64934	46.688	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.380%
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.807	75	10309	6.010	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059040.D
Acq On : 28 May 2024 19:22
Operator : MD/SY
Sample : P2570-14ME
Misc : 6.42g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 29 02:46:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 29 02:38:59 2024
Response via : Initial Calibration

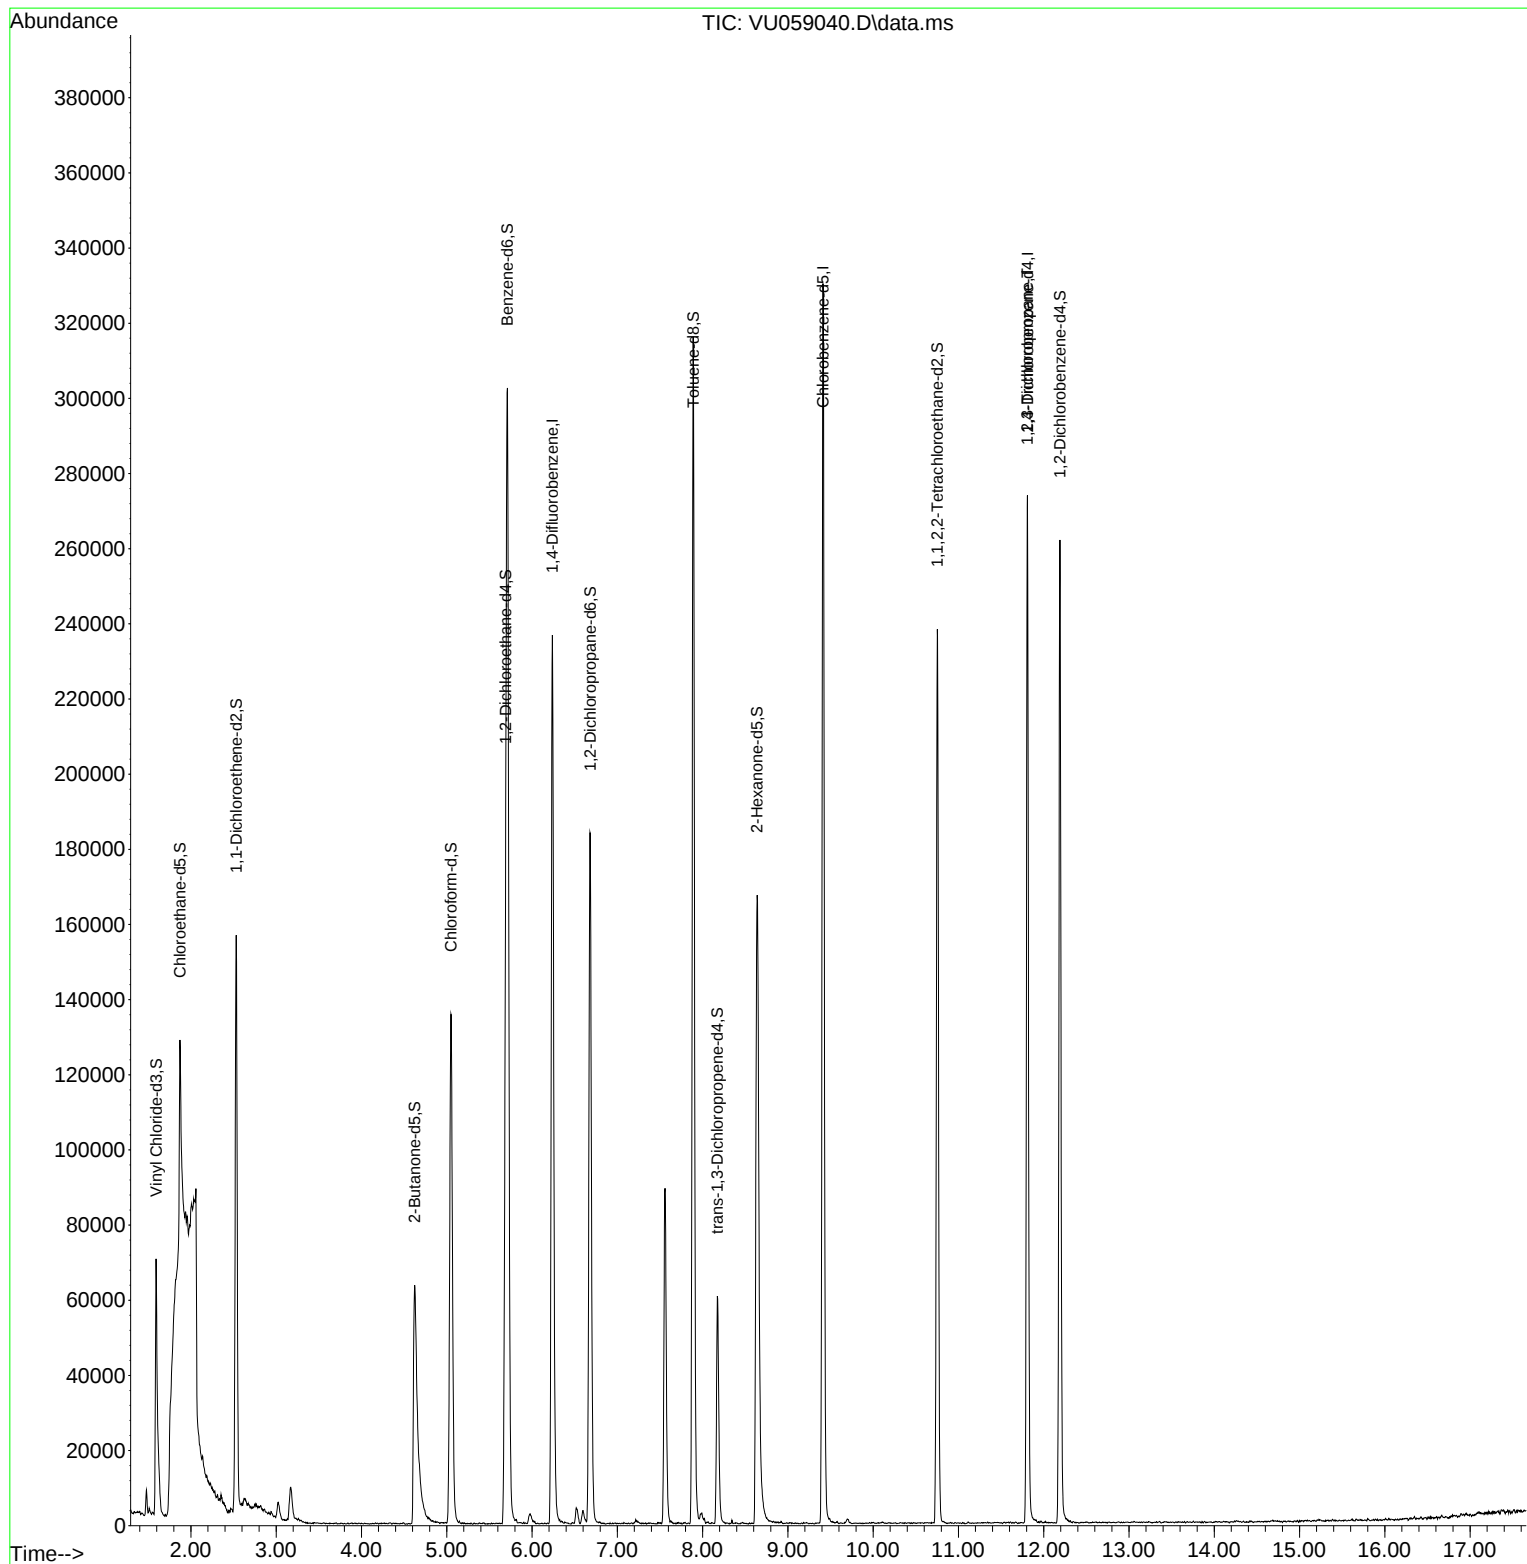

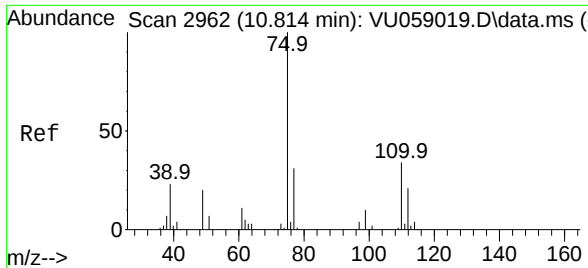

#60
 1,2,3-Trichloropropane
 Concen: 6.010 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.994 min
 Lab File: VU059040.D
 Acq: 28 May 2024 19:22

Instrument :
 MSVOA_U
 ClientSampleId :

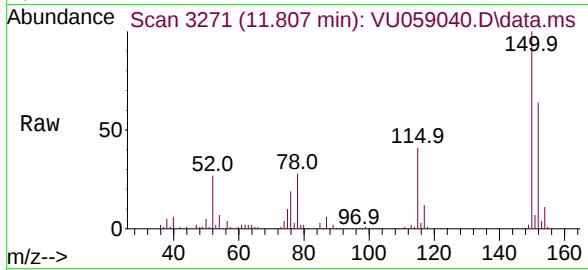

Tgt Ion:	75	Resp:	10309
Ion	Ratio	Lower	Upper
75	100		
77	31.2	25.8	38.6
110	0.5	28.3	42.5#

