

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059020.D
 Acq On : 28 May 2024 10:59
 Operator : MD/SY
 Sample : VU0528MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	119	rBV	97911	131822	15.48%	2.015%
2	1.875	136	182	207	rBV2	172679	578785	67.97%	8.846%
3	2.550	379	392	407	rBV	166106	269764	31.68%	4.123%
4	2.624	413	415	422	rVB2	931	753	0.09%	0.012%
5	2.695	434	437	447	rVB	224	234	0.03%	0.004%
6	2.772	453	461	471	rVV	1108	1977	0.23%	0.030%
7	2.923	506	508	511	rVB	337	168	0.02%	0.003%
8	3.029	531	541	550	rBV4	2508	4261	0.50%	0.065%
9	3.174	579	586	590	rBV3	633	962	0.11%	0.015%
10	3.341	635	638	641	rBB3	280	175	0.02%	0.003%
11	3.689	741	746	750	rVB2	201	181	0.02%	0.003%
12	3.933	818	822	825	rBV	261	176	0.02%	0.003%
13	3.984	835	838	844	rVB2	245	217	0.03%	0.003%
14	4.103	866	875	877	rBV2	222	302	0.04%	0.005%
15	4.248	917	920	923	rVV	261	175	0.02%	0.003%
16	4.418	967	973	975	rBV	264	246	0.03%	0.004%
17	4.473	985	990	993	rBV	281	217	0.03%	0.003%
18	4.611	1023	1033	1071	rBV2	76070	206446	24.25%	3.155%
19	5.049	1153	1169	1189	rBV	148619	332287	39.02%	5.078%
20	5.299	1242	1247	1252	rBV2	322	268	0.03%	0.004%
21	5.486	1299	1305	1307	rBV2	167	172	0.02%	0.003%
22	5.592	1334	1338	1341	rBV2	185	163	0.02%	0.002%
23	5.714	1356	1376	1402	rBV2	312251	851498	100.00%	13.014%
24	5.849	1416	1418	1422	rVB2	284	171	0.02%	0.003%
25	5.981	1447	1459	1465	rBV6	767	1586	0.19%	0.024%
26	6.036	1473	1476	1480	rBV2	212	163	0.02%	0.002%
27	6.087	1487	1492	1493	rBV2	198	162	0.02%	0.002%
28	6.123	1499	1503	1509	rVB3	357	327	0.04%	0.005%
29	6.238	1526	1539	1565	rBV	238214	455802	53.53%	6.966%
30	6.351	1572	1574	1577	rVB	467	215	0.03%	0.003%
31	6.489	1608	1617	1620	rVV2	334	361	0.04%	0.006%
32	6.525	1620	1628	1643	rVB7	3046	6380	0.75%	0.098%
33	6.582	1643	1646	1648	rBV	754	622	0.07%	0.010%
34	6.679	1664	1676	1696	rBV	197832	388505	45.63%	5.938%
35	6.775	1704	1706	1709	rBV	358	241	0.03%	0.004%
36	6.807	1714	1716	1726	rVB3	592	648	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059020.D
 Acq On : 28 May 2024 10:59
 Operator : MD/SY
 Sample : VU0528MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.856	1726	1731	1733	rBV	245	221	0.03%	0.003%
38	6.975	1762	1768	1772	rVB2	310	315	0.04%	0.005%
39	7.026	1781	1784	1788	rVB	226	166	0.02%	0.003%
40	7.058	1788	1794	1796	rBV2	319	305	0.04%	0.005%
41	7.081	1797	1801	1805	rVB2	176	184	0.02%	0.003%
42	7.213	1835	1842	1846	rBV4	521	620	0.07%	0.009%
43	7.328	1874	1878	1880	rBV2	275	195	0.02%	0.003%
44	7.354	1883	1886	1888	rVV2	259	178	0.02%	0.003%
45	7.367	1888	1890	1896	rVV2	167	187	0.02%	0.003%
46	7.483	1921	1926	1928	rBV2	260	190	0.02%	0.003%
47	7.557	1938	1949	1969	rBV	98608	178409	20.95%	2.727%
48	7.672	1982	1985	1989	rBB2	276	189	0.02%	0.003%
49	7.695	1989	1992	1996	rBV2	287	170	0.02%	0.003%
50	7.782	2015	2019	2021	rBV2	206	174	0.02%	0.003%
51	7.804	2025	2026	2033	rBV3	265	201	0.02%	0.003%
52	7.891	2037	2053	2075	rBV	357078	620421	72.86%	9.482%
53	8.026	2092	2095	2098	rVB3	350	218	0.03%	0.003%
54	8.090	2112	2115	2119	rVB3	367	259	0.03%	0.004%
55	8.174	2130	2141	2158	rBV	70643	120287	14.13%	1.838%
56	8.354	2192	2197	2199	rBV	210	164	0.02%	0.003%
57	8.367	2199	2201	2205	rVB2	337	213	0.03%	0.003%
58	8.454	2221	2228	2230	rBV	284	274	0.03%	0.004%
59	8.473	2231	2234	2239	rVB3	287	213	0.03%	0.003%
60	8.631	2272	2283	2315	rBV	214200	431449	50.67%	6.594%
61	8.846	2346	2350	2351	rBV	256	179	0.02%	0.003%
62	8.913	2368	2371	2374	rVV	213	163	0.02%	0.002%
63	8.933	2374	2377	2381	rVB3	475	390	0.05%	0.006%
64	8.958	2381	2385	2390	rBV	282	292	0.03%	0.004%
65	9.126	2434	2437	2441	rBV2	172	183	0.02%	0.003%
66	9.412	2514	2526	2555	rBV	330811	554690	65.14%	8.477%
67	9.560	2569	2572	2574	rBV2	429	268	0.03%	0.004%
68	9.698	2609	2615	2619	rBV2	776	1026	0.12%	0.016%
69	9.833	2652	2657	2660	rBV2	181	175	0.02%	0.003%
70	10.023	2710	2716	2720	rBV2	211	231	0.03%	0.004%
71	10.582	2888	2890	2894	rVB2	293	178	0.02%	0.003%
72	10.650	2905	2911	2917	rVV3	563	829	0.10%	0.013%
73	10.749	2930	2942	2965	rBV	271987	446183	52.40%	6.819%
74	10.910	2989	2992	2997	rBV2	207	225	0.03%	0.003%
75	10.974	3008	3012	3016	rBV2	299	297	0.03%	0.005%
76	11.807	3259	3271	3295	rBV	271486	450167	52.87%	6.880%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059020.D
 Acq On : 28 May 2024 10:59
 Operator : MD/SY
 Sample : VU0528MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.946	3310	3314	3321	rBV3	458	585	0.07%	0.009%
78	11.974	3321	3323	3328	rVB2	422	253	0.03%	0.004%
79	12.187	3377	3389	3413	rBV	289358	486651	57.15%	7.438%
80	12.614	3516	3522	3525	rBV2	190	263	0.03%	0.004%
81	12.675	3534	3541	3543	rBV2	357	362	0.04%	0.006%
82	12.733	3557	3559	3562	rVB2	392	208	0.02%	0.003%
83	12.749	3562	3564	3571	rBV2	161	166	0.02%	0.003%
84	12.936	3620	3622	3627	rVB2	264	170	0.02%	0.003%
85	12.974	3630	3634	3636	rBV	335	238	0.03%	0.004%
86	13.007	3641	3644	3649	rBV2	378	244	0.03%	0.004%
87	13.052	3655	3658	3662	rBV2	215	185	0.02%	0.003%
88	13.688	3852	3856	3859	rBV	275	248	0.03%	0.004%
89	13.785	3883	3886	3893	rVB2	297	323	0.04%	0.005%
90	13.859	3906	3909	3915	rVB2	441	413	0.05%	0.006%
91	13.923	3926	3929	3933	rBV2	347	280	0.03%	0.004%
92	14.109	3979	3987	3993	rBV5	1332	2316	0.27%	0.035%
93	14.566	4126	4129	4135	rVB2	500	471	0.06%	0.007%
94	14.775	4191	4194	4198	rVB2	354	314	0.04%	0.005%
95	14.878	4224	4226	4230	rVB	417	261	0.03%	0.004%
96	14.897	4230	4232	4234	rBV	376	230	0.03%	0.004%
97	15.093	4290	4293	4296	rBV2	450	283	0.03%	0.004%
98	15.203	4325	4327	4329	rBV	349	170	0.02%	0.003%
99	16.434	4707	4710	4712	rBV3	814	542	0.06%	0.008%
100	16.514	4731	4735	4740	rBV5	680	837	0.10%	0.013%




Sum of corrected areas: 6543123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059020.D
Acq On : 28 May 2024 10:59
Operator : MD/SY
Sample : VU0528MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

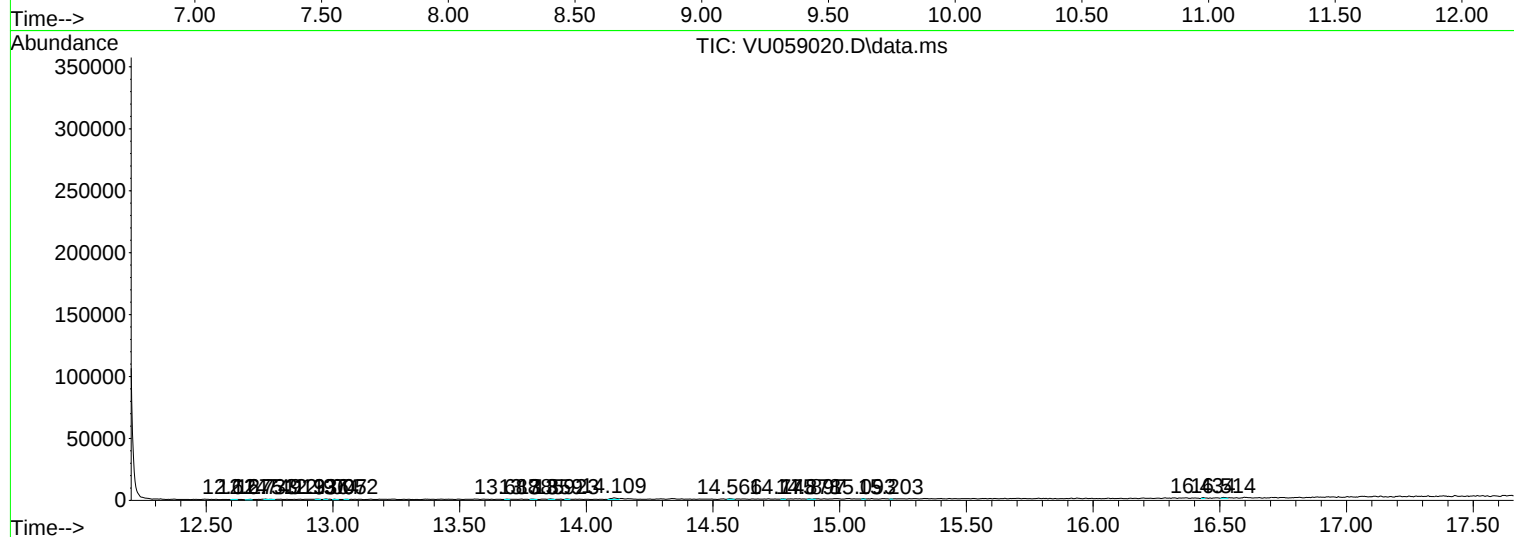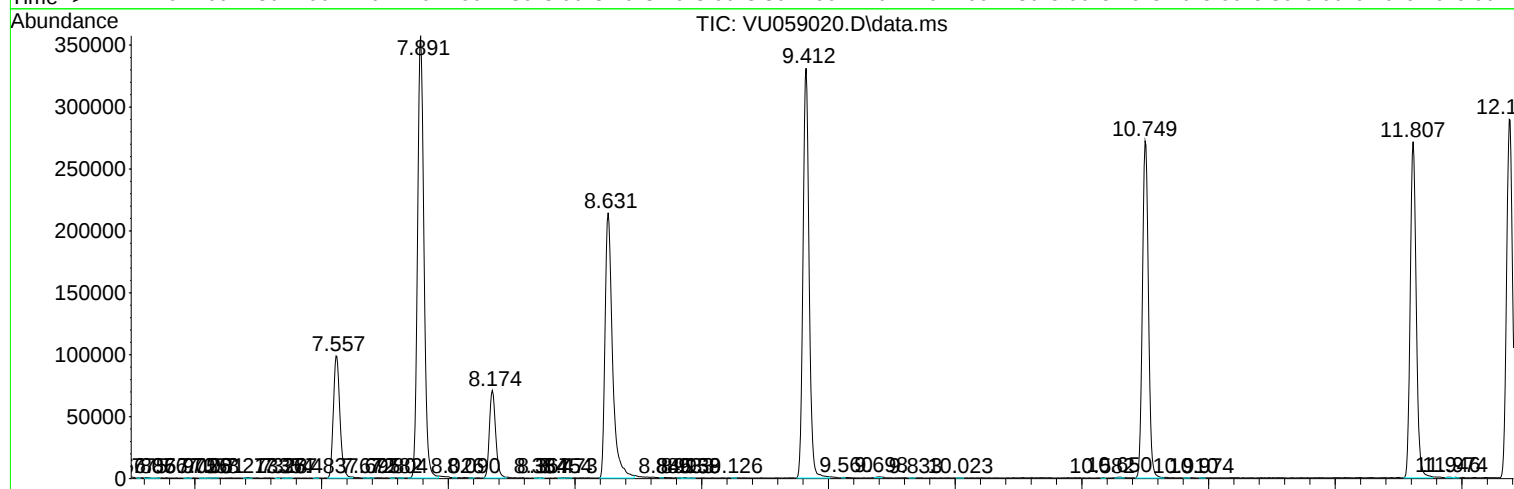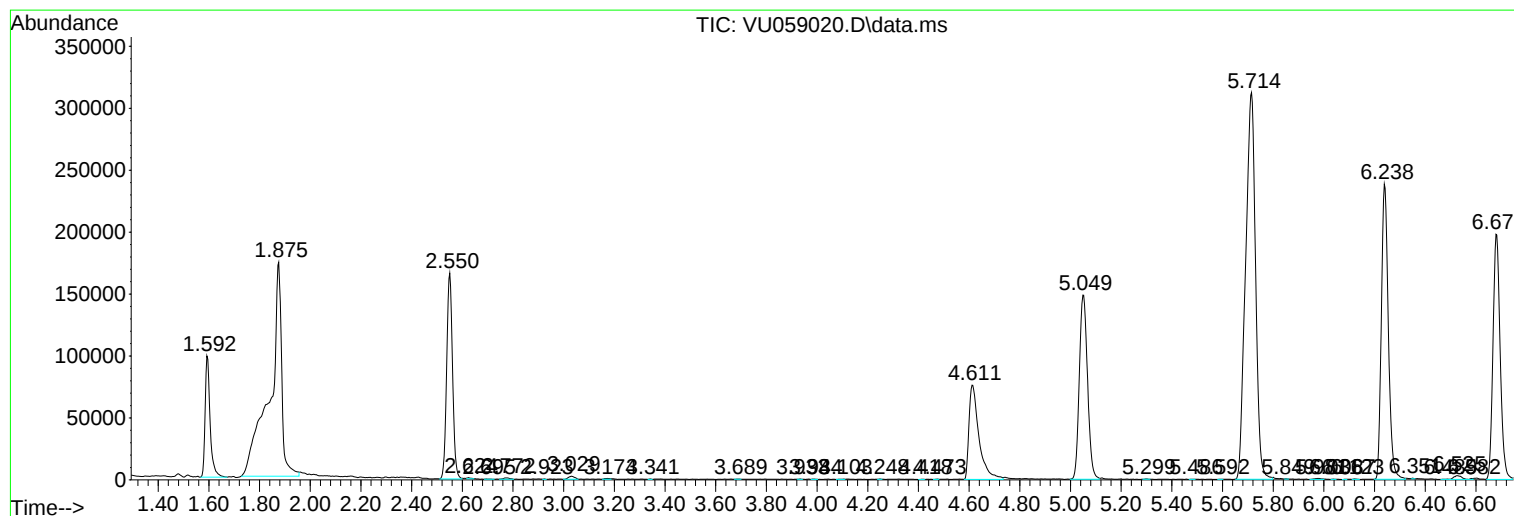

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059020.D
Acq On : 28 May 2024 10:59
Operator : MD/SY
Sample : VU0528MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059020.D
Acq On : 28 May 2024 10:59
Operator : MD/SY
Sample : VU0528MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc