

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059022.D
 Acq On : 28 May 2024 12:00
 Operator : MD/SY
 Sample : P2570-01ME
 Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	53	59	64	rBV3	4458	4838	1.04%	0.144%
2	1.592	87	94	115	rVB	28640	45009	9.65%	1.338%
3	1.850	134	174	176	rBV3	68719	312909	67.06%	9.303%
4	2.534	376	387	399	rBV	53980	86577	18.55%	2.574%
5	2.631	407	417	424	rBV6	1753	3287	0.70%	0.098%
6	2.763	451	458	466	rVB3	832	1368	0.29%	0.041%
7	2.801	466	470	471	rBV	301	226	0.05%	0.007%
8	2.833	477	480	481	rBV	272	168	0.04%	0.005%
9	2.882	491	495	498	rBV2	255	229	0.05%	0.007%
10	2.943	506	514	528	rBV4	2663	5318	1.14%	0.158%
11	3.023	531	539	551	rBV4	2945	5935	1.27%	0.176%
12	3.171	570	585	604	rBV	14994	39757	8.52%	1.182%
13	3.499	683	687	694	rVB2	273	339	0.07%	0.010%
14	3.557	700	705	707	rBV	192	183	0.04%	0.005%
15	3.647	730	733	737	rVB	264	188	0.04%	0.006%
16	3.679	737	743	745	rBV	331	302	0.06%	0.009%
17	3.866	797	801	806	rVB2	220	226	0.05%	0.007%
18	4.014	843	847	855	rVB2	282	337	0.07%	0.010%
19	4.075	863	866	873	rVB2	220	237	0.05%	0.007%
20	4.110	873	877	879	rBV2	265	192	0.04%	0.006%
21	4.306	936	938	942	rVB	343	202	0.04%	0.006%
22	4.441	977	980	986	rBV2	144	172	0.04%	0.005%
23	4.624	1027	1037	1072	rBV2	49429	155259	33.27%	4.616%
24	4.920	1125	1129	1130	rBV2	314	206	0.04%	0.006%
25	5.049	1154	1169	1197	rVV	83286	191099	40.95%	5.681%
26	5.194	1209	1214	1218	rBV2	222	221	0.05%	0.007%
27	5.316	1250	1252	1255	rVB	338	182	0.04%	0.005%
28	5.338	1255	1259	1262	rVB	265	193	0.04%	0.006%
29	5.364	1262	1267	1272	rBV2	198	243	0.05%	0.007%
30	5.438	1282	1290	1294	rBV2	219	317	0.07%	0.009%
31	5.708	1355	1374	1401	rBV2	164822	466629	100.00%	13.873%
32	5.878	1423	1427	1431	rVB	278	203	0.04%	0.006%
33	5.965	1449	1454	1455	rBV2	1587	1192	0.26%	0.035%
34	6.091	1488	1493	1496	rBV2	217	262	0.06%	0.008%
35	6.238	1527	1539	1559	rBV	99760	193339	41.43%	5.748%
36	6.361	1574	1577	1585	rVB3	301	425	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059022.D
 Acq On : 28 May 2024 12:00
 Operator : MD/SY
 Sample : P2570-01ME
 Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.390	1585	1586	1591	rBV2	349	234	0.05%	0.007%
38	6.415	1591	1594	1599	rVB2	384	326	0.07%	0.010%
39	6.451	1599	1605	1610	rBV2	290	415	0.09%	0.012%
40	6.521	1616	1627	1628	rBV3	2848	3042	0.65%	0.090%
41	6.592	1639	1649	1654	rBV2	2948	4279	0.92%	0.127%
42	6.682	1664	1677	1698	rVV	116350	234428	50.24%	6.970%
43	6.862	1728	1733	1740	rVB2	283	337	0.07%	0.010%
44	6.994	1771	1774	1781	rBV2	174	201	0.04%	0.006%
45	7.203	1832	1839	1840	rBV3	764	668	0.14%	0.020%
46	7.296	1863	1868	1872	rVB2	195	198	0.04%	0.006%
47	7.438	1905	1912	1914	rBV	177	184	0.04%	0.005%
48	7.489	1925	1928	1934	rVB3	236	176	0.04%	0.005%
49	7.560	1939	1950	1968	rBV	45037	81981	17.57%	2.437%
50	7.714	1996	1998	2006	rVB3	562	496	0.11%	0.015%
51	7.775	2011	2017	2027	rBV6	1155	2200	0.47%	0.065%
52	7.814	2027	2029	2037	rVB2	387	299	0.06%	0.009%
53	7.891	2040	2053	2075	rBV	128793	227645	48.79%	6.768%
54	7.978	2075	2080	2081	rBV2	1098	990	0.21%	0.029%
55	8.174	2131	2141	2161	rBV2	29360	56488	12.11%	1.679%
56	8.303	2178	2181	2184	rBV	276	181	0.04%	0.005%
57	8.357	2196	2198	2203	rVB2	347	231	0.05%	0.007%
58	8.457	2226	2229	2231	rBV	332	240	0.05%	0.007%
59	8.582	2263	2268	2273	rVB2	220	212	0.05%	0.006%
60	8.647	2273	2288	2316	rBV3	126795	351319	75.29%	10.445%
61	8.994	2394	2396	2400	rVB2	338	195	0.04%	0.006%
62	9.177	2445	2453	2458	rVV2	263	344	0.07%	0.010%
63	9.238	2469	2472	2476	rBV	256	234	0.05%	0.007%
64	9.415	2514	2527	2546	rBV	116752	217621	46.64%	6.470%
65	9.544	2563	2567	2571	rBV	277	260	0.06%	0.008%
66	9.573	2572	2576	2578	rBV	303	243	0.05%	0.007%
67	9.705	2609	2617	2623	rBV2	970	1088	0.23%	0.032%
68	9.840	2656	2659	2662	rBV2	229	167	0.04%	0.005%
69	9.955	2692	2695	2699	rVB	262	194	0.04%	0.006%
70	9.984	2700	2704	2707	rBV	269	197	0.04%	0.006%
71	10.081	2731	2734	2737	rBV	258	204	0.04%	0.006%
72	10.116	2740	2745	2752	rVB3	411	511	0.11%	0.015%
73	10.319	2804	2808	2812	rVB2	321	262	0.06%	0.008%
74	10.383	2824	2828	2831	rBV	350	248	0.05%	0.007%
75	10.402	2831	2834	2840	rVV2	314	293	0.06%	0.009%
76	10.502	2862	2865	2876	rVB	335	461	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059022.D
 Acq On : 28 May 2024 12:00
 Operator : MD/SY
 Sample : P2570-01ME
 Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	10.672	2913	2918	2921	rBV2	242	211	0.05%	0.006%
78	10.688	2921	2923	2928	rBV2	198	191	0.04%	0.006%
79	10.756	2931	2944	2962	rVV	184099	316994	67.93%	9.424%
80	11.000	3012	3020	3022	rBV2	256	306	0.07%	0.009%
81	11.486	3168	3171	3178	rVB2	341	286	0.06%	0.009%
82	11.550	3186	3191	3192	rBV	235	194	0.04%	0.006%
83	11.717	3238	3243	3246	rBV2	219	193	0.04%	0.006%
84	11.811	3262	3272	3293	rBV2	94545	155392	33.30%	4.620%
85	11.904	3297	3301	3303	rVV3	337	261	0.06%	0.008%
86	11.914	3303	3304	3308	rVB2	548	298	0.06%	0.009%
87	12.058	3343	3349	3352	rBV	256	306	0.07%	0.009%
88	12.135	3369	3373	3376	rBV	316	255	0.05%	0.008%
89	12.193	3379	3391	3412	rBV	102548	177973	38.14%	5.291%
90	12.537	3494	3498	3501	rVB2	227	188	0.04%	0.006%
91	12.711	3549	3552	3557	rVB	382	335	0.07%	0.010%
92	12.759	3564	3567	3578	rVB4	512	760	0.16%	0.023%
93	13.229	3709	3713	3716	rBV	298	306	0.07%	0.009%
94	13.682	3851	3854	3855	rBV	306	165	0.04%	0.005%
95	13.846	3901	3905	3908	rBV2	349	268	0.06%	0.008%
96	14.212	4015	4019	4024	rBV	430	320	0.07%	0.010%
97	14.833	4210	4212	4215	rBV2	288	213	0.05%	0.006%
98	15.737	4491	4493	4496	rBV2	390	218	0.05%	0.006%
99	16.126	4611	4614	4616	rBV2	488	312	0.07%	0.009%
100	16.367	4686	4689	4692	rBV3	714	597	0.13%	0.018%




Sum of corrected areas: 3363603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059022.D
Acq On : 28 May 2024 12:00
Operator : MD/SY
Sample : P2570-01ME
Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

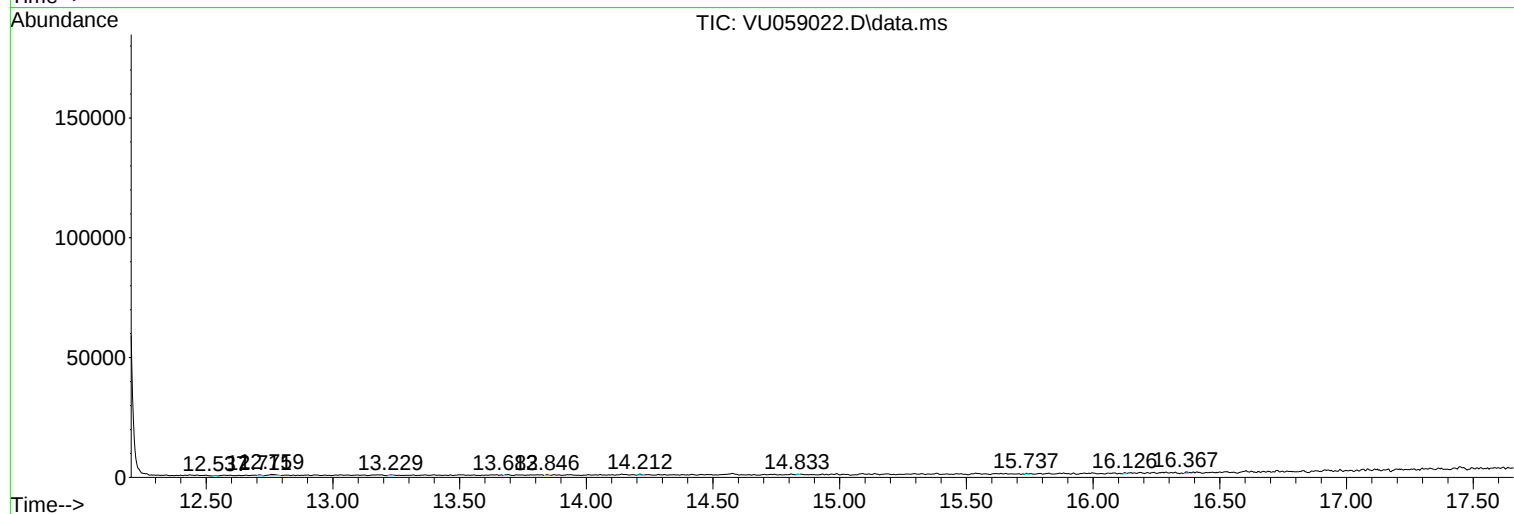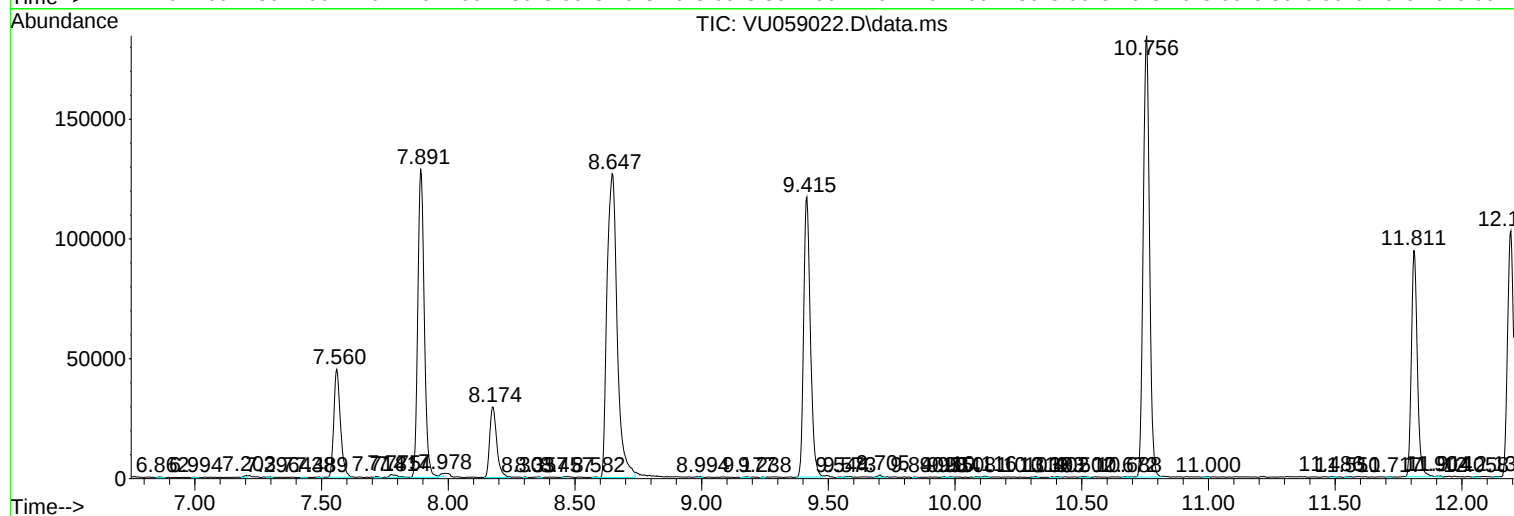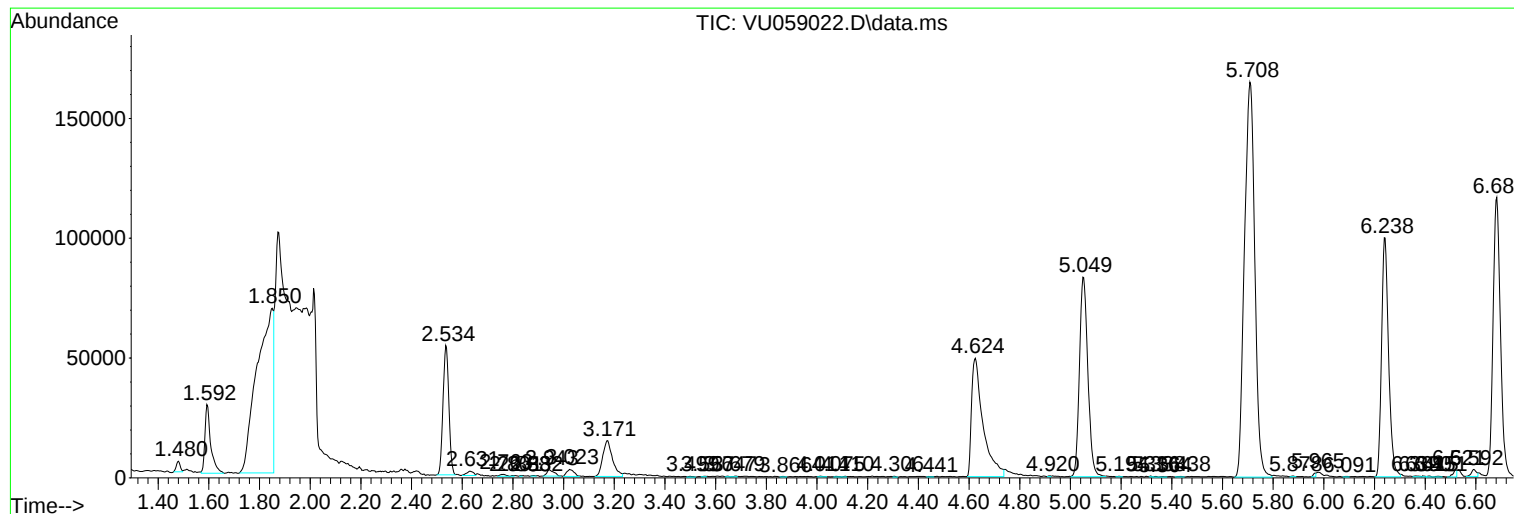

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059022.D
Acq On : 28 May 2024 12:00
Operator : MD/SY
Sample : P2570-01ME
Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059022.D
Acq On : 28 May 2024 12:00
Operator : MD/SY
Sample : P2570-01ME
Misc : 4.88g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc