

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059023.D
 Acq On : 28 May 2024 12:24
 Operator : MD/SY
 Sample : P2570-04ME
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6B2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	53	59	65	rBV	6072	7033	1.12%	0.173%
2	1.592	87	94	114	rBV	37066	63212	10.06%	1.551%
3	1.875	135	182	196	rBV6	102262	628528	100.00%	15.426%
4	2.531	375	386	397	rBV	94388	151259	24.07%	3.712%
5	3.107	561	565	568	rVB3	481	328	0.05%	0.008%
6	3.171	570	585	599	rBV2	8026	21997	3.50%	0.540%
7	3.438	665	668	672	rBV2	233	166	0.03%	0.004%
8	3.493	682	685	688	rBV2	276	179	0.03%	0.004%
9	3.541	697	700	703	rVB2	285	176	0.03%	0.004%
10	3.567	703	708	713	rBV2	270	212	0.03%	0.005%
11	4.181	895	899	903	rBV2	247	190	0.03%	0.005%
12	4.358	951	954	958	rVB2	205	159	0.03%	0.004%
13	4.480	990	992	996	rVB2	278	188	0.03%	0.005%
14	4.522	1001	1005	1009	rBV2	186	164	0.03%	0.004%
15	4.570	1014	1020	1025	rVB2	225	263	0.04%	0.006%
16	4.631	1029	1039	1078	rBV2	26553	95734	15.23%	2.350%
17	4.940	1128	1135	1140	rVB3	458	628	0.10%	0.015%
18	4.972	1140	1145	1150	rBV3	349	426	0.07%	0.010%
19	5.052	1154	1170	1193	rBV	95876	220630	35.10%	5.415%
20	5.222	1220	1223	1227	rVB	249	171	0.03%	0.004%
21	5.361	1260	1266	1268	rBV2	223	213	0.03%	0.005%
22	5.431	1285	1288	1293	rVB	351	283	0.05%	0.007%
23	5.467	1293	1299	1304	rBV	258	290	0.05%	0.007%
24	5.586	1332	1336	1342	rBV2	317	349	0.06%	0.009%
25	5.615	1342	1345	1350	rVV2	346	264	0.04%	0.006%
26	5.711	1355	1375	1403	rVV3	207902	560473	89.17%	13.756%
27	5.820	1407	1409	1412	rVV2	385	292	0.05%	0.007%
28	5.837	1412	1414	1417	rVV	406	242	0.04%	0.006%
29	5.865	1420	1423	1426	rVB3	347	249	0.04%	0.006%
30	5.939	1440	1446	1449	rBV2	233	224	0.04%	0.005%
31	5.972	1449	1456	1459	rBV4	2352	2979	0.47%	0.073%
32	6.039	1475	1477	1480	rVB2	450	250	0.04%	0.006%
33	6.136	1504	1507	1512	rVB2	222	189	0.03%	0.005%
34	6.238	1526	1539	1562	rBV	100208	200184	31.85%	4.913%
35	6.525	1620	1628	1640	rVB8	3028	6403	1.02%	0.157%
36	6.589	1640	1648	1651	rBV3	3118	3744	0.60%	0.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059023.D
 Acq On : 28 May 2024 12:24
 Operator : MD/SY
 Sample : P2570-04ME
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6B2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.682	1664	1677	1701	rVB	128490	263420	41.91%	6.465%
38	6.943	1755	1758	1764	rVV	235	181	0.03%	0.004%
39	7.100	1798	1807	1816	rBV2	399	723	0.12%	0.018%
40	7.197	1832	1837	1840	rBV2	721	780	0.12%	0.019%
41	7.222	1840	1845	1849	rBV4	752	797	0.13%	0.020%
42	7.287	1861	1865	1870	rVB3	175	174	0.03%	0.004%
43	7.383	1893	1895	1900	rVB3	253	174	0.03%	0.004%
44	7.492	1926	1929	1932	rVB2	348	228	0.04%	0.006%
45	7.521	1934	1938	1939	rBV	251	163	0.03%	0.004%
46	7.560	1939	1950	1968	rVV2	48627	92462	14.71%	2.269%
47	7.631	1968	1972	1976	rVB3	375	325	0.05%	0.008%
48	7.714	1996	1998	2004	rVB3	200	184	0.03%	0.005%
49	7.785	2011	2020	2022	rBV4	1049	1239	0.20%	0.030%
50	7.891	2040	2053	2074	rBV	202147	358681	57.07%	8.803%
51	7.991	2074	2084	2091	rVB6	1959	3573	0.57%	0.088%
52	8.049	2100	2102	2106	rBV	228	201	0.03%	0.005%
53	8.174	2130	2141	2160	rVV	33001	63369	10.08%	1.555%
54	8.351	2189	2196	2202	rVB3	480	739	0.12%	0.018%
55	8.399	2208	2211	2216	rVB2	374	306	0.05%	0.008%
56	8.451	2225	2227	2229	rBV	278	190	0.03%	0.005%
57	8.508	2242	2245	2250	rVB2	213	190	0.03%	0.005%
58	8.647	2274	2288	2322	rBV2	103974	304494	48.45%	7.473%
59	8.888	2360	2363	2365	rBV	294	209	0.03%	0.005%
60	8.901	2365	2367	2370	rVB2	346	177	0.03%	0.004%
61	8.943	2377	2380	2385	rBV2	268	245	0.04%	0.006%
62	8.988	2389	2394	2399	rVB	317	301	0.05%	0.007%
63	9.058	2413	2416	2418	rVV	297	189	0.03%	0.005%
64	9.071	2418	2420	2428	rVB2	314	297	0.05%	0.007%
65	9.299	2488	2491	2499	rBV2	198	170	0.03%	0.004%
66	9.415	2512	2527	2545	rBV	131041	239146	38.05%	5.869%
67	9.682	2606	2610	2611	rBV	633	458	0.07%	0.011%
68	9.698	2611	2615	2617	rVV2	1006	854	0.14%	0.021%
69	9.827	2652	2655	2661	rBV2	223	190	0.03%	0.005%
70	9.920	2680	2684	2689	rVV2	271	253	0.04%	0.006%
71	10.097	2735	2739	2742	rBV2	540	529	0.08%	0.013%
72	10.592	2889	2893	2895	rBV2	222	193	0.03%	0.005%
73	10.756	2930	2944	2959	rBV	177388	310961	49.47%	7.632%
74	10.881	2981	2983	2986	rVB	302	171	0.03%	0.004%
75	10.936	2993	3000	3007	rBV2	312	558	0.09%	0.014%
76	11.074	3036	3043	3048	rBV2	264	337	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059023.D
 Acq On : 28 May 2024 12:24
 Operator : MD/SY
 Sample : P2570-04ME
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH6B2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.325	3115	3121	3124	rBV2	309	351	0.06%	0.009%
78	11.486	3169	3171	3176	rBV	468	347	0.06%	0.009%
79	11.721	3240	3244	3247	rBV2	228	217	0.03%	0.005%
80	11.811	3261	3272	3291	rBV	108978	178273	28.36%	4.375%
81	12.029	3335	3340	3344	rBV2	272	296	0.05%	0.007%
82	12.190	3379	3390	3413	rBV	165278	273409	43.50%	6.710%
83	12.396	3451	3454	3457	rBV	295	227	0.04%	0.006%
84	12.508	3486	3489	3493	rBV2	319	235	0.04%	0.006%
85	12.598	3513	3517	3523	rBV2	315	384	0.06%	0.009%
86	12.656	3532	3535	3538	rBV2	232	164	0.03%	0.004%
87	12.766	3564	3569	3575	rBV2	526	677	0.11%	0.017%
88	13.579	3818	3822	3824	rBV	237	167	0.03%	0.004%
89	14.007	3952	3955	3959	rBV2	360	336	0.05%	0.008%
90	14.392	4072	4075	4077	rBV2	294	241	0.04%	0.006%
91	14.524	4114	4116	4118	rBV3	290	174	0.03%	0.004%
92	14.540	4118	4121	4124	rVV2	361	295	0.05%	0.007%
93	14.653	4153	4156	4164	rBV2	493	502	0.08%	0.012%
94	14.814	4204	4206	4209	rBV	350	246	0.04%	0.006%
95	14.868	4221	4223	4227	rVB2	366	166	0.03%	0.004%
96	14.939	4242	4245	4247	rBV	323	235	0.04%	0.006%
97	15.106	4293	4297	4300	rBV2	383	421	0.07%	0.010%
98	15.151	4308	4311	4314	rBV	534	397	0.06%	0.010%
99	15.942	4555	4557	4559	rBV	546	246	0.04%	0.006%
100	16.386	4693	4695	4697	rBV2	674	383	0.06%	0.009%




Sum of corrected areas: 4074491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059023.D
Acq On : 28 May 2024 12:24
Operator : MD/SY
Sample : P2570-04ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6B2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

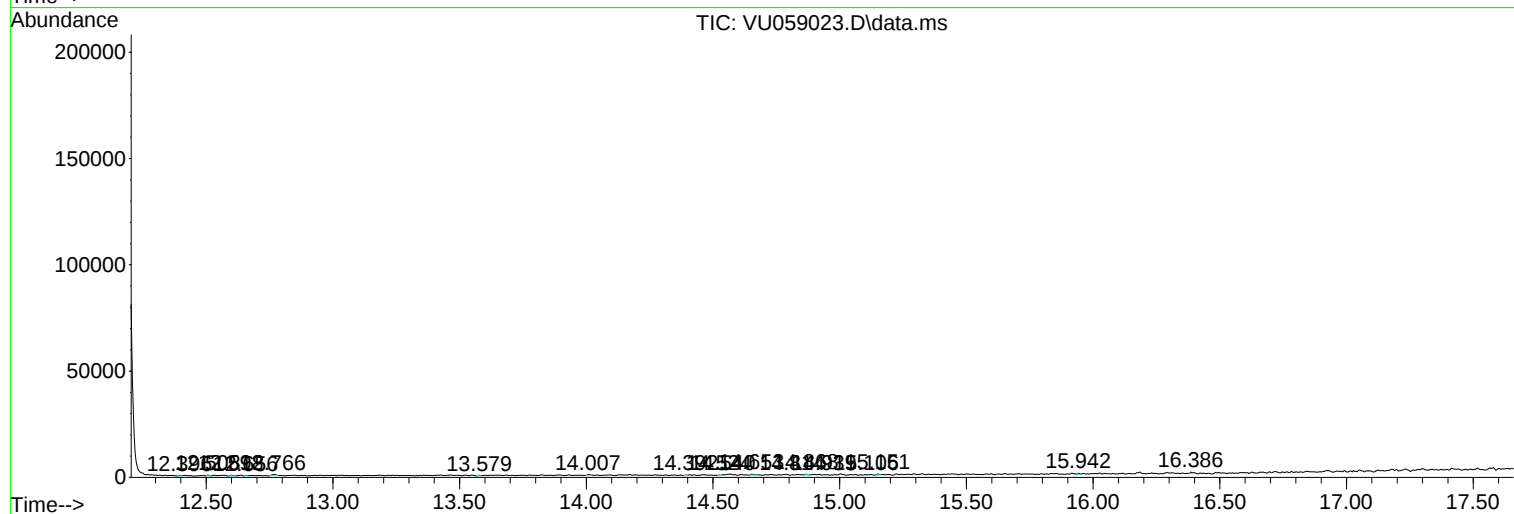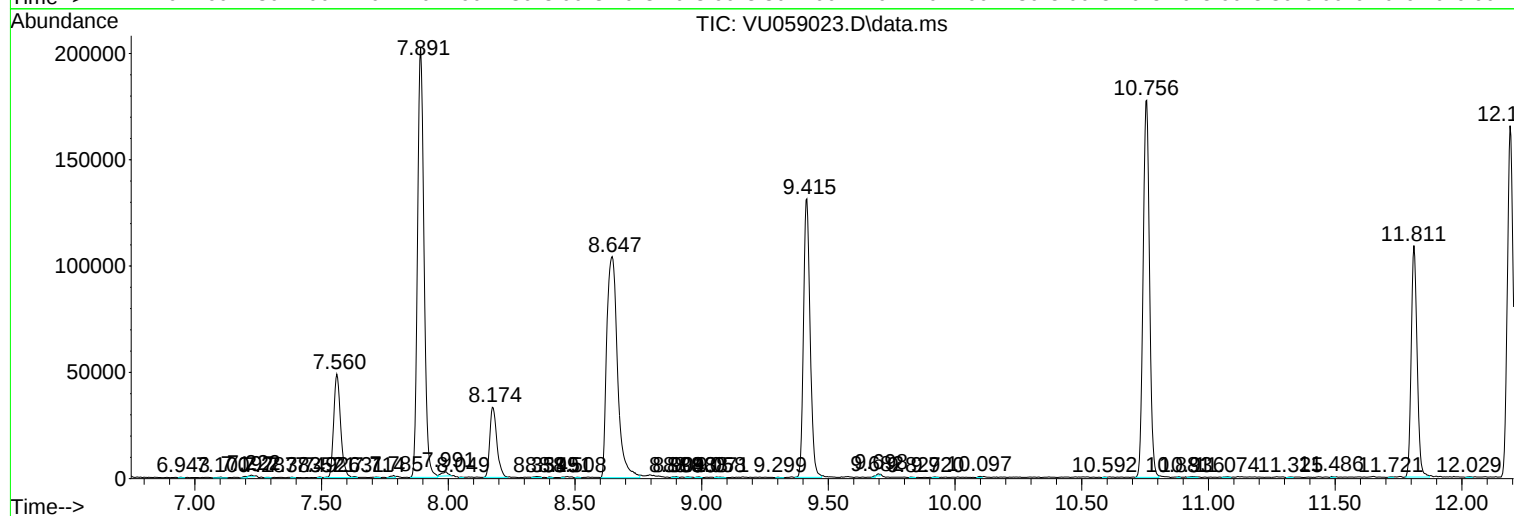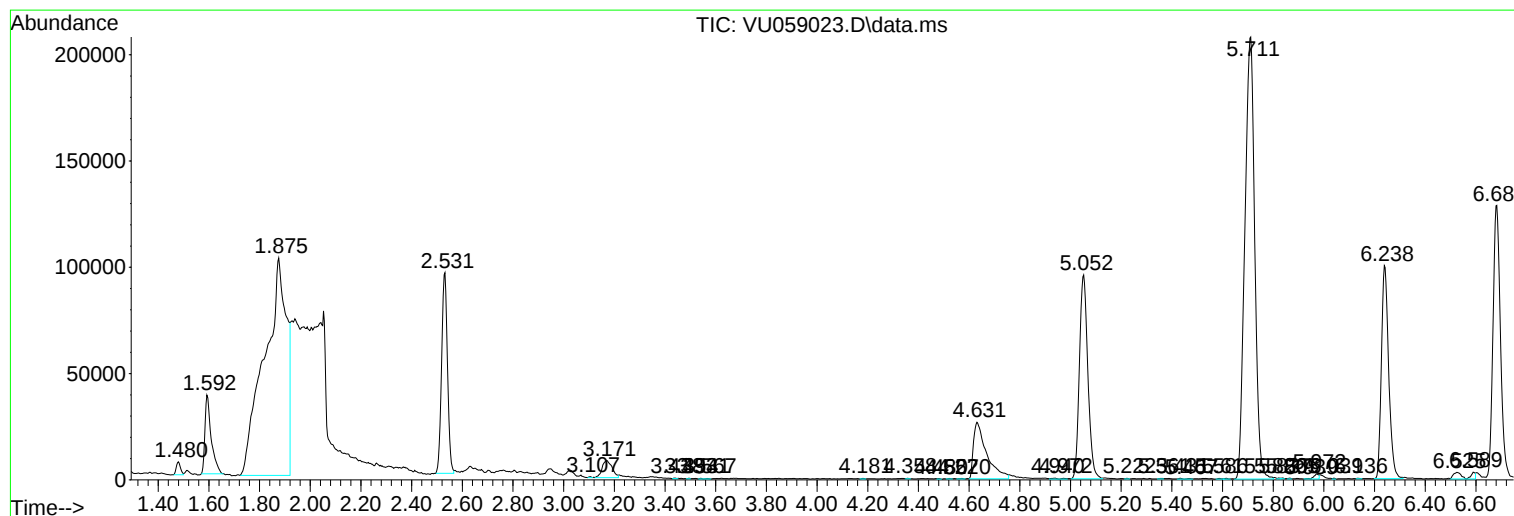

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059023.D
Acq On : 28 May 2024 12:24
Operator : MD/SY
Sample : P2570-04ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6B2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059023.D
Acq On : 28 May 2024 12:24
Operator : MD/SY
Sample : P2570-04ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH6B2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc