

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059024.D
 Acq On : 28 May 2024 12:49
 Operator : MD/SY
 Sample : P2566-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.354	15	20	29	rBB	8953	9724	1.29%	0.196%
2	1.483	55	60	66	rVB4	3447	3665	0.48%	0.074%
3	1.592	86	94	109	rBV	94931	120942	15.98%	2.444%
4	1.888	178	186	206	rVB	74632	109180	14.43%	2.206%
5	2.055	236	238	242	rBV2	875	460	0.06%	0.009%
6	2.139	260	264	265	rBV3	1371	1045	0.14%	0.021%
7	2.232	289	293	297	rBV3	570	521	0.07%	0.011%
8	2.554	381	393	406	rBV	148418	240831	31.83%	4.866%
9	2.673	426	430	434	rBV3	376	376	0.05%	0.008%
10	2.779	455	463	477	rVB3	1743	2816	0.37%	0.057%
11	2.843	479	483	486	rBV2	486	397	0.05%	0.008%
12	2.933	508	511	513	rBV2	227	176	0.02%	0.004%
13	3.033	535	542	551	rVB4	1724	2715	0.36%	0.055%
14	3.168	574	584	585	rBV4	1063	1253	0.17%	0.025%
15	3.528	691	696	700	rBV2	207	229	0.03%	0.005%
16	3.631	725	728	733	rBV2	236	248	0.03%	0.005%
17	3.657	733	736	741	rVV2	199	193	0.03%	0.004%
18	3.711	750	753	757	rVB2	231	182	0.02%	0.004%
19	3.740	757	762	766	rBV2	228	214	0.03%	0.004%
20	3.792	773	778	780	rBV	287	249	0.03%	0.005%
21	3.866	797	801	807	rVV2	262	280	0.04%	0.006%
22	4.097	867	873	876	rBV2	208	224	0.03%	0.005%
23	4.181	896	899	904	rBV	257	188	0.02%	0.004%
24	4.493	989	996	999	rBV2	221	176	0.02%	0.004%
25	4.608	1022	1032	1070	rBV	71808	182459	24.11%	3.687%
26	4.949	1135	1138	1140	rBV	266	216	0.03%	0.004%
27	5.049	1154	1169	1195	rBV	131549	293677	38.81%	5.934%
28	5.448	1289	1293	1295	rVV2	271	211	0.03%	0.004%
29	5.512	1308	1313	1319	rVB2	283	306	0.04%	0.006%
30	5.647	1349	1355	1356	rBV2	269	207	0.03%	0.004%
31	5.714	1356	1376	1405	rVV2	274466	756646	100.00%	15.289%
32	5.814	1405	1407	1409	rBV3	416	197	0.03%	0.004%
33	5.933	1442	1444	1448	rVB2	341	194	0.03%	0.004%
34	6.023	1469	1472	1477	rBV2	375	296	0.04%	0.006%
35	6.187	1520	1523	1526	rBV	238	189	0.02%	0.004%
36	6.242	1528	1540	1559	rBV	154514	293042	38.73%	5.921%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059024.D
 Acq On : 28 May 2024 12:49
 Operator : MD/SY
 Sample : P2566-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.374	1577	1581	1587	rVB2	202	301	0.04%	0.006%
38	6.451	1601	1605	1607	rBV	318	244	0.03%	0.005%
39	6.531	1620	1630	1640	rVB7	2573	5089	0.67%	0.103%
40	6.602	1650	1652	1654	rBV2	336	187	0.02%	0.004%
41	6.682	1663	1677	1704	rBV	175163	348699	46.08%	7.046%
42	6.910	1741	1748	1750	rBV2	164	191	0.03%	0.004%
43	7.203	1835	1839	1842	rBV3	454	322	0.04%	0.007%
44	7.229	1845	1847	1851	rVB	432	256	0.03%	0.005%
45	7.457	1916	1918	1926	rVB2	182	175	0.02%	0.004%
46	7.502	1929	1932	1938	rVV2	231	180	0.02%	0.004%
47	7.560	1938	1950	1971	rVV2	85208	152252	20.12%	3.077%
48	7.634	1971	1973	1977	rVB	611	363	0.05%	0.007%
49	7.804	2022	2026	2034	rVB2	182	278	0.04%	0.006%
50	7.849	2034	2040	2041	rBV	286	252	0.03%	0.005%
51	7.891	2041	2053	2071	rBV	302269	526882	69.63%	10.647%
52	8.107	2117	2120	2124	rVB2	283	190	0.03%	0.004%
53	8.174	2129	2141	2157	rBV	59363	100911	13.34%	2.039%
54	8.258	2165	2167	2171	rVB3	315	248	0.03%	0.005%
55	8.370	2198	2202	2207	rVB2	303	280	0.04%	0.006%
56	8.451	2223	2227	2228	rBV2	328	242	0.03%	0.005%
57	8.531	2248	2252	2258	rVB2	348	283	0.04%	0.006%
58	8.586	2264	2269	2271	rBV	225	203	0.03%	0.004%
59	8.627	2271	2282	2319	rVV	187701	363154	48.00%	7.338%
60	8.785	2328	2331	2334	rBV3	719	554	0.07%	0.011%
61	8.856	2349	2353	2355	rBV2	313	250	0.03%	0.005%
62	8.933	2374	2377	2380	rVB2	328	198	0.03%	0.004%
63	8.959	2380	2385	2389	rBV2	297	343	0.05%	0.007%
64	9.412	2514	2526	2548	rBV	213608	357326	47.22%	7.220%
65	9.695	2611	2614	2617	rBV3	370	247	0.03%	0.005%
66	9.859	2662	2665	2669	rVB	340	227	0.03%	0.005%
67	9.946	2688	2692	2695	rBV	226	195	0.03%	0.004%
68	10.052	2721	2725	2731	rVB2	329	360	0.05%	0.007%
69	10.094	2735	2738	2741	rBV3	317	217	0.03%	0.004%
70	10.325	2807	2810	2817	rBV2	238	256	0.03%	0.005%
71	10.422	2836	2840	2848	rBV	368	337	0.04%	0.007%
72	10.534	2872	2875	2881	rVB2	240	227	0.03%	0.005%
73	10.640	2904	2908	2911	rBV	297	251	0.03%	0.005%
74	10.750	2929	2942	2961	rBV	227103	367263	48.54%	7.421%
75	10.820	2961	2964	2971	rVB3	570	679	0.09%	0.014%
76	10.865	2971	2978	2979	rBV	231	248	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059024.D
 Acq On : 28 May 2024 12:49
 Operator : MD/SY
 Sample : P2566-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.023	3023	3027	3031	rBV2	209	187	0.02%	0.004%
78	11.049	3032	3035	3037	rBV2	290	200	0.03%	0.004%
79	11.277	3101	3106	3109	rBV	294	329	0.04%	0.007%
80	11.315	3115	3118	3120	rBV	257	176	0.02%	0.004%
81	11.454	3157	3161	3164	rBV	209	188	0.02%	0.004%
82	11.624	3210	3214	3218	rBV2	220	245	0.03%	0.005%
83	11.807	3260	3271	3294	rBV	169063	278927	36.86%	5.636%
84	12.013	3330	3335	3338	rBV2	363	353	0.05%	0.007%
85	12.187	3377	3389	3412	rBV	241985	409792	54.16%	8.281%
86	12.383	3447	3450	3453	rVB	483	259	0.03%	0.005%
87	12.717	3551	3554	3558	rBV	199	195	0.03%	0.004%
88	12.942	3621	3624	3630	rVB2	535	496	0.07%	0.010%
89	12.987	3633	3638	3642	rBV3	317	317	0.04%	0.006%
90	13.110	3673	3676	3678	rBV2	254	190	0.03%	0.004%
91	13.434	3774	3777	3779	rBV	270	179	0.02%	0.004%
92	13.457	3782	3784	3788	rBV	207	196	0.03%	0.004%
93	13.521	3801	3804	3810	rVB2	468	359	0.05%	0.007%
94	13.547	3810	3812	3815	rBV2	278	201	0.03%	0.004%
95	13.743	3870	3873	3876	rVB2	322	193	0.03%	0.004%
96	14.068	3971	3974	3977	rVB2	359	197	0.03%	0.004%
97	14.093	3978	3982	3987	rBV2	468	538	0.07%	0.011%
98	14.283	4038	4041	4046	rBV	310	356	0.05%	0.007%
99	14.528	4115	4117	4121	rBV2	368	204	0.03%	0.004%
100	14.646	4151	4154	4157	rBV	358	276	0.04%	0.006%




Sum of corrected areas: 4948837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059024.D
Acq On : 28 May 2024 12:49
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

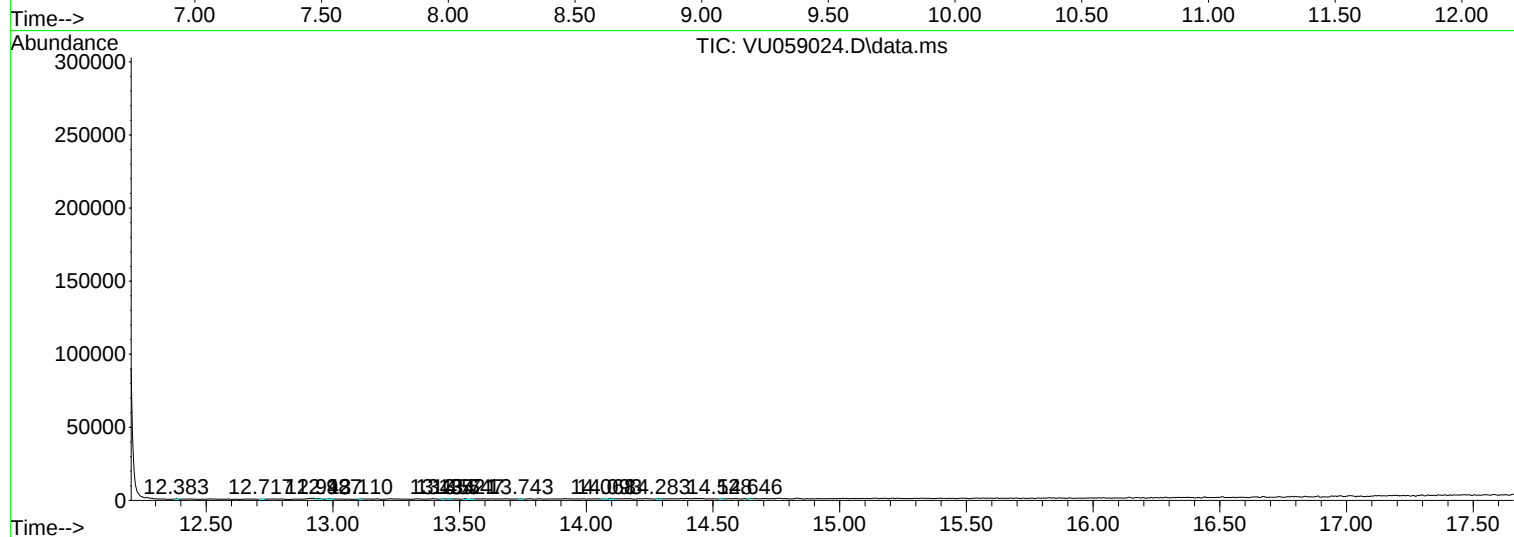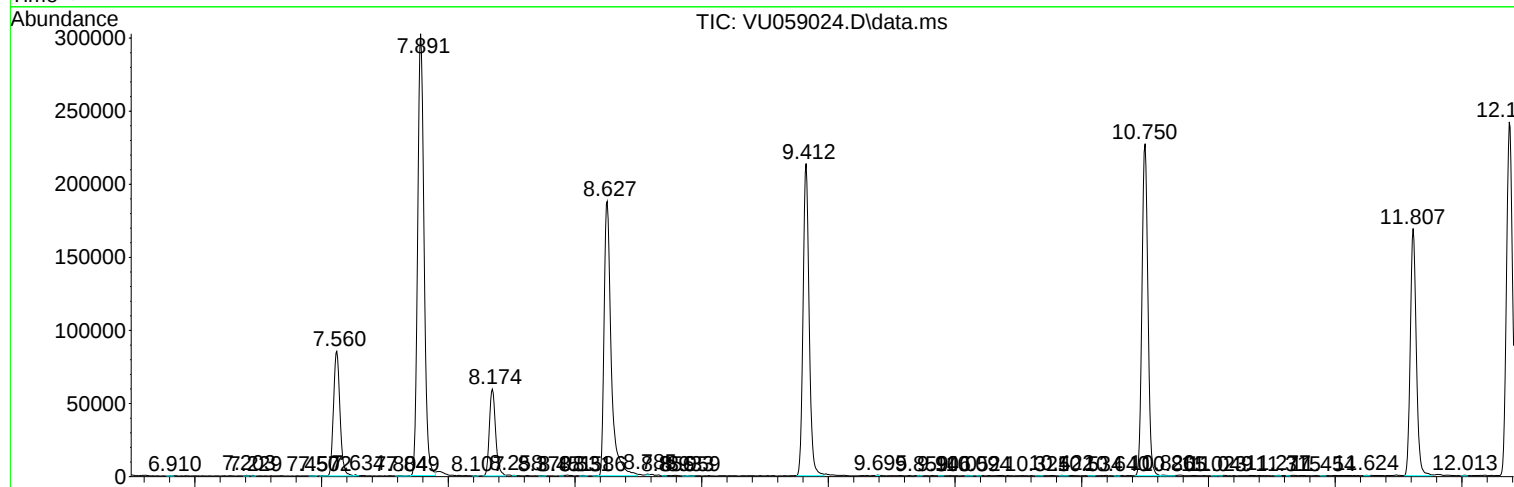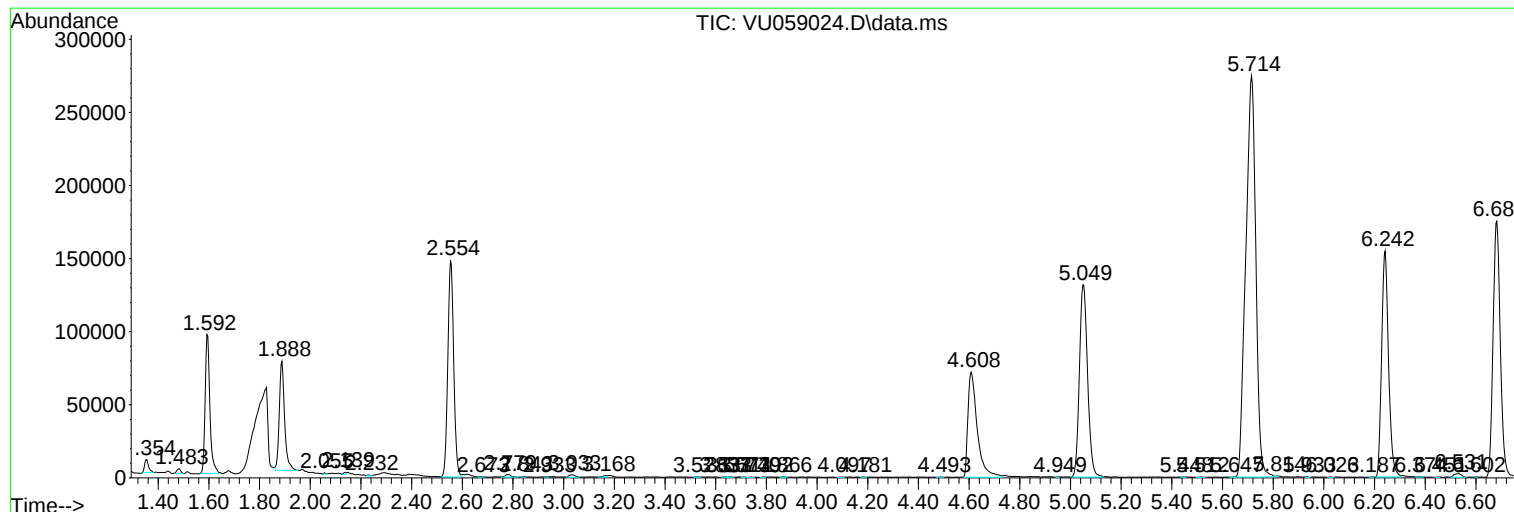

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059024.D
Acq On : 28 May 2024 12:49
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059024.D
Acq On : 28 May 2024 12:49
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------