

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059026.D
 Acq On : 28 May 2024 13:38
 Operator : MD/SY
 Sample : P2566-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU059026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.352	15	19	26	rBV4	3164	3430	0.43%	0.055%
2	1.480	55	59	65	rVB2	3319	3573	0.44%	0.058%
3	1.593	86	94	114	rBV	95546	123449	15.34%	1.990%
4	1.872	133	181	202	rBV3	185610	543284	67.49%	8.759%
5	2.474	365	368	370	rBV3	333	188	0.02%	0.003%
6	2.551	379	392	407	rBV	155953	253949	31.55%	4.094%
7	2.712	439	442	449	rVB3	332	293	0.04%	0.005%
8	2.760	453	457	458	rVV	575	432	0.05%	0.007%
9	2.773	458	461	470	rVB2	1353	1834	0.23%	0.030%
10	2.843	479	483	484	rBV	242	172	0.02%	0.003%
11	2.930	507	510	512	rBV	282	189	0.02%	0.003%
12	3.027	532	540	542	rBV4	1206	1448	0.18%	0.023%
13	3.445	667	670	674	rBV2	185	150	0.02%	0.002%
14	3.676	739	742	748	rVB3	305	213	0.03%	0.003%
15	3.705	748	751	753	rBV	227	170	0.02%	0.003%
16	3.866	798	801	803	rBV2	229	158	0.02%	0.003%
17	4.052	855	859	860	rBV	185	145	0.02%	0.002%
18	4.236	911	916	920	rBV2	187	187	0.02%	0.003%
19	4.306	936	938	941	rBV	224	127	0.02%	0.002%
20	4.467	985	988	993	rBV2	202	174	0.02%	0.003%
21	4.573	1017	1021	1023	rBV2	179	142	0.02%	0.002%
22	4.612	1023	1033	1063	rBV	73844	202248	25.13%	3.261%
23	4.917	1122	1128	1133	rBV2	305	414	0.05%	0.007%
24	5.049	1154	1169	1191	rBV	140923	317478	39.44%	5.119%
25	5.220	1219	1222	1226	rVB3	345	278	0.03%	0.004%
26	5.281	1239	1241	1247	rVB4	392	398	0.05%	0.006%
27	5.361	1263	1266	1268	rBV	250	197	0.02%	0.003%
28	5.406	1272	1280	1283	rVV2	270	378	0.05%	0.006%
29	5.538	1318	1321	1323	rBV	199	133	0.02%	0.002%
30	5.580	1330	1334	1337	rBV2	179	148	0.02%	0.002%
31	5.599	1337	1340	1343	rBV	211	128	0.02%	0.002%
32	5.715	1355	1376	1407	rBV2	296787	804959	100.00%	12.978%
33	5.969	1452	1455	1458	rBV2	386	260	0.03%	0.004%
34	6.030	1471	1474	1479	rBV3	260	253	0.03%	0.004%
35	6.113	1496	1500	1504	rBV2	344	238	0.03%	0.004%
36	6.142	1504	1509	1518	rVV2	198	353	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059026.D
 Acq On : 28 May 2024 13:38
 Operator : MD/SY
 Sample : P2566-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.239	1525	1539	1562	rBV	222923	429650	53.38%	6.927%
38	6.396	1585	1588	1594	rBV2	343	365	0.05%	0.006%
39	6.470	1607	1611	1613	rBV2	238	176	0.02%	0.003%
40	6.535	1620	1631	1643	rVB6	8388	16529	2.05%	0.266%
41	6.593	1643	1649	1657	rBV2	755	1165	0.14%	0.019%
42	6.679	1663	1676	1695	rBV	188072	366708	45.56%	5.912%
43	6.792	1708	1711	1716	rVV2	228	211	0.03%	0.003%
44	6.814	1716	1718	1724	rVB2	382	347	0.04%	0.006%
45	6.843	1724	1727	1732	rBV2	238	206	0.03%	0.003%
46	7.084	1799	1802	1805	rVB	251	149	0.02%	0.002%
47	7.129	1813	1816	1820	rVV2	208	185	0.02%	0.003%
48	7.152	1820	1823	1828	rVV2	185	186	0.02%	0.003%
49	7.200	1834	1838	1841	rBV2	367	364	0.05%	0.006%
50	7.255	1851	1855	1857	rBV	197	149	0.02%	0.002%
51	7.290	1862	1866	1870	rBV	339	294	0.04%	0.005%
52	7.416	1901	1905	1910	rVB	239	214	0.03%	0.003%
53	7.441	1910	1913	1916	rBV2	172	127	0.02%	0.002%
54	7.557	1938	1949	1969	rBV	92324	167630	20.82%	2.703%
55	7.650	1975	1978	1981	rBV	265	168	0.02%	0.003%
56	7.686	1987	1989	1993	rBV2	316	194	0.02%	0.003%
57	7.731	2000	2003	2006	rBV2	339	282	0.04%	0.005%
58	7.792	2020	2022	2027	rVB2	171	144	0.02%	0.002%
59	7.892	2037	2053	2075	rBV	325424	568890	70.67%	9.172%
60	8.100	2115	2118	2119	rVV2	234	138	0.02%	0.002%
61	8.123	2123	2125	2130	rBV2	254	194	0.02%	0.003%
62	8.174	2130	2141	2164	rBV2	64062	110489	13.73%	1.781%
63	8.515	2240	2247	2252	rBV2	261	328	0.04%	0.005%
64	8.547	2252	2257	2263	rBV5	889	1059	0.13%	0.017%
65	8.631	2271	2283	2319	rBV	209526	423009	52.55%	6.820%
66	8.914	2368	2371	2373	rBV3	245	181	0.02%	0.003%
67	9.033	2405	2408	2411	rVB2	320	215	0.03%	0.003%
68	9.258	2475	2478	2480	rBV	191	147	0.02%	0.002%
69	9.412	2514	2526	2551	rBV	312564	521994	64.85%	8.416%
70	9.570	2571	2575	2582	rVB2	424	506	0.06%	0.008%
71	9.692	2606	2613	2614	rBV	1349	891	0.11%	0.014%
72	10.104	2737	2741	2747	rVB2	438	535	0.07%	0.009%
73	10.136	2747	2751	2754	rBV	233	148	0.02%	0.002%
74	10.213	2772	2775	2778	rBV	277	202	0.03%	0.003%
75	10.242	2778	2784	2787	rBV3	500	520	0.06%	0.008%
76	10.383	2825	2828	2830	rBV3	278	206	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059026.D
 Acq On : 28 May 2024 13:38
 Operator : MD/SY
 Sample : P2566-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	10.544	2876	2878	2880	rBV	255	137	0.02%	0.002%
78	10.750	2930	2942	2966	rBV	260446	426209	52.95%	6.872%
79	10.875	2978	2981	2983	rBV3	377	303	0.04%	0.005%
80	10.885	2983	2984	2990	rVB	831	648	0.08%	0.010%
81	10.936	2997	3000	3004	rVB2	234	171	0.02%	0.003%
82	11.094	3047	3049	3051	rBV	252	137	0.02%	0.002%
83	11.290	3107	3110	3115	rBV2	240	180	0.02%	0.003%
84	11.409	3144	3147	3153	rBV3	429	376	0.05%	0.006%
85	11.460	3160	3163	3166	rBV	329	205	0.03%	0.003%
86	11.624	3211	3214	3217	rBV2	197	164	0.02%	0.003%
87	11.705	3231	3239	3242	rBV5	1160	1089	0.14%	0.018%
88	11.808	3259	3271	3294	rBV	260459	426513	52.99%	6.877%
89	12.120	3361	3368	3371	rBV2	532	642	0.08%	0.010%
90	12.187	3376	3389	3410	rBV	279473	464564	57.71%	7.490%
91	12.319	3427	3430	3434	rVB2	600	488	0.06%	0.008%
92	12.454	3469	3472	3475	rBV	283	211	0.03%	0.003%
93	12.808	3579	3582	3585	rBV	337	201	0.02%	0.003%
94	12.840	3589	3592	3596	rBV2	504	448	0.06%	0.007%
95	12.907	3607	3613	3616	rBV5	1173	1514	0.19%	0.024%
96	13.058	3657	3660	3662	rBV2	303	213	0.03%	0.003%
97	13.345	3746	3749	3751	rBV	318	205	0.03%	0.003%
98	13.853	3905	3907	3910	rVB	303	138	0.02%	0.002%
99	14.628	4144	4148	4150	rBV3	397	396	0.05%	0.006%
100	15.129	4301	4304	4309	rBV3	548	572	0.07%	0.009%




Sum of corrected areas: 6202389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059026.D
Acq On : 28 May 2024 13:38
Operator : MD/SY
Sample : P2566-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

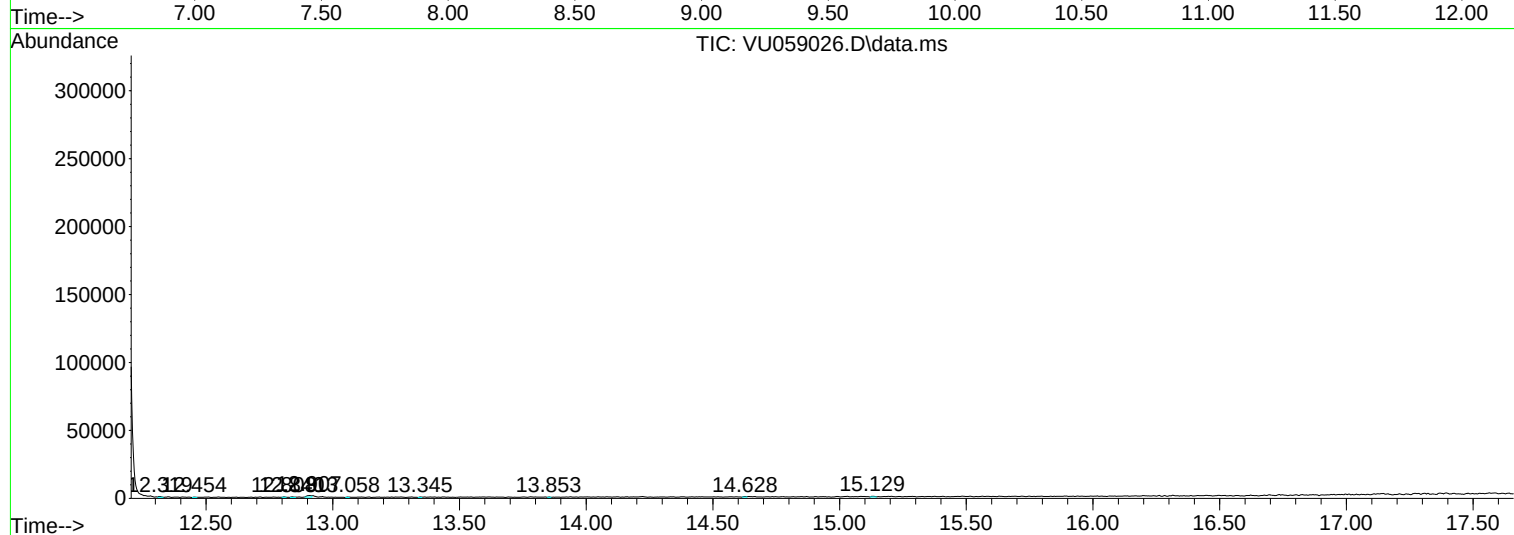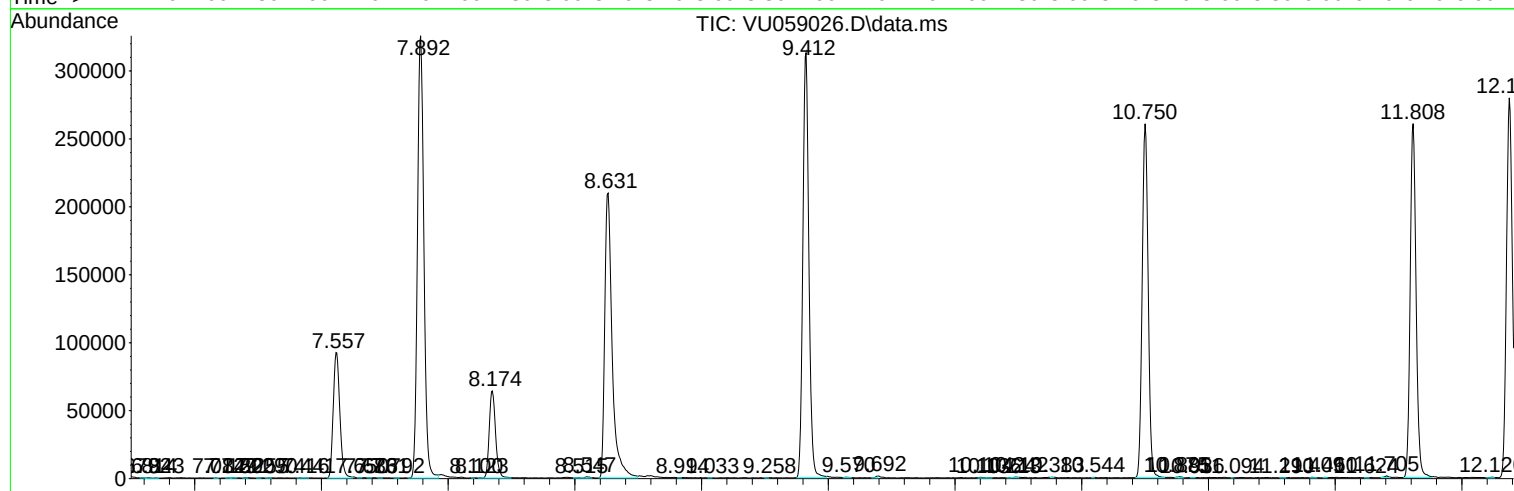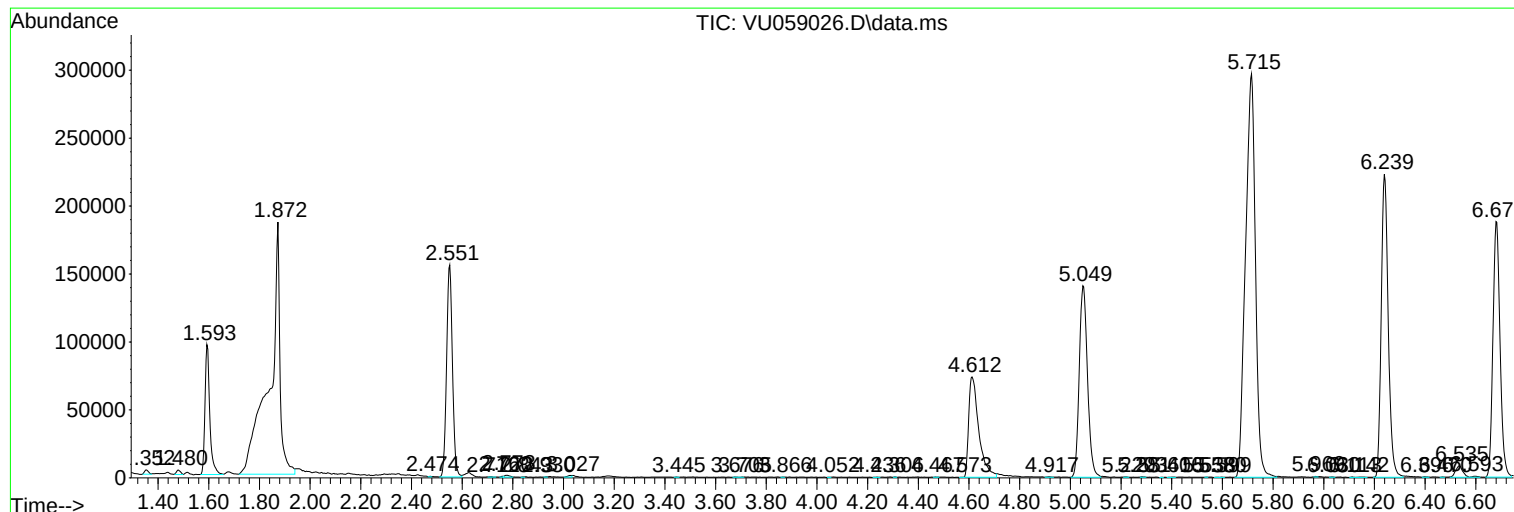

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059026.D
Acq On : 28 May 2024 13:38
Operator : MD/SY
Sample : P2566-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059026.D
Acq On : 28 May 2024 13:38
Operator : MD/SY
Sample : P2566-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------