

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059041.D
 Acq On : 28 May 2024 19:46
 Operator : MD/SY
 Sample : P2570-13ME
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5Q9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	126	rVB	63833	120140	14.71%	2.076%
2	2.528	375	385	401	rVB	153091	251844	30.83%	4.351%
3	3.171	570	585	603	rBV	10012	27181	3.33%	0.470%
4	3.370	643	647	650	rVB4	384	271	0.03%	0.005%
5	3.528	693	696	699	rVB	218	117	0.01%	0.002%
6	3.592	713	716	718	rBV	230	158	0.02%	0.003%
7	3.644	727	732	733	rBV2	401	298	0.04%	0.005%
8	3.689	743	746	749	rBV	152	112	0.01%	0.002%
9	3.730	755	759	762	rBV2	197	185	0.02%	0.003%
10	3.785	772	776	779	rBV2	279	271	0.03%	0.005%
11	3.859	797	799	801	rBV2	121	69	0.01%	0.001%
12	3.920	816	818	824	rVB	234	177	0.02%	0.003%
13	3.952	824	828	829	rBV	109	84	0.01%	0.001%
14	4.033	851	853	854	rBV	147	44	0.01%	0.001%
15	4.081	866	868	873	rVB2	102	62	0.01%	0.001%
16	4.116	873	879	882	rBV	160	192	0.02%	0.003%
17	4.238	911	917	918	rBV	231	165	0.02%	0.003%
18	4.345	944	950	953	rBV	183	229	0.03%	0.004%
19	4.390	961	964	966	rBV	123	83	0.01%	0.001%
20	4.438	976	979	981	rBV	117	78	0.01%	0.001%
21	4.537	1008	1010	1011	rBV	96	45	0.01%	0.001%
22	4.566	1016	1019	1022	rBV2	205	161	0.02%	0.003%
23	4.627	1027	1038	1085	rBV	59947	213184	26.10%	3.683%
24	5.049	1153	1169	1196	rBV2	136779	313026	38.32%	5.408%
25	5.251	1229	1232	1235	rVB2	300	192	0.02%	0.003%
26	5.283	1241	1242	1243	rBV2	104	23	0.00%	0.000%
27	5.299	1243	1247	1249	rBV2	143	119	0.01%	0.002%
28	5.406	1276	1280	1283	rBV	249	184	0.02%	0.003%
29	5.454	1292	1295	1296	rBV2	109	59	0.01%	0.001%
30	5.505	1307	1311	1314	rBV	258	176	0.02%	0.003%
31	5.525	1314	1317	1319	rBV2	156	103	0.01%	0.002%
32	5.563	1325	1329	1331	rBV	133	92	0.01%	0.002%
33	5.708	1356	1374	1406	rBV2	310525	816848	100.00%	14.113%
34	5.971	1448	1456	1458	rBV6	2627	3116	0.38%	0.054%
35	6.055	1480	1482	1487	rVB	291	213	0.03%	0.004%
36	6.081	1488	1490	1498	rBV2	229	279	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059041.D
 Acq On : 28 May 2024 19:46
 Operator : MD/SY
 Sample : P2570-13ME
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5Q9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.116	1499	1501	1505	rBV2	186	128	0.02%	0.002%
38	6.152	1510	1512	1515	rBV2	149	77	0.01%	0.001%
39	6.238	1527	1539	1562	rBV	243411	481620	58.96%	8.321%
40	6.418	1593	1595	1596	rBV	152	68	0.01%	0.001%
41	6.428	1596	1598	1604	rVB3	177	145	0.02%	0.003%
42	6.518	1619	1626	1639	rVB8	4410	8915	1.09%	0.154%
43	6.595	1641	1650	1663	rBV3	3840	8620	1.06%	0.149%
44	6.682	1664	1677	1699	rVB	184639	376010	46.03%	6.497%
45	6.798	1712	1713	1716	rBV2	317	177	0.02%	0.003%
46	6.814	1716	1718	1721	rVB	256	107	0.01%	0.002%
47	6.846	1726	1728	1729	rBV	226	104	0.01%	0.002%
48	6.897	1741	1744	1745	rBV2	155	86	0.01%	0.001%
49	7.052	1790	1792	1795	rVB	207	95	0.01%	0.002%
50	7.081	1799	1801	1807	rVB2	213	149	0.02%	0.003%
51	7.116	1807	1812	1813	rBV2	145	124	0.02%	0.002%
52	7.180	1828	1832	1833	rBV	194	129	0.02%	0.002%
53	7.222	1841	1845	1849	rVB5	968	860	0.11%	0.015%
54	7.328	1875	1878	1882	rVB3	320	175	0.02%	0.003%
55	7.348	1882	1884	1885	rBV	167	42	0.01%	0.001%
56	7.373	1889	1892	1896	rBV2	116	96	0.01%	0.002%
57	7.454	1912	1917	1918	rBV	295	201	0.02%	0.003%
58	7.486	1922	1927	1928	rBV2	395	258	0.03%	0.004%
59	7.560	1938	1950	1973	rBV	89420	167175	20.47%	2.888%
60	7.685	1985	1989	1991	rBV2	185	164	0.02%	0.003%
61	7.705	1991	1995	1996	rBV2	249	147	0.02%	0.003%
62	7.759	2009	2012	2014	rBV2	193	102	0.01%	0.002%
63	7.782	2014	2019	2024	rBV2	587	541	0.07%	0.009%
64	7.827	2031	2033	2040	rVB2	185	154	0.02%	0.003%
65	7.891	2040	2053	2075	rBV	323270	579186	70.90%	10.007%
66	8.055	2102	2104	2112	rVB3	507	437	0.05%	0.008%
67	8.123	2122	2125	2128	rBV3	192	124	0.02%	0.002%
68	8.174	2130	2141	2157	rBV	59624	111759	13.68%	1.931%
69	8.399	2207	2211	2213	rBV2	189	131	0.02%	0.002%
70	8.463	2227	2231	2233	rBV2	278	251	0.03%	0.004%
71	8.518	2244	2248	2251	rBV2	195	175	0.02%	0.003%
72	8.647	2274	2288	2323	rBV2	148489	417113	51.06%	7.207%
73	9.020	2400	2404	2405	rBV2	242	150	0.02%	0.003%
74	9.209	2460	2463	2467	rVB2	235	184	0.02%	0.003%
75	9.306	2490	2493	2498	rBV2	237	193	0.02%	0.003%
76	9.415	2513	2527	2552	rBV	332670	595439	72.89%	10.288%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
 Data File : VU059041.D
 Acq On : 28 May 2024 19:46
 Operator : MD/SY
 Sample : P2570-13ME
 Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5Q9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	9.557	2568	2571	2572	rBV	220	114	0.01%	0.002%
78	9.698	2607	2615	2622	rBV5	1634	2508	0.31%	0.043%
79	9.843	2657	2660	2662	rBV	232	155	0.02%	0.003%
80	9.881	2669	2672	2674	rBV	233	166	0.02%	0.003%
81	9.936	2687	2689	2691	rBV2	176	104	0.01%	0.002%
82	10.026	2715	2717	2718	rBV	176	54	0.01%	0.001%
83	10.106	2737	2742	2748	rVB3	503	596	0.07%	0.010%
84	10.254	2784	2788	2793	rBV2	282	269	0.03%	0.005%
85	10.756	2930	2944	2963	rBV	238394	407068	49.83%	7.033%
86	10.878	2979	2982	2983	rBV	370	179	0.02%	0.003%
87	10.891	2983	2986	2989	rVB2	366	279	0.03%	0.005%
88	10.913	2989	2993	2994	rBV	171	124	0.02%	0.002%
89	11.132	3058	3061	3066	rVB3	391	278	0.03%	0.005%
90	11.399	3141	3144	3147	rBV2	220	139	0.02%	0.002%
91	11.810	3260	3272	3299	rBV	266646	441270	54.02%	7.624%
92	12.003	3330	3332	3335	rBV2	456	249	0.03%	0.004%
93	12.190	3379	3390	3408	rBV	265495	433120	53.02%	7.483%




Sum of corrected areas: 5787863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059041.D
Acq On : 28 May 2024 19:46
Operator : MD/SY
Sample : P2570-13ME
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5Q9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

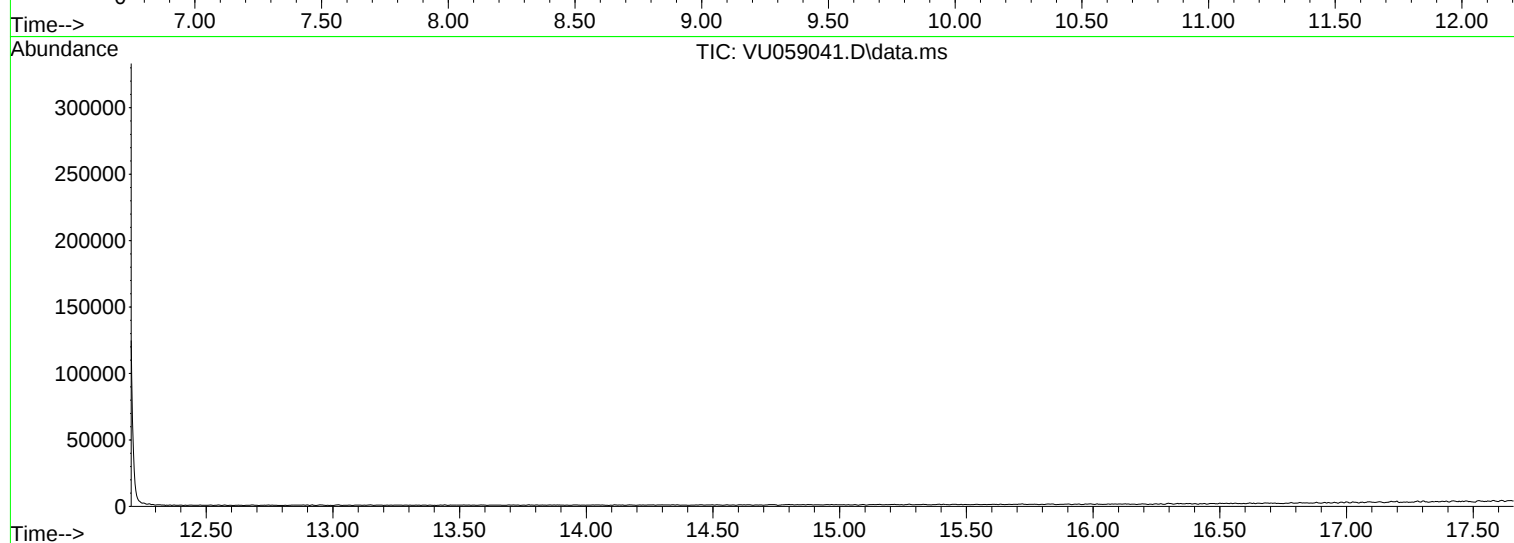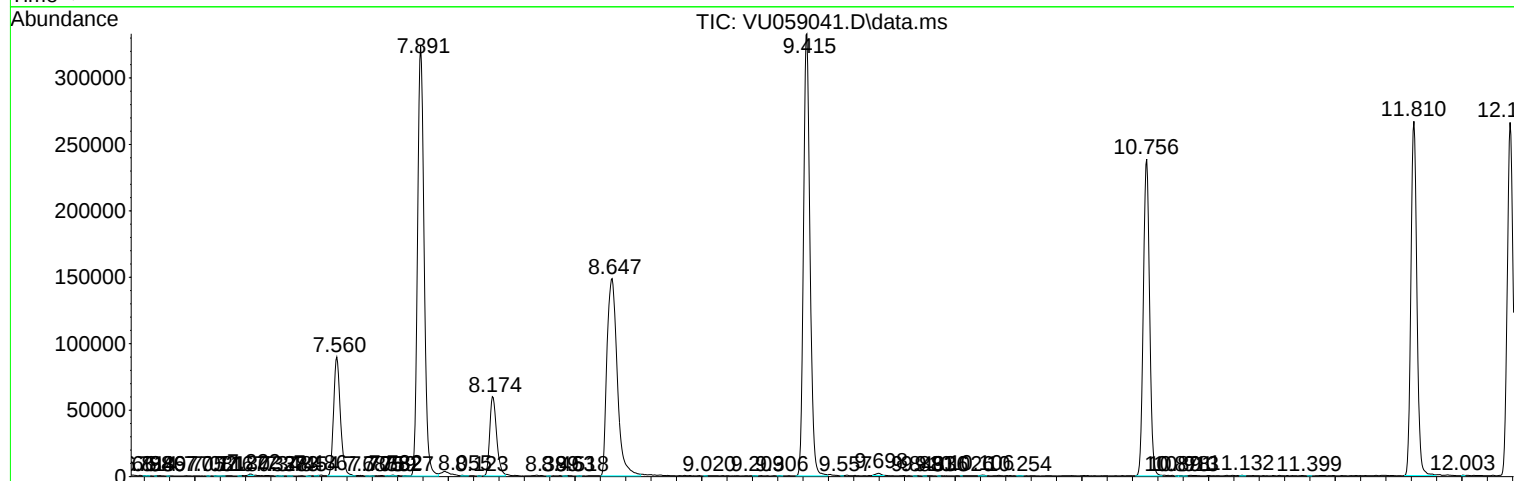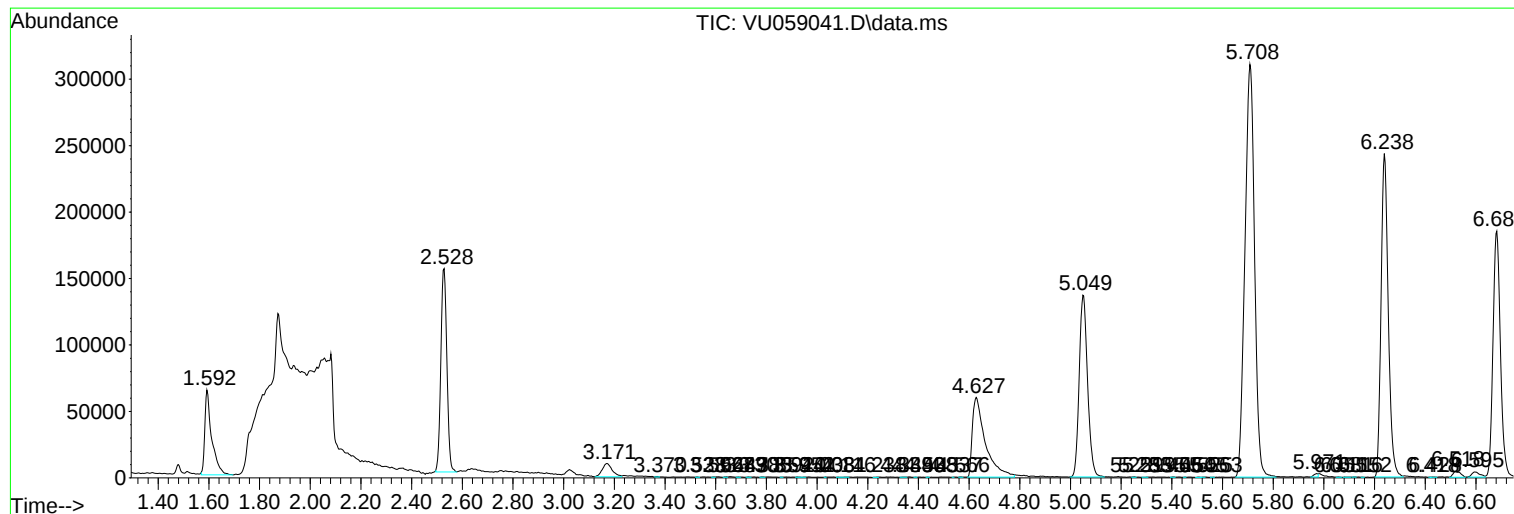

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059041.D
Acq On : 28 May 2024 19:46
Operator : MD/SY
Sample : P2570-13ME
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5Q9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059041.D
Acq On : 28 May 2024 19:46
Operator : MD/SY
Sample : P2570-13ME
Misc : 5.58g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5Q9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc