
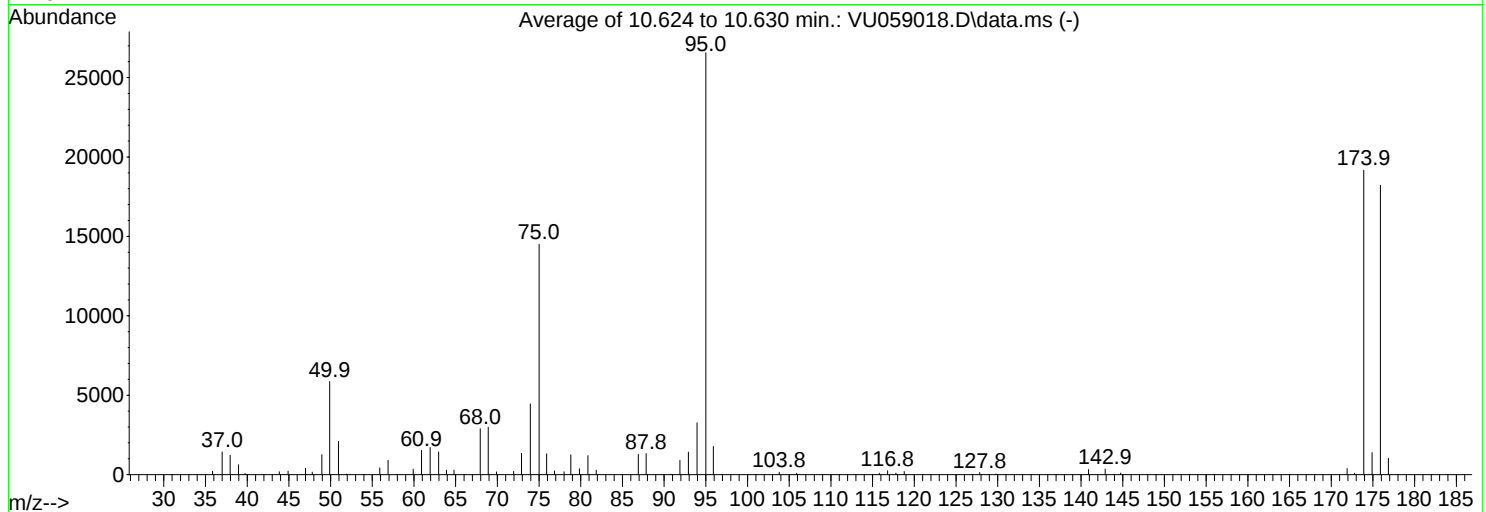


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052824\
Data File : VU059018.D
Acq On : 28 May 2024 08:52
Operator : MD/SY
Sample : BFB054
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB054

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis
Last Update : Wed May 29 02:38:59 2024

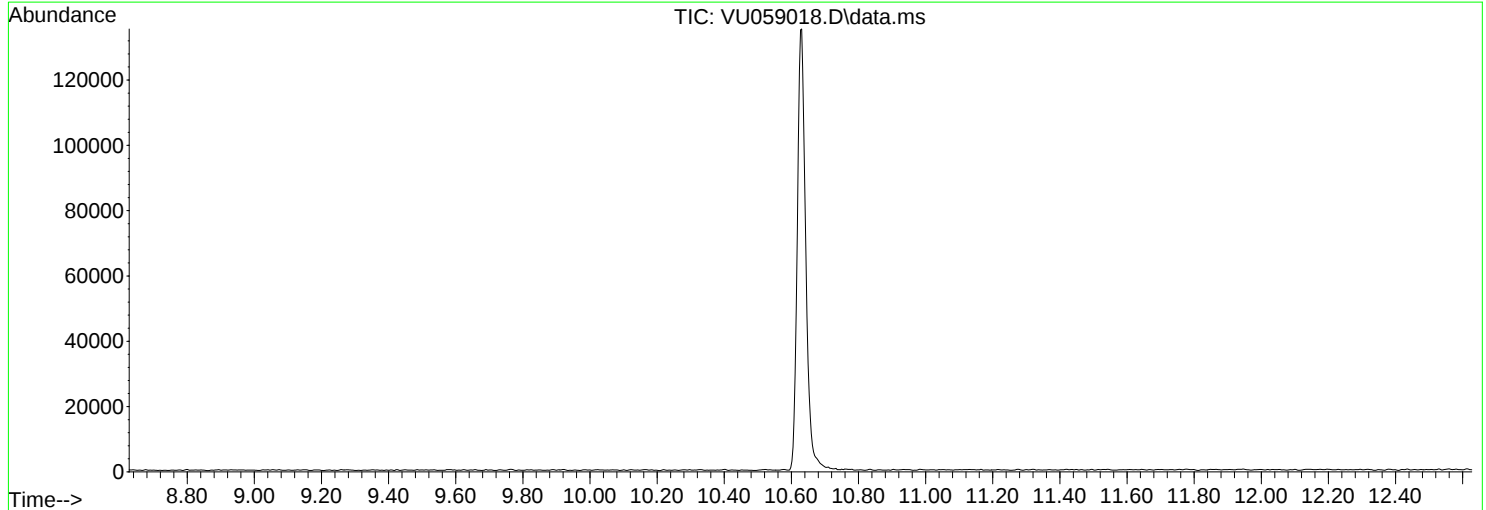

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	5858	PASS
75	95	30	80	54.6	14501	PASS
95	95	100	100	100.0	26555	PASS
96	95	5	9	6.7	1778	PASS
173	174	0.00	2	0.5	88	PASS
174	95	50	120	72.2	19173	PASS
175	174	5	9	7.3	1394	PASS
176	174	95	101	95.0	18219	PASS
177	176	5	9	5.6	1024	PASS

m/z	Abundance
39.80	216.0
43.80	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.80	204.0
37.00	1353.0
37.90	1153.0
39.00	620.0
39.80	368.0
43.90	600.0
44.90	227.0
47.00	378.0
47.80	130.0
48.90	1140.0
49.90	5362.0
50.90	2075.0
51.90	113.0
55.90	451.0
56.90	908.0
59.90	314.0
60.90	1544.0
61.90	1552.0
62.90	1244.0
63.90	251.0
64.80	276.0
68.00	2878.0
68.90	2843.0
69.90	182.0
72.10	208.0
72.90	1189.0
74.00	4365.0
75.00	13781.0
75.90	1246.0
76.80	211.0
78.00	195.0
78.80	1262.0
79.80	311.0
80.90	1125.0
81.80	263.0
86.90	1209.0
87.80	1189.0
91.90	908.0
92.90	1328.0
93.90	2974.0
95.00	25048.0
95.90	1720.0
103.80	137.0
115.80	137.0
116.80	216.0
118.80	126.0
127.90	141.0
140.90	268.0
142.90	327.0
144.70	105.0
171.90	332.0
173.90	17624.0
174.90	1261.0
175.90	16624.0
176.80	885.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	218.0
37.00	1505.0
38.00	1230.0
38.90	650.0
39.70	305.0
43.90	497.0
44.90	239.0
47.00	422.0
47.80	168.0
48.90	1277.0
49.90	6049.0
50.90	2173.0
55.90	441.0
56.90	934.0
59.90	356.0
60.90	1589.0
61.90	1804.0
63.00	1488.0
63.90	306.0
64.80	295.0
67.90	2964.0
68.90	3038.0
69.90	163.0
71.90	206.0
72.90	1377.0
74.00	4519.0
75.00	14968.0
75.90	1332.0
76.90	210.0
78.00	194.0
78.80	1291.0
79.90	367.0
80.80	1247.0
81.80	281.0
86.90	1346.0
87.90	1374.0
91.90	913.0
92.90	1483.0
93.90	3412.0
95.00	27384.0
95.90	1813.0
103.80	171.0
105.90	124.0
115.80	122.0
116.80	268.0
117.80	151.0
118.80	210.0
127.90	149.0
140.90	324.0
142.90	352.0
144.80	100.0
171.90	404.0
173.90	19872.0
174.90	1455.0
175.90	18784.0
176.80	1037.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	206.0
37.00	1448.0
38.00	1273.0
38.90	611.0
39.80	217.0
43.90	459.0
44.90	211.0
47.00	413.0
47.80	179.0
49.00	1368.0
49.90	6163.0
51.00	2024.0
55.90	384.0
56.90	839.0
59.90	349.0
60.90	1454.0
62.00	1781.0
63.00	1572.0
63.90	301.0
64.80	286.0
67.90	2844.0
68.90	3069.0
69.90	183.0
71.90	204.0
72.90	1468.0
73.90	4475.0
75.00	14753.0
75.90	1363.0
76.90	263.0
78.00	168.0
78.80	1196.0
79.90	441.0
80.80	1223.0
81.90	292.0
86.90	1281.0
87.90	1394.0
90.80	104.0
91.90	854.0
92.90	1464.0
94.00	3405.0
95.00	27232.0
95.90	1801.0
103.80	133.0
105.90	150.0
116.80	239.0
117.80	166.0
118.80	235.0
127.80	115.0
129.80	117.0
140.90	376.0
142.90	365.0
144.80	108.0
171.90	424.0
172.80	265.0
173.90	20024.0
174.90	1467.0
175.90	19248.0
176.90	1150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054