

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059054.D
 Acq On : 29 May 2024 16:26
 Operator : MD/SY
 Sample : VU0529WBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 30 02:29:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 00:34:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	196789	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	186757	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	77765	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	57366	48.687	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.380%		
7) Chloroethane-d5	1.878	69	48405	47.958	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.920%		
11) 1,1-Dichloroethene-d2	2.550	63	74858	32.187	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.380%		
21) 2-Butanone-d5	4.612	46	116969	105.322	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.320%		
24) Chloroform-d	5.052	84	112115	47.798	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.600%		
26) 1,2-Dichloroethane-d4	5.692	65	73892	51.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.800%		
32) Benzene-d6	5.718	84	215319	50.233	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.460%		
36) 1,2-Dichloropropane-d6	6.682	67	76761	51.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	103.880%		
41) Toluene-d8	7.891	98	177647	48.821	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.640%		
43) trans-1,3-Dichloroprop...	8.174	79	30026	50.261	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	100.520%		
47) 2-Hexanone-d5	8.627	63	69457	101.629	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.630%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84	123966	49.561	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.120%		
66) 1,2-Dichlorobenzene-d4	12.190	152	60972	52.539	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.080%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	7765	4.055	ug/L	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059054.D
Acq On : 29 May 2024 16:26
Operator : MD/SY
Sample : VU0529WBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 30 02:29:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 00:34:31 2024
Response via : Initial Calibration

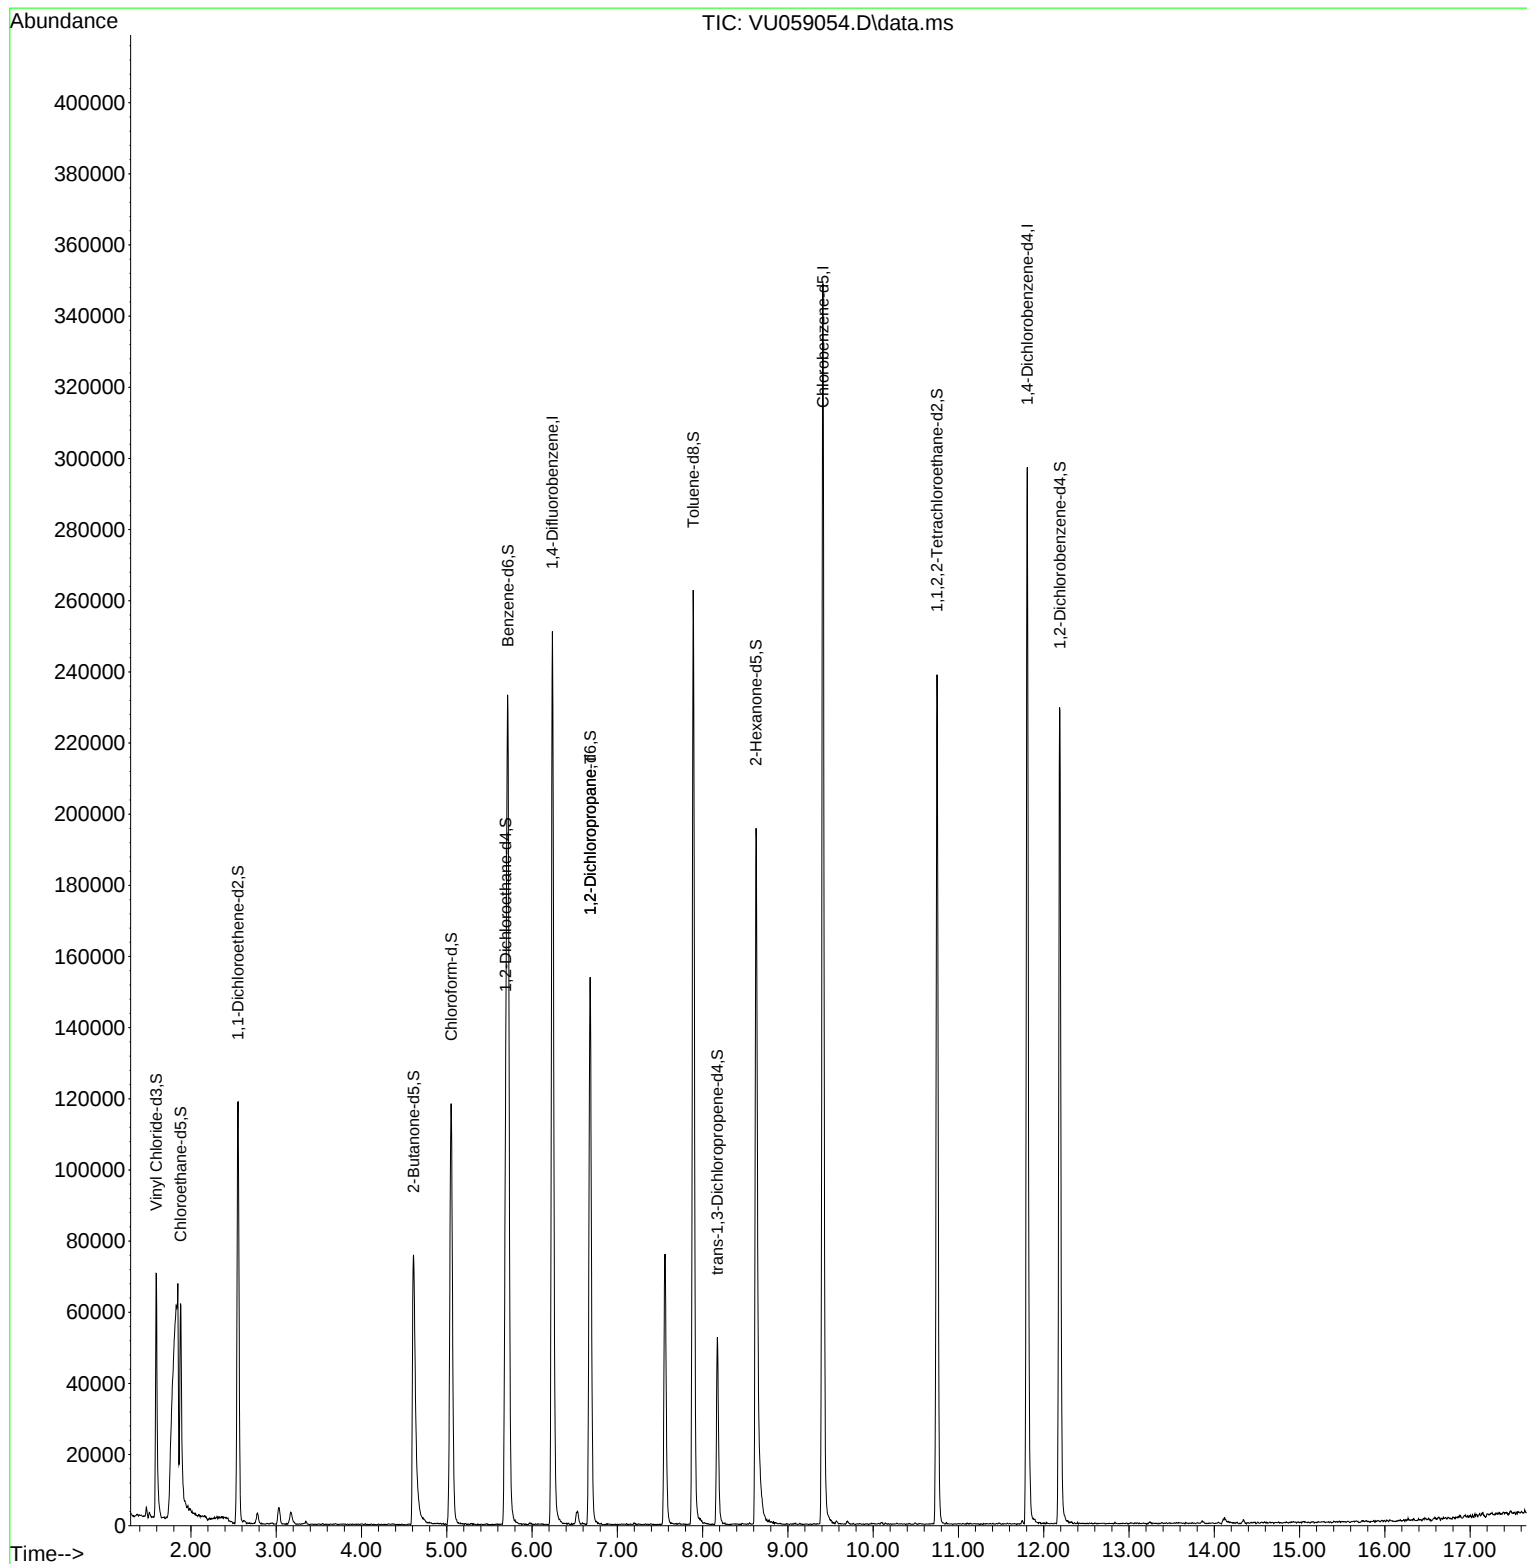

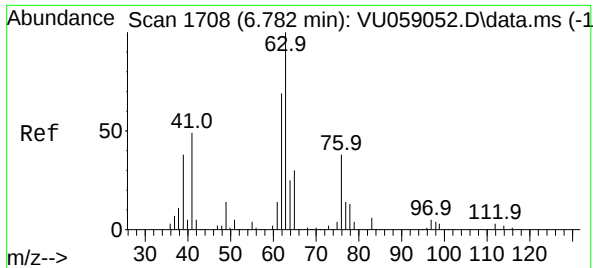

#37
 1,2-Dichloropropane
 Concen: 4.055 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.099 min
 Lab File: VU059054.D
 Acq: 29 May 2024 16:26

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 7765
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 4.0#

