

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059055.D
 Acq On : 29 May 2024 16:50
 Operator : MD/SY
 Sample : P2588-07ME
 Misc : 5.87g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 30 02:29:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 00:34:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	223506	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	216198	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	89431	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	46858	35.015	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.020%		
7) Chloroethane-d5	1.875	69	37158	32.414	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	64.820%#		
11) 1,1-Dichloroethene-d2	2.534	63	63902	24.192	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	48.380%#		
21) 2-Butanone-d5	4.621	46	95056	75.360	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	75.360%		
24) Chloroform-d	5.052	84	92533	34.734	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	69.460%#		
26) 1,2-Dichloroethane-d4	5.692	65	62781	38.449	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.900%		
32) Benzene-d6	5.714	84	186211	37.527	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.060%		
36) 1,2-Dichloropropane-d6	6.682	67	64086	37.457	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	74.920%		
41) Toluene-d8	7.891	98	154697	36.725	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.440%#		
43) trans-1,3-Dichloroprop...	8.177	79	26135	37.790	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.580%		
47) 2-Hexanone-d5	8.643	63	59065	74.655	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	74.650%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	103655	35.798	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	71.600%		
66) 1,2-Dichlorobenzene-d4	12.193	152	52384	39.250	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.500%#		
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.811	75	12504	5.028	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059055.D
Acq On : 29 May 2024 16:50
Operator : MD/SY
Sample : P2588-07ME
Misc : 5.87g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 30 02:29:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 00:34:31 2024
Response via : Initial Calibration

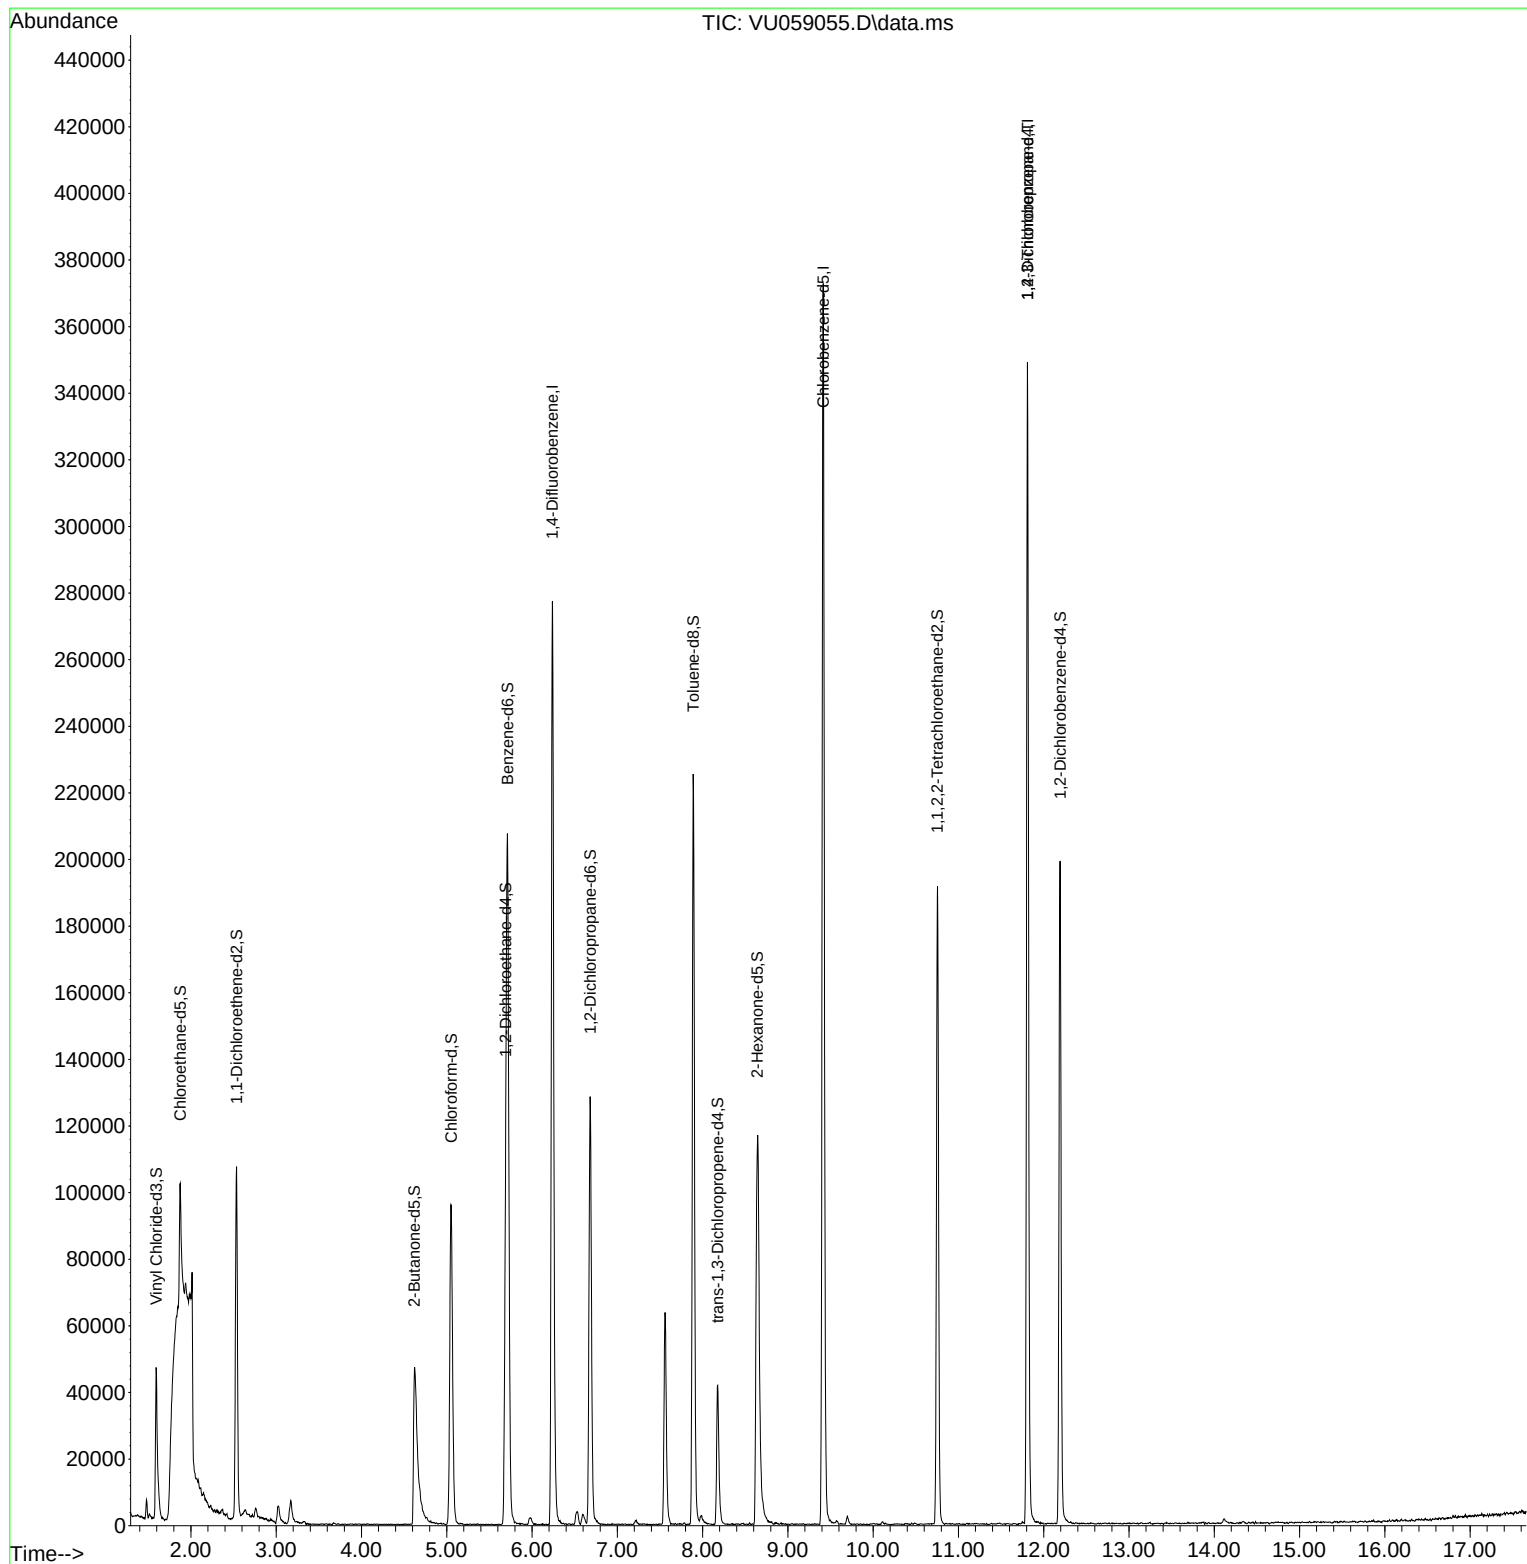

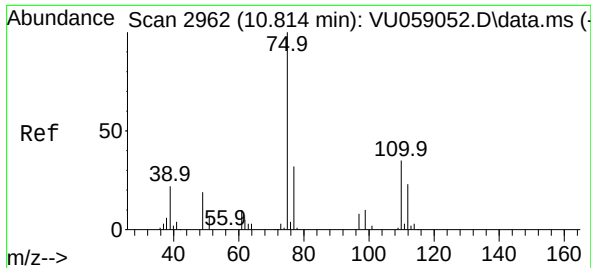

#60

1,2,3-Trichloropropane

Concen: 5.028 ug/L

RT: 11.811 min Scan# 31

Delta R.T. 0.997 min


Lab File: VU059055.D

Acq: 29 May 2024 16:50

Instrument :

MSVOA_U

ClientSampleId :

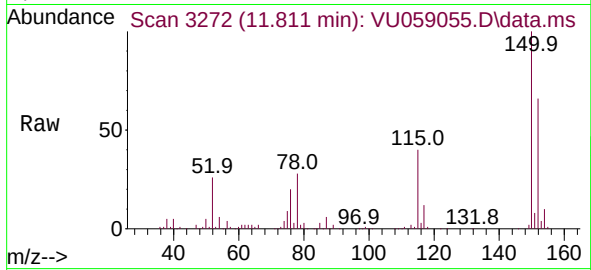

Tgt Ion: 75 Resp: 12504

Ion Ratio Lower Upper

75 100

77 32.3 26.2 39.2

110 1.7 28.4 42.6#

