

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059069.D
 Acq On : 29 May 2024 22:14
 Operator : MD/SY
 Sample : P2590-17ME
 Misc : 6.29g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 30 02:32:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 00:34:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	196633	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	197006	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	87225	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	47932	40.713	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.420%		
7) Chloroethane-d5	1.872	69	39179	38.848	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.700%		
11) 1,1-Dichloroethene-d2	2.541	63	65711	28.276	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.560%#		
21) 2-Butanone-d5	4.618	46	98015	88.325	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.330%		
24) Chloroform-d	5.052	84	96714	41.265	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.520%		
26) 1,2-Dichloroethane-d4	5.692	65	64946	45.211	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.420%		
32) Benzene-d6	5.714	84	191477	42.347	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.700%		
36) 1,2-Dichloropropane-d6	6.679	67	66318	42.538	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.080%		
41) Toluene-d8	7.891	98	154208	40.175	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.340%		
43) trans-1,3-Dichloroprop...	8.174	79	27471	43.592	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.180%		
47) 2-Hexanone-d5	8.640	63	60661	84.141	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	84.140%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	112785	42.745	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.500%		
66) 1,2-Dichlorobenzene-d4	12.190	152	57231	43.967	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.940%		
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	6.682	63	7128	3.529	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059069.D
Acq On : 29 May 2024 22:14
Operator : MD/SY
Sample : P2590-17ME
Misc : 6.29g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 30 02:32:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 00:34:31 2024
Response via : Initial Calibration

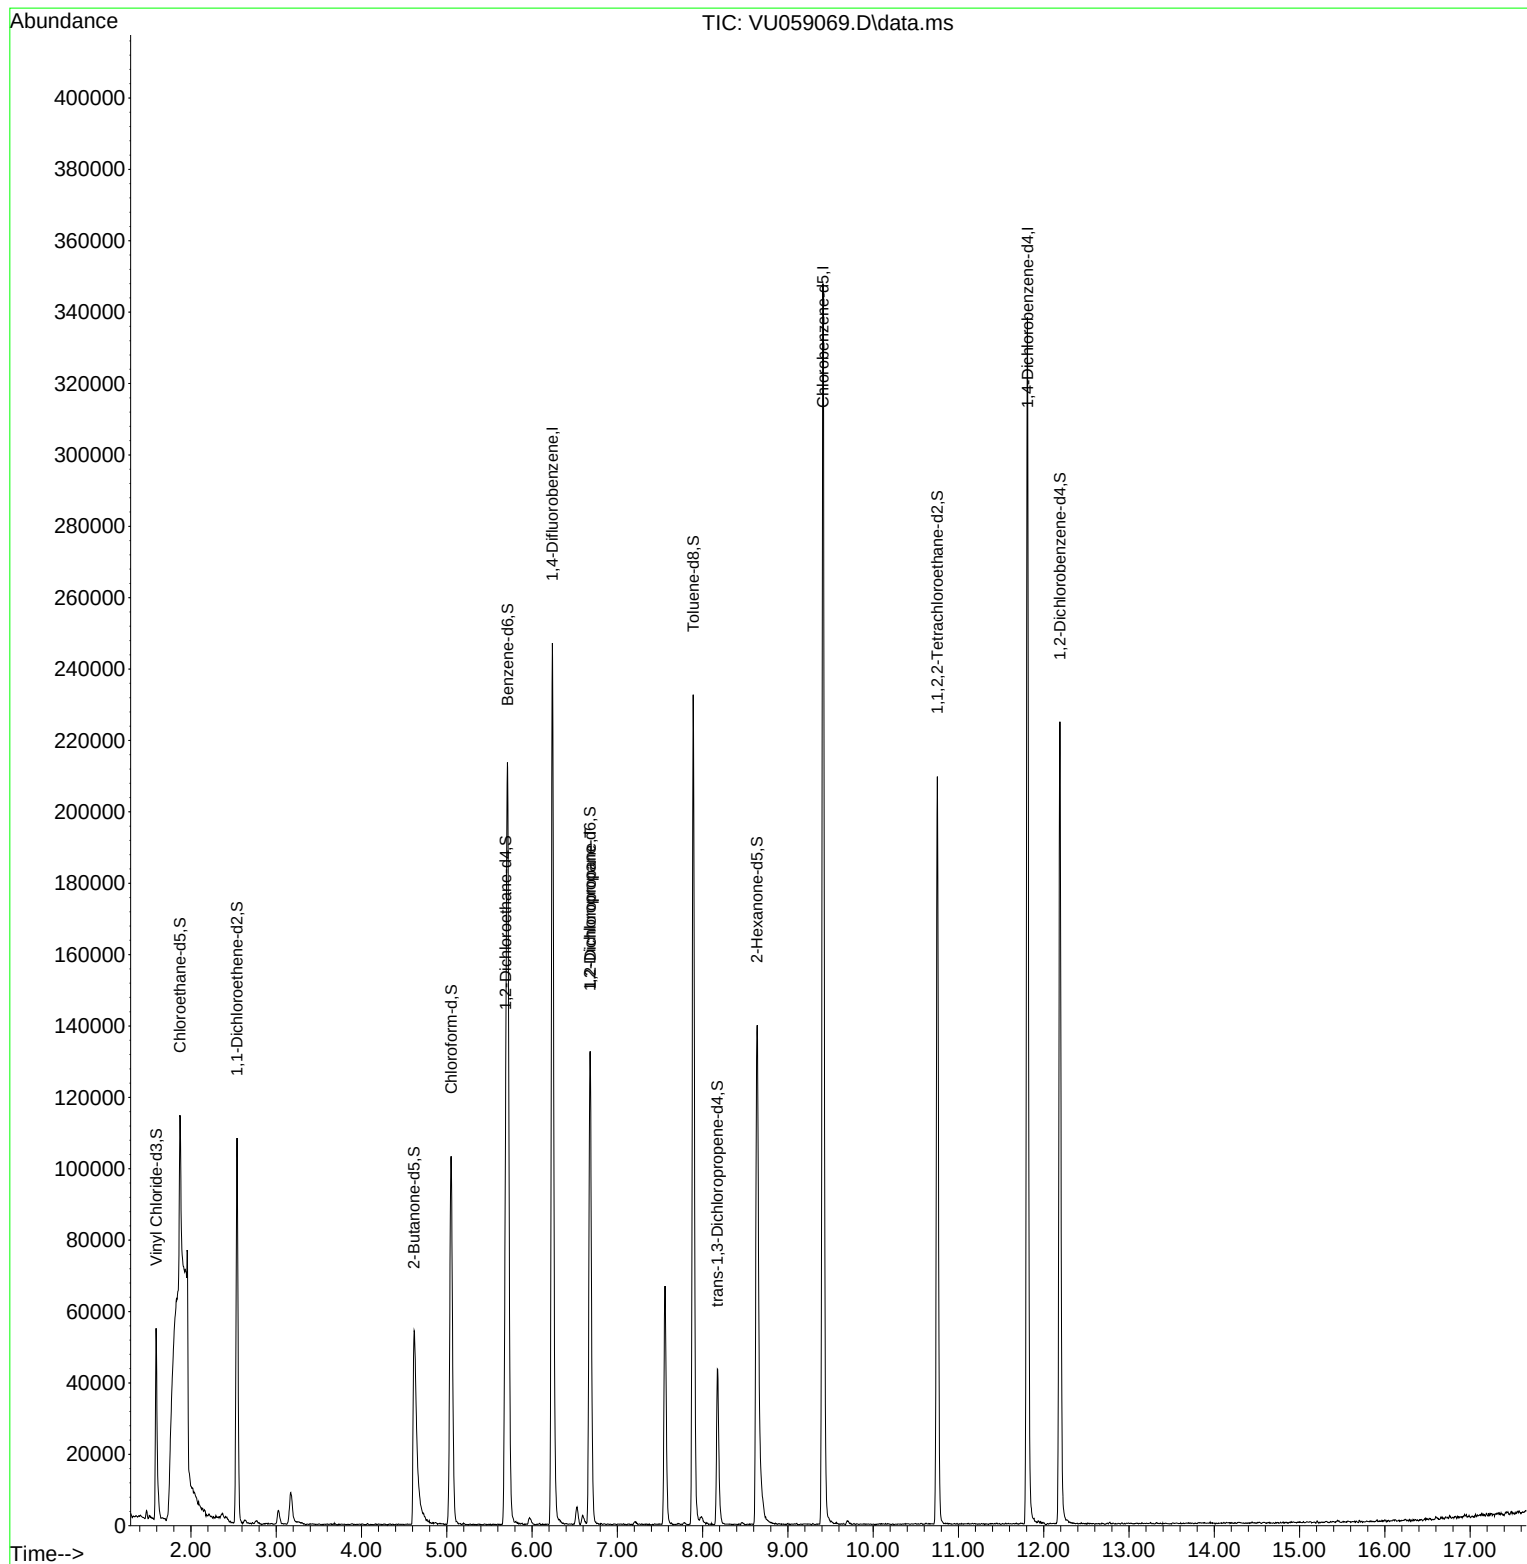

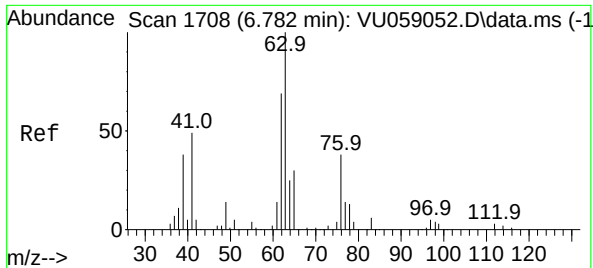

#37
 1,2-Dichloropropane
 Concen: 3.529 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.099 min
 Lab File: VU059069.D
 Acq: 29 May 2024 22:14

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 7128
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 4.0#

