

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059075.D
 Acq On : 30 May 2024 00:32
 Operator : MD/SY
 Sample : P2570-09ME
 Misc : 5.32g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 30 02:34:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 00:34:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	176787	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	179347	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	76798	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	63780	60.255	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 120.520%			
7) Chloroethane-d5	1.875	69	55940	61.694	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 123.380%			
11) 1,1-Dichloroethene-d2	2.541	63	78738	37.686	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery = 75.380%			
21) 2-Butanone-d5	4.618	46	121712	121.992	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 121.990%			
24) Chloroform-d	5.052	84	125927	59.761	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 119.520%			
26) 1,2-Dichloroethane-d4	5.689	65	87848	68.019	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 136.040%#			
32) Benzene-d6	5.714	84	247859	60.214	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 120.420%			
36) 1,2-Dichloropropane-d6	6.682	67	87205	61.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 122.880%#			
41) Toluene-d8	7.891	98	195725	56.012	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 112.020%			
43) trans-1,3-Dichloroprop...	8.174	79	32715	57.025	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 114.040%			
47) 2-Hexanone-d5	8.640	63	71245	108.552	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery = 108.550%			
56) 1,1,2,2-Tetrachloroeth...	10.753	84	134321	55.920	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 111.840%			
66) 1,2-Dichlorobenzene-d4	12.190	152	70873	61.839	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 123.680%#			
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.807	75	10295	4.821	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059075.D
Acq On : 30 May 2024 00:32
Operator : MD/SY
Sample : P2570-09ME
Misc : 5.32g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 30 02:34:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 00:34:31 2024
Response via : Initial Calibration

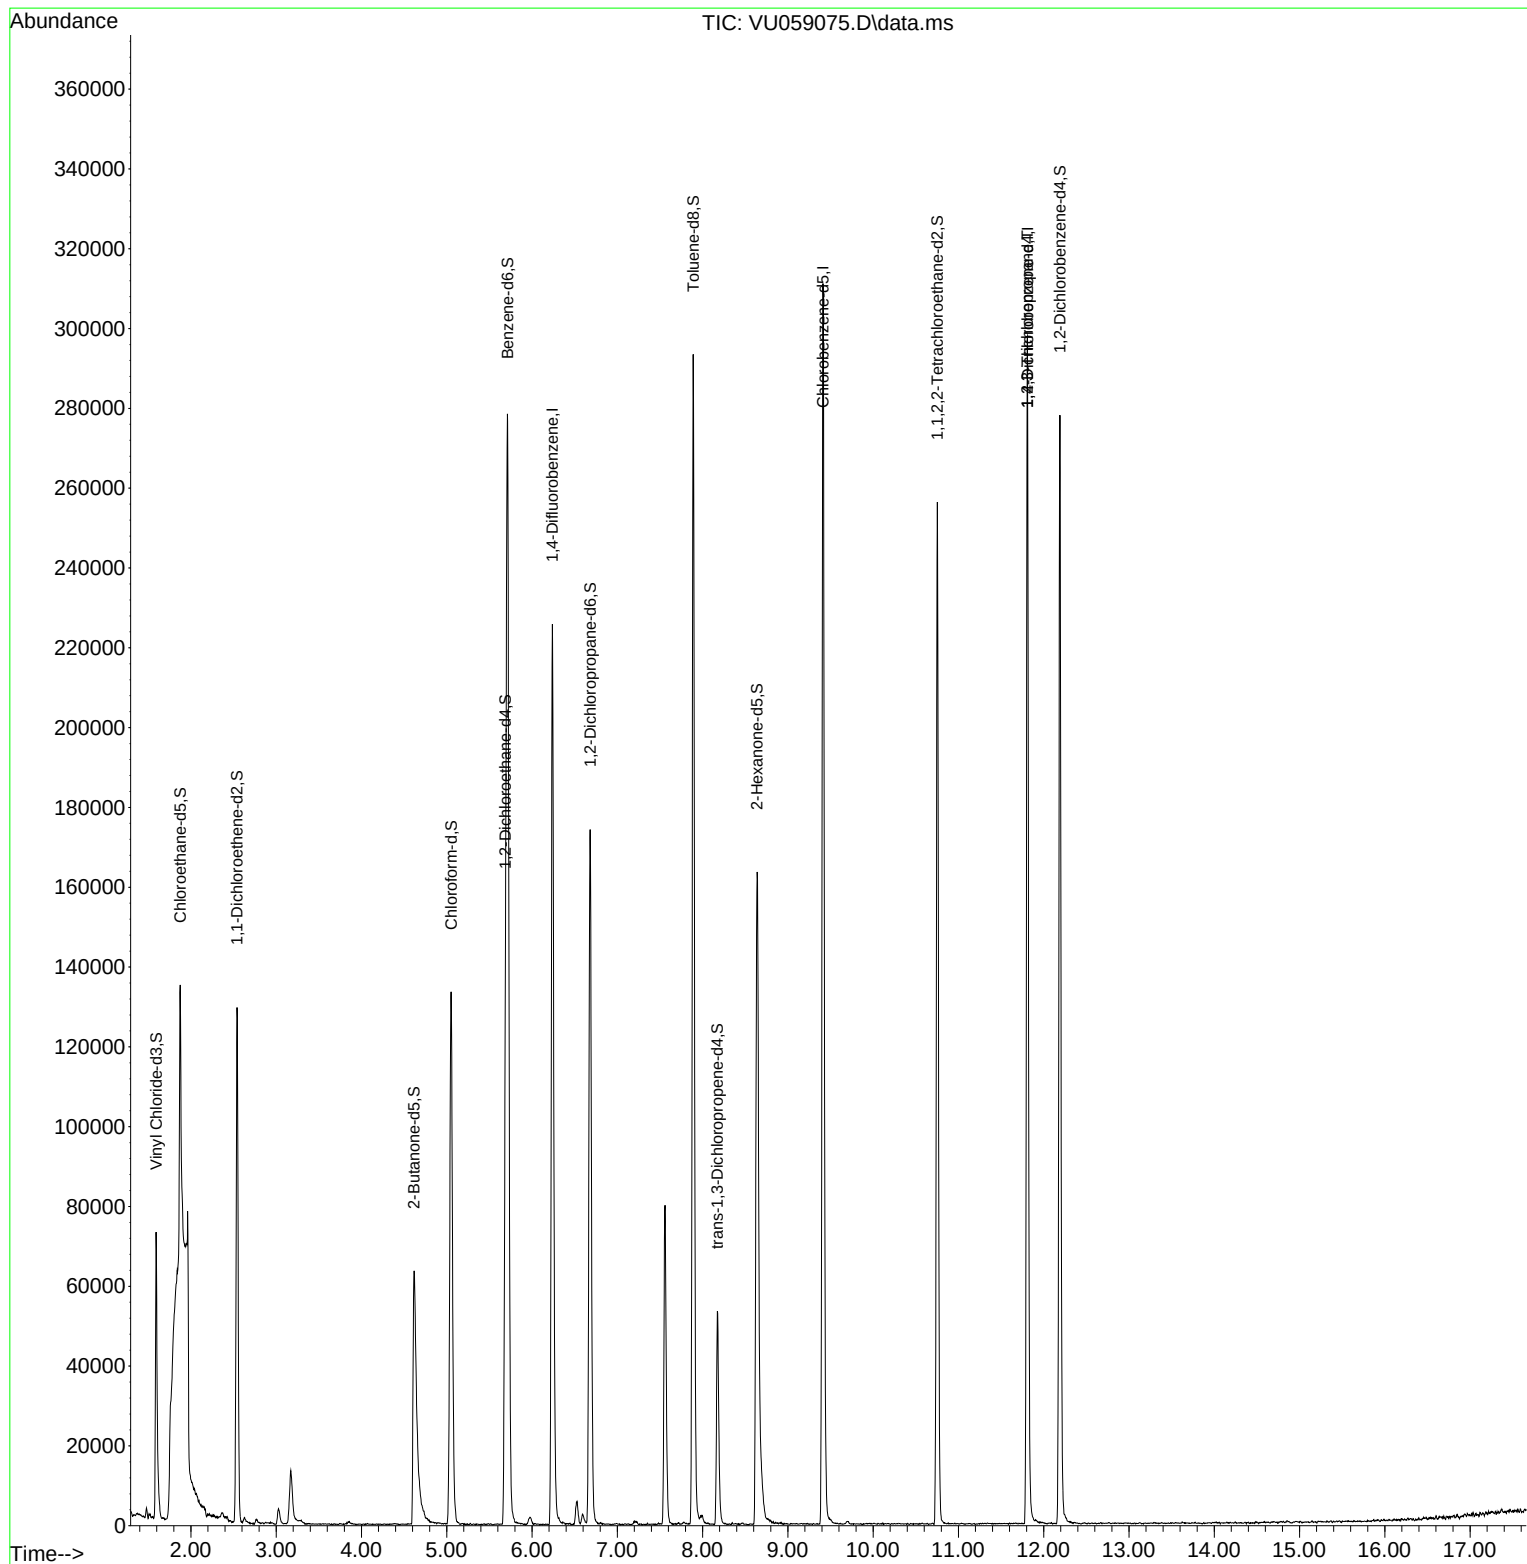

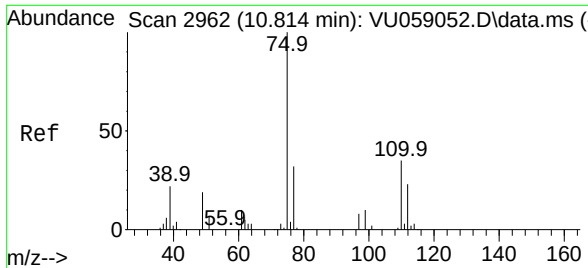

#60
 1,2,3-Trichloropropane
 Concen: 4.821 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.994 min
 Lab File: VU059075.D
 Acq: 30 May 2024 00:32

Instrument :
 MSVOA_U
 ClientSampleId :

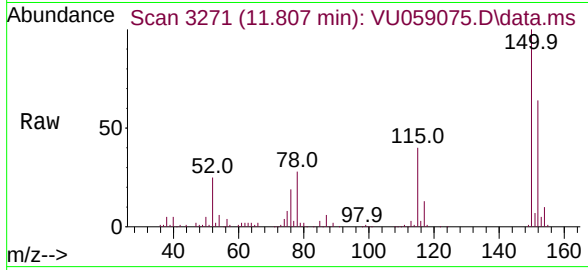

Tgt Ion: 75	Resp:	10295
Ion	Ratio	Lower Upper
75	100	
77	37.8	26.2 39.2
110	1.3	28.4 42.6#

