

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059057.D
 Acq On : 29 May 2024 17:37
 Operator : MD/SY
 Sample : P2591-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.486	57	61	66	rVB3	2327	2027	0.30%	0.037%
2	1.595	86	95	111	rBV	81111	100337	15.00%	1.816%
3	1.766	141	148	154	rBV3	9524	11327	1.69%	0.205%
4	1.907	184	192	210	rVB	68448	90705	13.56%	1.642%
5	2.560	383	395	409	rBV	125620	205906	30.78%	3.728%
6	2.621	410	414	426	rVB5	3151	4797	0.72%	0.087%
7	2.750	443	454	458	rVV2	1527	2395	0.36%	0.043%
8	2.788	461	466	479	rVB	2200	3606	0.54%	0.065%
9	2.865	484	490	493	rBV2	222	224	0.03%	0.004%
10	2.946	511	515	520	rVB2	381	382	0.06%	0.007%
11	3.039	535	544	554	rVV2	3552	6105	0.91%	0.111%
12	3.174	577	586	595	rBV2	953	2121	0.32%	0.038%
13	3.245	604	608	611	rBV2	280	321	0.05%	0.006%
14	3.351	635	641	649	rBV4	936	1462	0.22%	0.026%
15	3.615	720	723	730	rVB2	425	552	0.08%	0.010%
16	3.676	736	742	745	rVV2	244	248	0.04%	0.004%
17	4.255	917	922	925	rBV2	252	205	0.03%	0.004%
18	4.341	945	949	952	rBV2	301	273	0.04%	0.005%
19	4.451	980	983	986	rVB	306	240	0.04%	0.004%
20	4.611	1022	1033	1059	rBV	81617	202715	30.30%	3.670%
21	4.910	1123	1126	1129	rBV2	372	348	0.05%	0.006%
22	4.984	1146	1149	1155	rVB3	267	257	0.04%	0.005%
23	5.055	1155	1171	1199	rBV	127044	303536	45.37%	5.495%
24	5.203	1213	1217	1222	rVB4	522	574	0.09%	0.010%
25	5.354	1257	1264	1269	rBV2	273	467	0.07%	0.008%
26	5.393	1273	1276	1284	rVB2	336	416	0.06%	0.008%
27	5.563	1326	1329	1332	rBV2	228	211	0.03%	0.004%
28	5.717	1357	1377	1402	rBV2	245390	669018	100.00%	12.112%
29	5.962	1450	1453	1455	rBV	402	292	0.04%	0.005%
30	5.997	1459	1464	1467	rBV2	225	262	0.04%	0.005%
31	6.139	1505	1508	1511	rVB	450	318	0.05%	0.006%
32	6.161	1511	1515	1518	rBV2	418	362	0.05%	0.007%
33	6.242	1527	1540	1572	rBV	262228	510268	76.27%	9.238%
34	6.431	1595	1599	1603	rBV2	382	351	0.05%	0.006%
35	6.531	1620	1630	1640	rBV6	4865	9432	1.41%	0.171%
36	6.570	1640	1642	1646	rVB3	359	228	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059057.D
 Acq On : 29 May 2024 17:37
 Operator : MD/SY
 Sample : P2591-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.592	1646	1649	1652	rBV2	240	229	0.03%	0.004%
38	6.631	1658	1661	1665	rVB2	311	253	0.04%	0.005%
39	6.682	1665	1677	1698	rBV	159273	313972	46.93%	5.684%
40	7.200	1830	1838	1845	rBV3	640	977	0.15%	0.018%
41	7.296	1865	1868	1872	rVB2	369	290	0.04%	0.005%
42	7.364	1885	1889	1890	rBV	454	219	0.03%	0.004%
43	7.425	1901	1908	1910	rBV2	241	273	0.04%	0.005%
44	7.560	1938	1950	1967	rBV	77301	138264	20.67%	2.503%
45	7.666	1981	1983	1987	rVB2	539	294	0.04%	0.005%
46	7.721	1996	2000	2003	rBV2	231	218	0.03%	0.004%
47	7.891	2040	2053	2072	rBV	267555	476936	71.29%	8.634%
48	8.174	2131	2141	2160	rBV	53554	93930	14.04%	1.700%
49	8.283	2172	2175	2184	rBV3	292	389	0.06%	0.007%
50	8.473	2232	2234	2241	rVB3	284	241	0.04%	0.004%
51	8.627	2271	2282	2328	rBV	190555	389216	58.18%	7.046%
52	8.930	2373	2376	2378	rBV2	392	290	0.04%	0.005%
53	8.975	2387	2390	2392	rVB2	345	227	0.03%	0.004%
54	9.049	2410	2413	2418	rVB3	275	213	0.03%	0.004%
55	9.283	2483	2486	2491	rVB2	227	211	0.03%	0.004%
56	9.412	2512	2526	2550	rBV	371904	638144	95.39%	11.553%
57	9.569	2571	2575	2578	rBV	544	460	0.07%	0.008%
58	9.621	2590	2591	2597	rBV2	304	200	0.03%	0.004%
59	9.653	2598	2601	2603	rBV	344	204	0.03%	0.004%
60	9.782	2639	2641	2647	rVV2	267	201	0.03%	0.004%
61	9.862	2663	2666	2672	rBV2	182	226	0.03%	0.004%
62	10.116	2741	2745	2746	rBV2	266	234	0.03%	0.004%
63	10.232	2777	2781	2788	rVB2	351	460	0.07%	0.008%
64	10.274	2788	2794	2796	rBV	286	312	0.05%	0.006%
65	10.360	2817	2821	2825	rBV	255	219	0.03%	0.004%
66	10.476	2854	2857	2863	rVB2	253	287	0.04%	0.005%
67	10.666	2912	2916	2919	rBV	269	220	0.03%	0.004%
68	10.749	2930	2942	2964	rVV	234075	383048	57.26%	6.935%
69	10.846	2970	2972	2978	rVB2	392	258	0.04%	0.005%
70	10.872	2978	2980	2985	rVB2	268	218	0.03%	0.004%
71	10.897	2985	2988	2989	rBV2	346	192	0.03%	0.003%
72	10.981	3011	3014	3019	rVB2	279	230	0.03%	0.004%
73	11.045	3032	3034	3038	rVB2	357	204	0.03%	0.004%
74	11.074	3038	3043	3045	rBV2	291	288	0.04%	0.005%
75	11.749	3248	3253	3257	rVB3	549	592	0.09%	0.011%
76	11.807	3259	3271	3290	rBV	322073	530452	79.29%	9.603%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059057.D
 Acq On : 29 May 2024 17:37
 Operator : MD/SY
 Sample : P2591-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH5S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.132	3369	3372	3376	rBV	323	305	0.05%	0.006%
78	12.187	3377	3389	3414	rVV	239088	410346	61.34%	7.429%
79	12.560	3501	3505	3508	rBV	310	279	0.04%	0.005%
80	12.598	3513	3517	3522	rBV2	293	303	0.05%	0.005%
81	12.679	3538	3542	3544	rBV2	234	220	0.03%	0.004%
82	12.827	3583	3588	3590	rBV2	271	210	0.03%	0.004%
83	13.299	3733	3735	3739	rBV	252	207	0.03%	0.004%
84	13.862	3907	3910	3913	rBV2	296	218	0.03%	0.004%
85	13.894	3915	3920	3924	rBV2	572	578	0.09%	0.010%
86	14.026	3959	3961	3966	rVB	335	206	0.03%	0.004%
87	14.126	3989	3992	3995	rBV2	452	343	0.05%	0.006%
88	14.248	4026	4030	4032	rBV2	459	342	0.05%	0.006%
89	14.306	4039	4048	4050	rBV2	413	572	0.09%	0.010%
90	14.569	4124	4130	4133	rBV2	385	419	0.06%	0.008%
91	14.900	4228	4233	4235	rBV3	452	405	0.06%	0.007%
92	14.987	4255	4260	4262	rBV2	496	469	0.07%	0.008%
93	15.074	4281	4287	4288	rBV3	363	357	0.05%	0.006%
94	15.505	4418	4421	4423	rBV	443	284	0.04%	0.005%
95	15.576	4441	4443	4446	rBV2	350	195	0.03%	0.004%
96	15.666	4468	4471	4476	rVB2	437	341	0.05%	0.006%
97	16.125	4612	4614	4616	rBV	438	231	0.03%	0.004%
98	16.498	4728	4730	4732	rBV3	485	304	0.05%	0.006%
99	16.547	4743	4745	4747	rBV	546	271	0.04%	0.005%
100	17.080	4908	4911	4913	rBV2	1146	751	0.11%	0.014%




Sum of corrected areas: 5523735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059057.D
Acq On : 29 May 2024 17:37
Operator : MD/SY
Sample : P2591-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

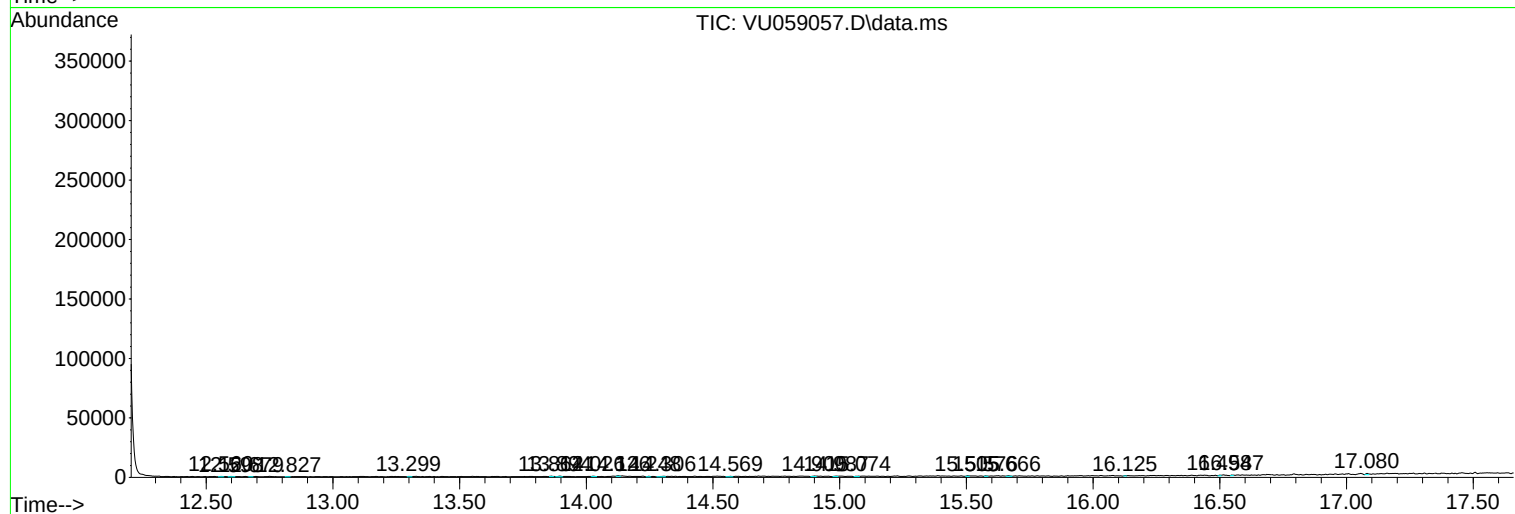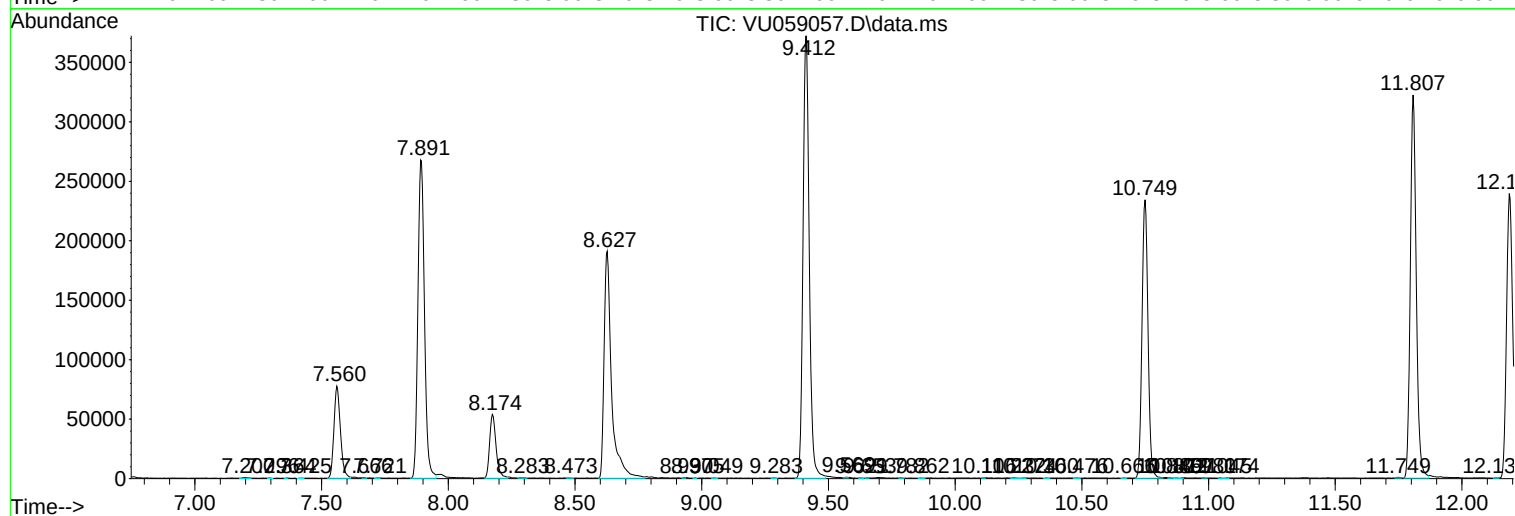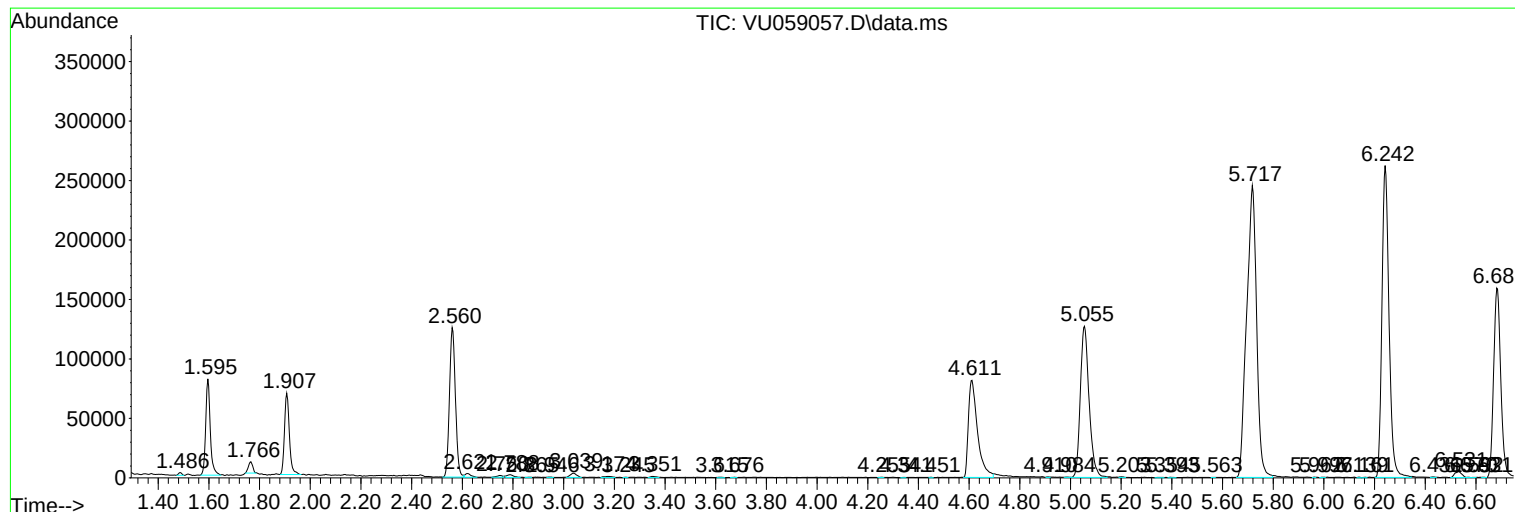

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059057.D
Acq On : 29 May 2024 17:37
Operator : MD/SY
Sample : P2591-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059057.D
Acq On : 29 May 2024 17:37
Operator : MD/SY
Sample : P2591-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH5S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------