

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059058.D
 Acq On : 29 May 2024 18:00
 Operator : MD/SY
 Sample : P2566-03 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	59	62	65	rBV	1066	646	0.02%	0.007%
2	1.596	87	95	114	rVB	77641	94121	2.38%	0.999%
3	1.763	140	147	154	rBV2	7044	9308	0.24%	0.099%
4	1.907	184	192	210	rVB	67358	89916	2.27%	0.955%
5	2.338	323	326	328	rBV2	599	368	0.01%	0.004%
6	2.454	359	362	369	rVB3	458	451	0.01%	0.005%
7	2.560	380	395	411	rBV	123993	202950	5.13%	2.155%
8	2.753	448	455	457	rVV3	644	808	0.02%	0.009%
9	2.785	459	465	476	rVB3	1843	3158	0.08%	0.034%
10	3.036	535	543	557	rVB3	3311	6137	0.16%	0.065%
11	3.100	557	563	566	rBV2	276	313	0.01%	0.003%
12	3.174	575	586	588	rBV2	3429	4742	0.12%	0.050%
13	3.412	655	660	667	rBV	248	286	0.01%	0.003%
14	3.605	717	720	725	rBV	235	257	0.01%	0.003%
15	3.946	821	826	830	rBV2	304	304	0.01%	0.003%
16	4.100	869	874	878	rBV2	367	414	0.01%	0.004%
17	4.611	1017	1033	1062	rBV	83296	210538	5.33%	2.235%
18	4.927	1128	1131	1134	rBV2	303	245	0.01%	0.003%
19	4.956	1139	1140	1144	rVB2	522	266	0.01%	0.003%
20	4.984	1144	1149	1151	rBV2	409	338	0.01%	0.004%
21	5.055	1156	1171	1190	rBV	120472	271426	6.87%	2.882%
22	5.213	1216	1220	1221	rBV2	305	214	0.01%	0.002%
23	5.290	1241	1244	1250	rVB3	374	361	0.01%	0.004%
24	5.361	1261	1266	1273	rBV	288	362	0.01%	0.004%
25	5.419	1281	1284	1287	rBV	298	241	0.01%	0.003%
26	5.457	1292	1296	1302	rVB2	214	225	0.01%	0.002%
27	5.512	1306	1313	1318	rBV2	185	269	0.01%	0.003%
28	5.718	1357	1377	1411	rBV2	237501	659388	16.68%	7.001%
29	5.959	1449	1452	1456	rVB3	307	239	0.01%	0.003%
30	6.013	1466	1469	1476	rVB3	252	256	0.01%	0.003%
31	6.046	1476	1479	1483	rBV2	261	284	0.01%	0.003%
32	6.123	1499	1503	1507	rBV2	247	307	0.01%	0.003%
33	6.158	1511	1514	1520	rBV2	273	322	0.01%	0.003%
34	6.242	1528	1540	1564	rBV	264246	504415	12.76%	5.356%
35	6.534	1616	1631	1665	rBV	2116027	3953452	100.00%	41.976%
36	6.682	1665	1677	1695	rVB	159387	311882	7.89%	3.311%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059058.D
 Acq On : 29 May 2024 18:00
 Operator : MD/SY
 Sample : P2566-03 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.849	1726	1729	1731	rBV2	413	246	0.01%	0.003%
38	6.881	1737	1739	1744	rVB3	516	404	0.01%	0.004%
39	6.968	1762	1766	1770	rBV2	308	268	0.01%	0.003%
40	7.023	1779	1783	1787	rBV2	352	296	0.01%	0.003%
41	7.084	1799	1802	1808	rVB2	307	357	0.01%	0.004%
42	7.200	1835	1838	1841	rVB2	368	258	0.01%	0.003%
43	7.216	1841	1843	1848	rBV2	312	224	0.01%	0.002%
44	7.361	1885	1888	1892	rBV	222	231	0.01%	0.002%
45	7.560	1936	1950	1970	rBV	78783	143678	3.63%	1.525%
46	7.653	1976	1979	1982	rBV3	307	223	0.01%	0.002%
47	7.891	2041	2053	2076	rBV	266442	477523	12.08%	5.070%
48	8.084	2109	2113	2116	rVB3	328	236	0.01%	0.003%
49	8.107	2116	2120	2124	rBV3	327	295	0.01%	0.003%
50	8.174	2131	2141	2163	rBV	54411	94513	2.39%	1.003%
51	8.460	2227	2230	2234	rVB2	518	429	0.01%	0.005%
52	8.550	2250	2258	2266	rVB6	3070	4747	0.12%	0.050%
53	8.624	2271	2281	2316	rBV	186124	385550	9.75%	4.094%
54	8.897	2362	2366	2373	rVB	472	554	0.01%	0.006%
55	8.939	2375	2379	2381	rBV	339	258	0.01%	0.003%
56	9.084	2421	2424	2431	rVB2	225	234	0.01%	0.002%
57	9.319	2494	2497	2502	rBV2	227	224	0.01%	0.002%
58	9.412	2514	2526	2561	rBV	372375	640092	16.19%	6.796%
59	9.566	2572	2574	2576	rBV	299	225	0.01%	0.002%
60	9.698	2609	2615	2620	rVB4	490	643	0.02%	0.007%
61	9.930	2678	2687	2690	rVB	398	563	0.01%	0.006%
62	9.962	2690	2697	2699	rBV2	412	349	0.01%	0.004%
63	10.116	2742	2745	2751	rVB3	285	270	0.01%	0.003%
64	10.235	2777	2782	2785	rBV2	241	251	0.01%	0.003%
65	10.299	2798	2802	2807	rVB2	378	433	0.01%	0.005%
66	10.328	2807	2811	2817	rBV2	326	389	0.01%	0.004%
67	10.357	2817	2820	2824	rBV2	251	216	0.01%	0.002%
68	10.405	2832	2835	2839	rVB2	307	262	0.01%	0.003%
69	10.634	2902	2906	2909	rBV	346	305	0.01%	0.003%
70	10.749	2930	2942	2962	rBV	225016	375815	9.51%	3.990%
71	10.968	3004	3010	3013	rBV2	457	468	0.01%	0.005%
72	11.225	3087	3090	3094	rBV	252	242	0.01%	0.003%
73	11.258	3094	3100	3105	rBV2	325	290	0.01%	0.003%
74	11.293	3107	3111	3114	rBV2	279	233	0.01%	0.002%
75	11.370	3129	3135	3136	rBV2	252	295	0.01%	0.003%
76	11.405	3140	3146	3148	rBV2	285	309	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059058.D
 Acq On : 29 May 2024 18:00
 Operator : MD/SY
 Sample : P2566-03 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.476	3163	3168	3171	rBV2	520	487	0.01%	0.005%
78	11.746	3242	3252	3256	rBV3	785	1130	0.03%	0.012%
79	11.807	3259	3271	3293	rBV	320525	538553	13.62%	5.718%
80	11.930	3307	3309	3317	rVB4	730	799	0.02%	0.008%
81	12.119	3366	3368	3372	rBV2	277	256	0.01%	0.003%
82	12.187	3378	3389	3413	rBV	241807	409307	10.35%	4.346%
83	12.319	3427	3430	3433	rVB3	542	353	0.01%	0.004%
84	12.418	3456	3461	3465	rBV2	463	492	0.01%	0.005%
85	12.495	3483	3485	3491	rVB2	297	235	0.01%	0.002%
86	12.878	3600	3604	3609	rBV2	331	316	0.01%	0.003%
87	13.013	3643	3646	3650	rBV2	244	225	0.01%	0.002%
88	13.081	3663	3667	3670	rBV2	275	251	0.01%	0.003%
89	13.148	3684	3688	3694	rBV2	426	425	0.01%	0.005%
90	13.515	3794	3802	3804	rBV2	328	432	0.01%	0.005%
91	13.621	3832	3835	3841	rVB2	333	293	0.01%	0.003%
92	14.097	3981	3983	3987	rBV	258	231	0.01%	0.002%
93	14.344	4057	4060	4065	rVB2	620	452	0.01%	0.005%
94	14.608	4139	4142	4144	rBV2	399	246	0.01%	0.003%
95	14.679	4159	4164	4166	rBV3	587	546	0.01%	0.006%
96	14.717	4171	4176	4177	rBV2	304	286	0.01%	0.003%
97	14.839	4210	4214	4216	rBV2	301	249	0.01%	0.003%
98	15.765	4499	4502	4505	rBV3	419	341	0.01%	0.004%
99	15.987	4569	4571	4574	rVB	483	247	0.01%	0.003%
100	16.540	4740	4743	4748	rBV4	785	690	0.02%	0.007%




Sum of corrected areas: 9418449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059058.D
Acq On : 29 May 2024 18:00
Operator : MD/SY
Sample : P2566-03 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

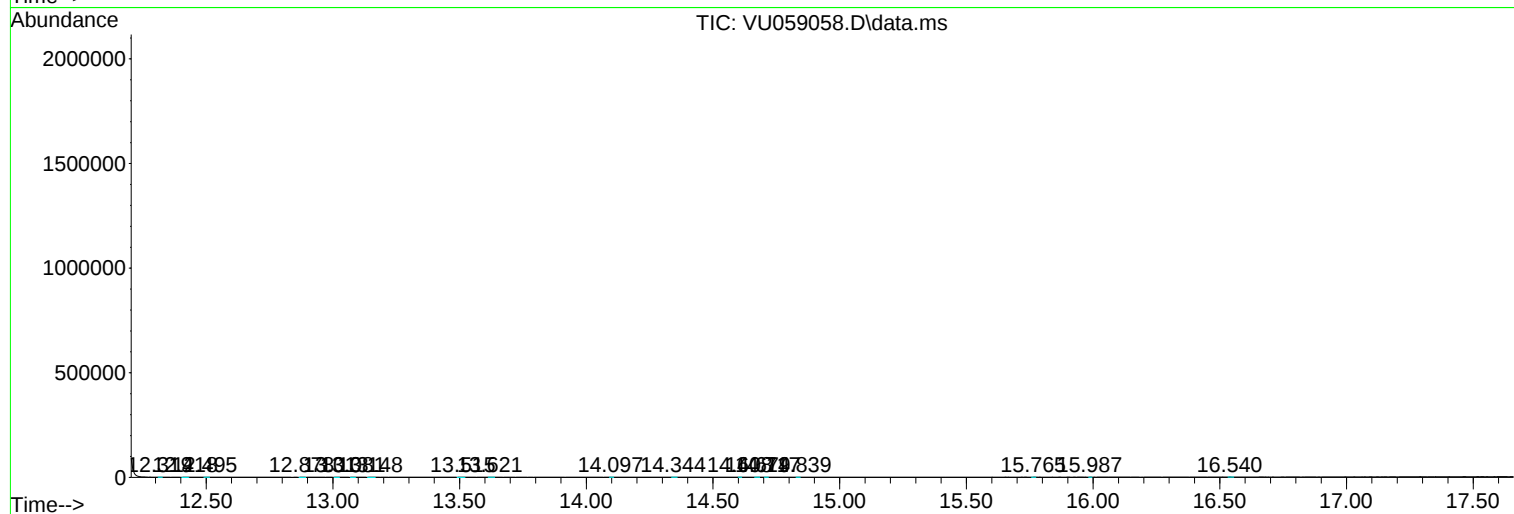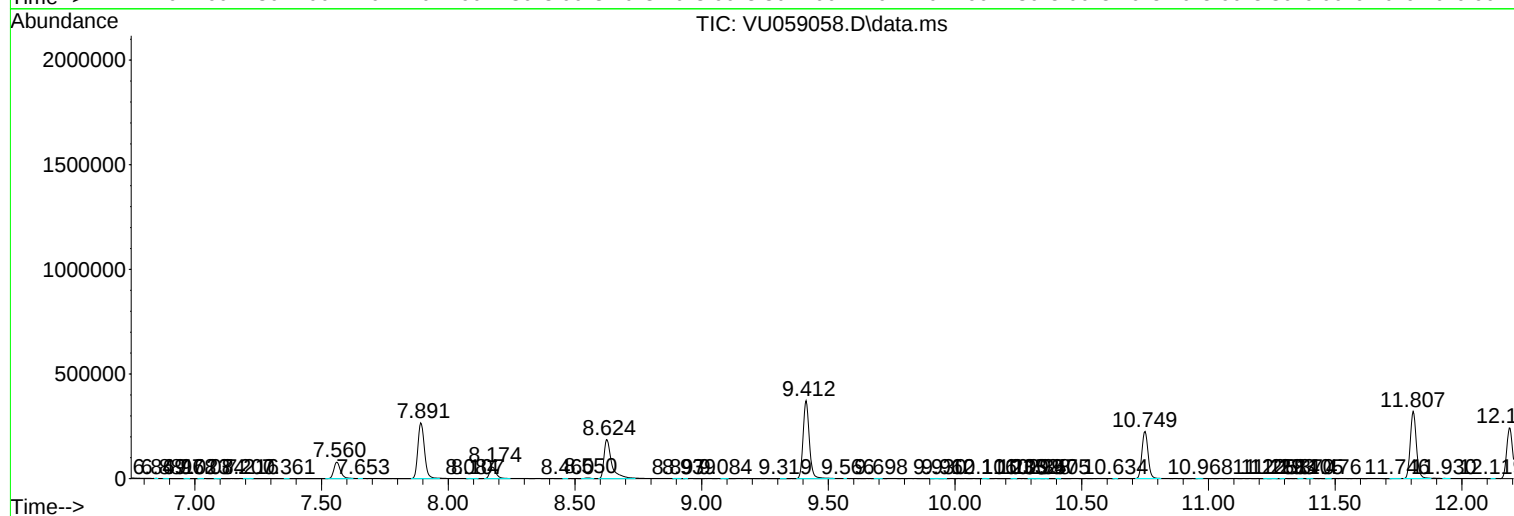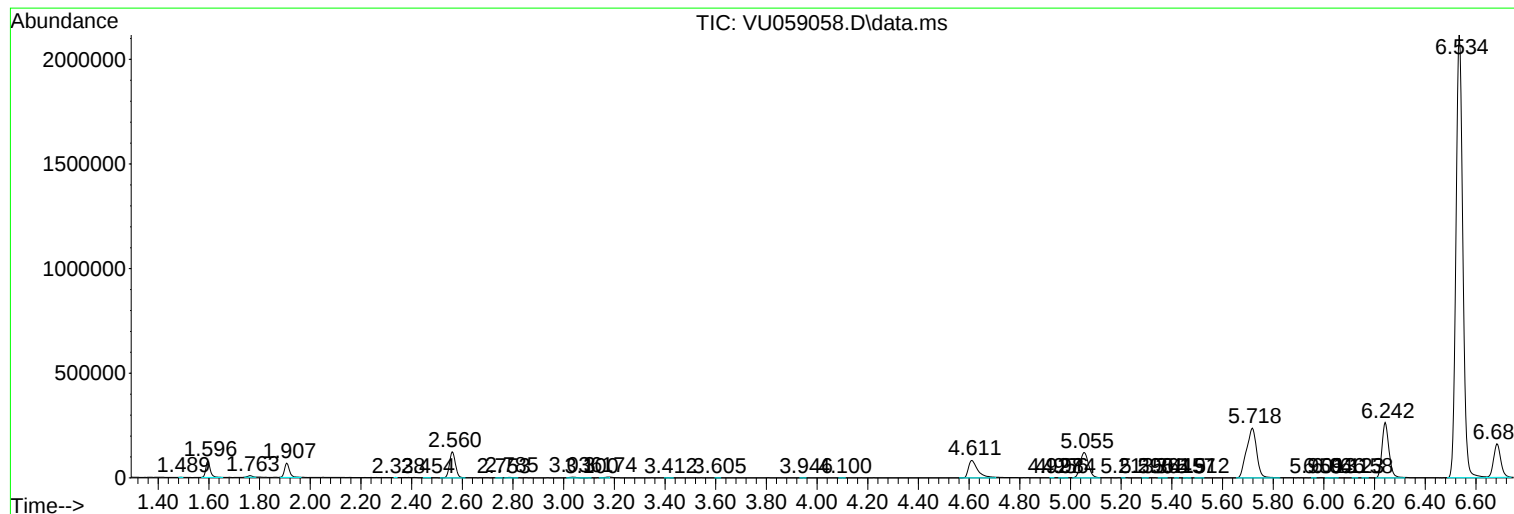

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059058.D
Acq On : 29 May 2024 18:00
Operator : MD/SY
Sample : P2566-03 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059058.D
Acq On : 29 May 2024 18:00
Operator : MD/SY
Sample : P2566-03 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------