

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059060.D
 Acq On : 29 May 2024 18:46
 Operator : MD/SY
 Sample : P2566-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.486	58	61	65	rVB3	912	636	0.10%	0.012%
2	1.596	88	95	113	rVB	76205	92750	14.44%	1.739%
3	1.759	140	146	158	rVB2	5236	7764	1.21%	0.146%
4	1.907	183	192	210	rBV	66930	90506	14.09%	1.697%
5	2.560	384	395	410	rBV	120709	198662	30.93%	3.725%
6	2.682	430	433	437	rBV2	362	323	0.05%	0.006%
7	2.740	443	451	452	rBV4	785	816	0.13%	0.015%
8	2.782	461	464	467	rBV2	613	579	0.09%	0.011%
9	2.830	474	479	481	rBV	286	237	0.04%	0.004%
10	2.927	506	509	514	rBV2	269	296	0.05%	0.006%
11	2.959	514	519	522	rVB3	292	287	0.04%	0.005%
12	3.039	535	544	551	rBV4	3520	5798	0.90%	0.109%
13	3.110	560	566	570	rBV2	229	314	0.05%	0.006%
14	3.184	584	589	595	rVB4	506	690	0.11%	0.013%
15	3.425	661	664	670	rVB	223	252	0.04%	0.005%
16	3.457	670	674	676	rBV2	217	198	0.03%	0.004%
17	3.586	710	714	719	rBV2	177	239	0.04%	0.004%
18	3.740	759	762	765	rBV	264	213	0.03%	0.004%
19	4.017	844	848	852	rVV2	349	337	0.05%	0.006%
20	4.042	852	856	859	rVB2	235	214	0.03%	0.004%
21	4.081	859	868	870	rBV	203	311	0.05%	0.006%
22	4.338	944	948	951	rBV2	225	191	0.03%	0.004%
23	4.435	974	978	982	rVB2	213	230	0.04%	0.004%
24	4.611	1023	1033	1066	rBV	75068	188095	29.28%	3.526%
25	5.055	1155	1171	1192	rVV	119738	265637	41.35%	4.980%
26	5.251	1230	1232	1237	rVB2	301	282	0.04%	0.005%
27	5.296	1243	1246	1253	rVB3	346	364	0.06%	0.007%
28	5.341	1253	1260	1264	rBV2	269	358	0.06%	0.007%
29	5.544	1319	1323	1326	rBV2	257	257	0.04%	0.005%
30	5.579	1331	1334	1341	rVB2	213	260	0.04%	0.005%
31	5.718	1356	1377	1403	rBV2	231119	642375	100.00%	12.044%
32	5.991	1459	1462	1466	rBV2	272	238	0.04%	0.004%
33	6.129	1499	1505	1507	rVB2	225	200	0.03%	0.004%
34	6.177	1513	1520	1525	rBV2	215	282	0.04%	0.005%
35	6.242	1528	1540	1567	rBV	252664	494601	77.00%	9.273%
36	6.534	1619	1631	1646	rBV4	17432	36730	5.72%	0.689%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059060.D
 Acq On : 29 May 2024 18:46
 Operator : MD/SY
 Sample : P2566-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.682	1662	1677	1704	rBV	152070	304129	47.34%	5.702%
38	6.923	1747	1752	1755	rBV2	219	217	0.03%	0.004%
39	6.984	1768	1771	1773	rBV2	327	229	0.04%	0.004%
40	7.052	1789	1792	1795	rBV2	338	290	0.05%	0.005%
41	7.107	1806	1809	1816	rBV2	208	307	0.05%	0.006%
42	7.203	1834	1839	1841	rBV3	219	259	0.04%	0.005%
43	7.299	1863	1869	1876	rVB2	327	488	0.08%	0.009%
44	7.335	1876	1880	1885	rBV2	305	299	0.05%	0.006%
45	7.380	1885	1894	1897	rBV2	241	358	0.06%	0.007%
46	7.560	1939	1950	1971	rBV	76558	137442	21.40%	2.577%
47	7.714	1996	1998	2001	rBV	419	231	0.04%	0.004%
48	7.891	2041	2053	2076	rVV	257065	456230	71.02%	8.554%
49	8.126	2123	2126	2128	rBV	332	254	0.04%	0.005%
50	8.177	2132	2142	2164	rBV	50553	89412	13.92%	1.676%
51	8.451	2222	2227	2229	rBV2	271	271	0.04%	0.005%
52	8.467	2229	2232	2240	rVB3	859	975	0.15%	0.018%
53	8.627	2271	2282	2316	rBV	173524	362312	56.40%	6.793%
54	8.949	2374	2382	2384	rBV	318	351	0.05%	0.007%
55	9.180	2450	2454	2458	rVB2	392	358	0.06%	0.007%
56	9.412	2514	2526	2557	rBV	371444	625755	97.41%	11.732%
57	9.637	2591	2596	2599	rVB2	295	253	0.04%	0.005%
58	9.669	2602	2606	2612	rBV2	364	438	0.07%	0.008%
59	9.698	2612	2615	2620	rBV3	357	323	0.05%	0.006%
60	9.775	2635	2639	2642	rBV	315	308	0.05%	0.006%
61	9.862	2662	2666	2671	rVB2	357	415	0.06%	0.008%
62	9.959	2689	2696	2703	rBV2	328	549	0.09%	0.010%
63	10.177	2758	2764	2766	rBV	189	196	0.03%	0.004%
64	10.235	2778	2782	2788	rVB2	259	323	0.05%	0.006%
65	10.370	2820	2824	2826	rBV	290	281	0.04%	0.005%
66	10.486	2858	2860	2863	rVB	367	199	0.03%	0.004%
67	10.528	2869	2873	2879	rBV	450	471	0.07%	0.009%
68	10.589	2890	2892	2897	rVB2	315	284	0.04%	0.005%
69	10.749	2930	2942	2964	rBV	227901	371246	57.79%	6.960%
70	10.878	2978	2982	2983	rBV	421	264	0.04%	0.005%
71	11.026	3023	3028	3029	rBV	231	217	0.03%	0.004%
72	11.479	3163	3169	3174	rBV3	212	245	0.04%	0.005%
73	11.743	3248	3251	3253	rVB2	366	212	0.03%	0.004%
74	11.807	3259	3271	3291	rBV	316726	532666	82.92%	9.987%
75	11.923	3305	3307	3311	rVB3	645	467	0.07%	0.009%
76	11.946	3311	3314	3315	rBV2	357	207	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059060.D
 Acq On : 29 May 2024 18:46
 Operator : MD/SY
 Sample : P2566-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.994	3326	3329	3333	rBV3	438	363	0.06%	0.007%
78	12.110	3361	3365	3367	rBV2	278	222	0.03%	0.004%
79	12.187	3377	3389	3409	rBV	237608	404913	63.03%	7.591%
80	12.335	3433	3435	3438	rVB3	503	254	0.04%	0.005%
81	12.929	3616	3620	3626	rBV2	337	455	0.07%	0.009%
82	12.968	3630	3632	3639	rVB	605	436	0.07%	0.008%
83	13.003	3639	3643	3644	rBV	271	204	0.03%	0.004%
84	13.200	3701	3704	3707	rBV	245	190	0.03%	0.004%
85	13.245	3715	3718	3723	rVB2	444	344	0.05%	0.006%
86	13.280	3723	3729	3732	rBV2	333	430	0.07%	0.008%
87	13.344	3744	3749	3751	rBV	233	264	0.04%	0.005%
88	13.431	3773	3776	3778	rBV	249	196	0.03%	0.004%
89	13.724	3864	3867	3870	rBV2	391	353	0.05%	0.007%
90	14.122	3988	3991	3996	rBV3	440	435	0.07%	0.008%
91	14.315	4048	4051	4056	rBV	251	243	0.04%	0.005%
92	14.376	4066	4070	4074	rBV2	356	362	0.06%	0.007%
93	14.499	4104	4108	4112	rBV	368	328	0.05%	0.006%
94	14.579	4130	4133	4135	rBV	479	301	0.05%	0.006%
95	14.756	4186	4188	4193	rVB2	325	253	0.04%	0.005%
96	14.913	4231	4237	4240	rBV	585	618	0.10%	0.012%
97	15.916	4547	4549	4552	rBV3	403	275	0.04%	0.005%
98	16.109	4606	4609	4610	rBV	466	245	0.04%	0.005%
99	16.328	4674	4677	4680	rBV3	452	335	0.05%	0.006%
100	16.627	4766	4770	4771	rBV2	721	506	0.08%	0.009%




Sum of corrected areas: 5333778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059060.D
Acq On : 29 May 2024 18:46
Operator : MD/SY
Sample : P2566-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

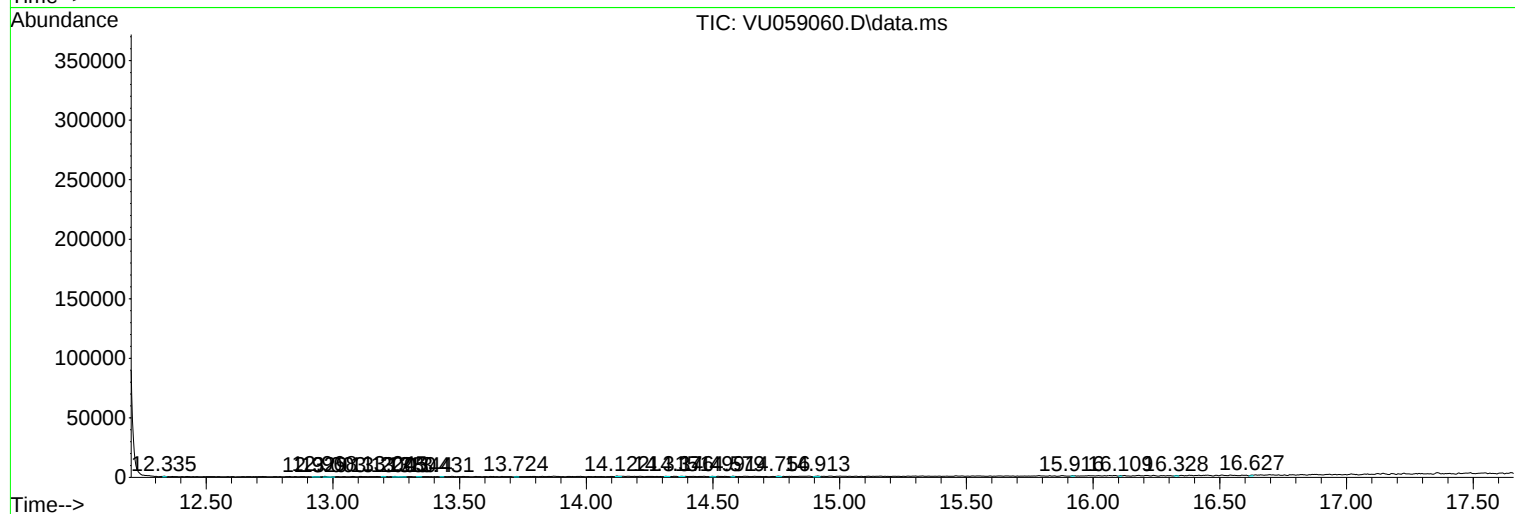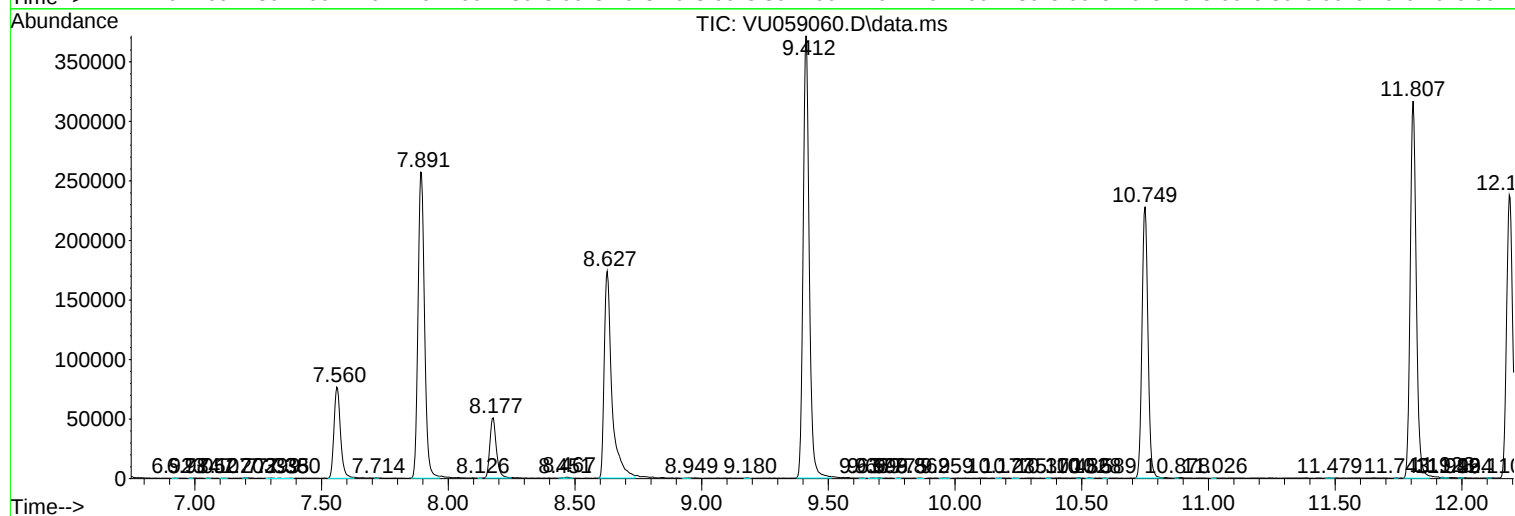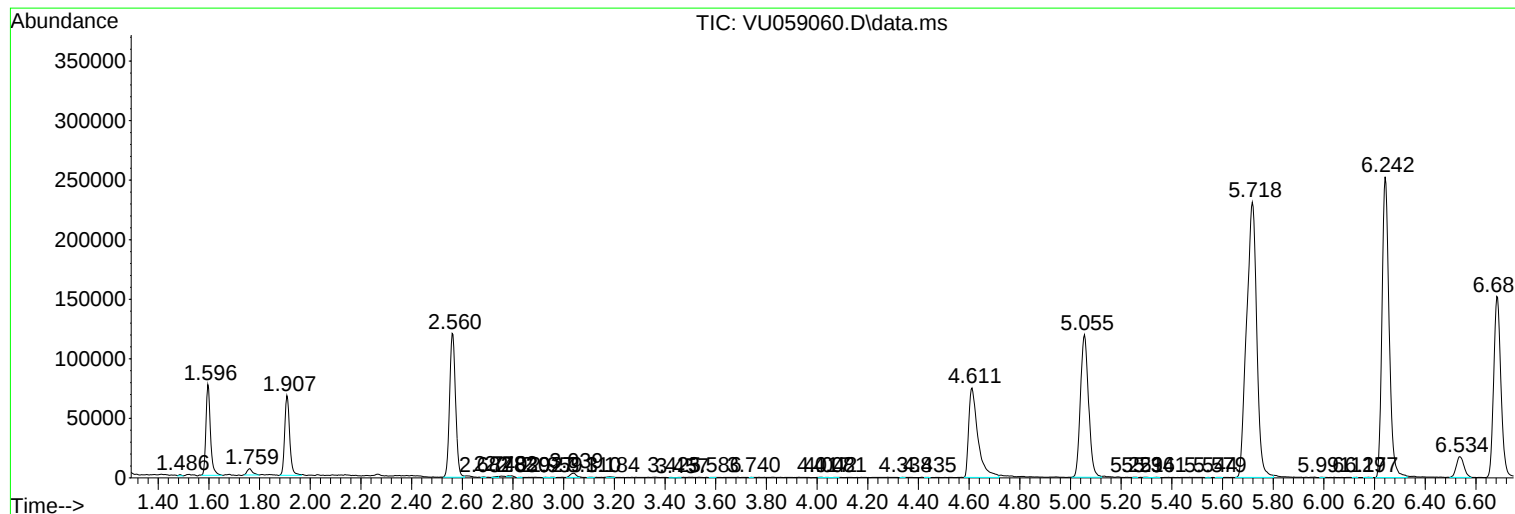

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059060.D
Acq On : 29 May 2024 18:46
Operator : MD/SY
Sample : P2566-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059060.D
Acq On : 29 May 2024 18:46
Operator : MD/SY
Sample : P2566-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------