

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059061.D
 Acq On : 29 May 2024 19:09
 Operator : MD/SY
 Sample : P2591-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	115	rBV	75482	90847	14.28%	1.744%
2	1.763	140	147	157	rVB3	6093	7863	1.24%	0.151%
3	1.907	184	192	210	rVB	65146	88823	13.96%	1.705%
4	2.560	384	395	410	rBV	119502	194060	30.50%	3.725%
5	2.737	446	450	451	rBV2	594	374	0.06%	0.007%
6	2.975	518	524	528	rBV	199	247	0.04%	0.005%
7	3.039	536	544	554	rBV4	1985	3463	0.54%	0.066%
8	3.158	578	581	582	rBV	521	276	0.04%	0.005%
9	3.271	613	616	621	rVB2	326	264	0.04%	0.005%
10	3.673	731	741	745	rBV2	333	568	0.09%	0.011%
11	4.139	881	886	889	rBV2	205	212	0.03%	0.004%
12	4.171	889	896	902	rVV2	383	592	0.09%	0.011%
13	4.226	908	913	916	rBV2	246	265	0.04%	0.005%
14	4.271	922	927	932	rVV2	162	225	0.04%	0.004%
15	4.319	936	942	948	rBV2	211	280	0.04%	0.005%
16	4.611	1023	1033	1066	rBV	73315	185418	29.15%	3.559%
17	4.978	1144	1147	1152	rBV2	206	204	0.03%	0.004%
18	5.055	1156	1171	1199	rVB	115951	260988	41.03%	5.010%
19	5.193	1211	1214	1218	rBV4	330	259	0.04%	0.005%
20	5.219	1220	1222	1227	rVB3	501	342	0.05%	0.007%
21	5.560	1321	1328	1329	rBV	266	253	0.04%	0.005%
22	5.618	1343	1346	1352	rBV2	229	267	0.04%	0.005%
23	5.718	1357	1377	1409	rVV2	231884	636164	100.00%	12.212%
24	6.197	1519	1526	1528	rBV2	294	303	0.05%	0.006%
25	6.242	1528	1540	1568	rBV	246879	472980	74.35%	9.080%
26	6.396	1583	1588	1590	rBV2	259	254	0.04%	0.005%
27	6.467	1605	1610	1611	rBV3	332	275	0.04%	0.005%
28	6.476	1611	1613	1615	rVV	315	193	0.03%	0.004%
29	6.489	1615	1617	1620	rVV	399	288	0.05%	0.006%
30	6.537	1620	1632	1646	rVB5	11295	24656	3.88%	0.473%
31	6.615	1651	1656	1658	rBV2	262	191	0.03%	0.004%
32	6.682	1664	1677	1707	rVV	150682	300308	47.21%	5.765%
33	6.785	1707	1709	1713	rVV2	331	208	0.03%	0.004%
34	6.808	1713	1716	1720	rVB	556	436	0.07%	0.008%
35	6.853	1726	1730	1733	rBV2	222	273	0.04%	0.005%
36	7.017	1778	1781	1785	rVB2	275	261	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059061.D
 Acq On : 29 May 2024 19:09
 Operator : MD/SY
 Sample : P2591-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.171	1823	1829	1833	rBV	231	368	0.06%	0.007%
38	7.190	1833	1835	1841	rVV2	253	279	0.04%	0.005%
39	7.219	1841	1844	1847	rVB2	333	271	0.04%	0.005%
40	7.235	1847	1849	1853	rBV2	308	273	0.04%	0.005%
41	7.277	1858	1862	1867	rBV2	314	377	0.06%	0.007%
42	7.319	1870	1875	1880	rBV2	228	290	0.05%	0.006%
43	7.560	1937	1950	1972	rBV	72317	132156	20.77%	2.537%
44	7.891	2041	2053	2081	rBV	257798	454458	71.44%	8.724%
45	8.074	2106	2110	2113	rVB3	398	298	0.05%	0.006%
46	8.174	2130	2141	2161	rBV	48945	86442	13.59%	1.659%
47	8.270	2168	2171	2178	rVB3	579	647	0.10%	0.012%
48	8.463	2222	2231	2238	rBV3	573	897	0.14%	0.017%
49	8.537	2252	2254	2261	rVB2	224	245	0.04%	0.005%
50	8.627	2268	2282	2331	rBV2	173355	365996	57.53%	7.026%
51	9.103	2427	2430	2435	rBV2	192	229	0.04%	0.004%
52	9.264	2474	2480	2485	rVB2	299	394	0.06%	0.008%
53	9.306	2485	2493	2496	rBV2	319	364	0.06%	0.007%
54	9.412	2513	2526	2554	rBV	358726	606535	95.34%	11.644%
55	9.576	2573	2577	2580	rVB3	422	344	0.05%	0.007%
56	9.923	2680	2685	2687	rBV2	186	196	0.03%	0.004%
57	9.955	2691	2695	2698	rVB2	438	334	0.05%	0.006%
58	10.065	2725	2729	2733	rBV	400	417	0.07%	0.008%
59	10.174	2760	2763	2765	rBV	291	230	0.04%	0.004%
60	10.299	2798	2802	2807	rBV2	264	298	0.05%	0.006%
61	10.396	2827	2832	2837	rBV	366	366	0.06%	0.007%
62	10.557	2878	2882	2885	rBV2	356	338	0.05%	0.006%
63	10.611	2896	2899	2904	rBV	230	199	0.03%	0.004%
64	10.659	2910	2914	2918	rBV	280	297	0.05%	0.006%
65	10.749	2929	2942	2966	rBV	225454	364418	57.28%	6.996%
66	10.888	2980	2985	2987	rBV2	464	471	0.07%	0.009%
67	11.032	3027	3030	3033	rBV2	290	275	0.04%	0.005%
68	11.058	3036	3038	3045	rVB2	207	194	0.03%	0.004%
69	11.151	3063	3067	3072	rBV2	330	343	0.05%	0.007%
70	11.364	3126	3133	3135	rBV2	244	316	0.05%	0.006%
71	11.457	3157	3162	3167	rBV2	344	419	0.07%	0.008%
72	11.749	3248	3253	3259	rBV3	583	643	0.10%	0.012%
73	11.807	3259	3271	3294	rBV	306744	515210	80.99%	9.890%
74	11.910	3299	3303	3307	rVB3	624	631	0.10%	0.012%
75	12.007	3330	3333	3336	rVB2	495	306	0.05%	0.006%
76	12.061	3345	3350	3354	rBV2	291	375	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
 Data File : VU059061.D
 Acq On : 29 May 2024 19:09
 Operator : MD/SY
 Sample : P2591-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.090	3356	3359	3363	rVB2	435	326	0.05%	0.006%
78	12.119	3363	3368	3370	rBV2	299	302	0.05%	0.006%
79	12.190	3377	3390	3408	rBV	228299	391886	61.60%	7.523%
80	12.331	3431	3434	3438	rBV2	392	248	0.04%	0.005%
81	12.470	3474	3477	3481	rBV3	303	239	0.04%	0.005%
82	12.495	3482	3485	3493	rVV2	293	290	0.05%	0.006%
83	12.727	3554	3557	3562	rVB	343	283	0.04%	0.005%
84	12.814	3581	3584	3587	rBV2	270	197	0.03%	0.004%
85	12.904	3608	3612	3615	rBV	344	315	0.05%	0.006%
86	13.145	3681	3687	3688	rBV2	229	243	0.04%	0.005%
87	13.277	3723	3728	3732	rBV2	315	331	0.05%	0.006%
88	13.511	3799	3801	3807	rVV2	217	252	0.04%	0.005%
89	13.566	3813	3818	3822	rBV2	361	477	0.07%	0.009%
90	13.691	3855	3857	3862	rBV2	299	220	0.03%	0.004%
91	14.264	4031	4035	4036	rBV	383	270	0.04%	0.005%
92	14.666	4157	4160	4163	rBV2	327	237	0.04%	0.005%
93	14.733	4178	4181	4184	rBV3	329	235	0.04%	0.005%
94	14.801	4199	4202	4207	rBV2	496	512	0.08%	0.010%
95	14.974	4254	4256	4262	rBV3	282	282	0.04%	0.005%
96	15.071	4284	4286	4289	rBV2	334	210	0.03%	0.004%
97	15.990	4569	4572	4575	rBV3	624	458	0.07%	0.009%
98	16.296	4664	4667	4668	rBV2	722	414	0.07%	0.008%
99	16.457	4715	4717	4718	rBV2	519	214	0.03%	0.004%
100	16.801	4821	4824	4828	rBV5	1012	748	0.12%	0.014%




Sum of corrected areas: 5209208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059061.D
Acq On : 29 May 2024 19:09
Operator : MD/SY
Sample : P2591-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

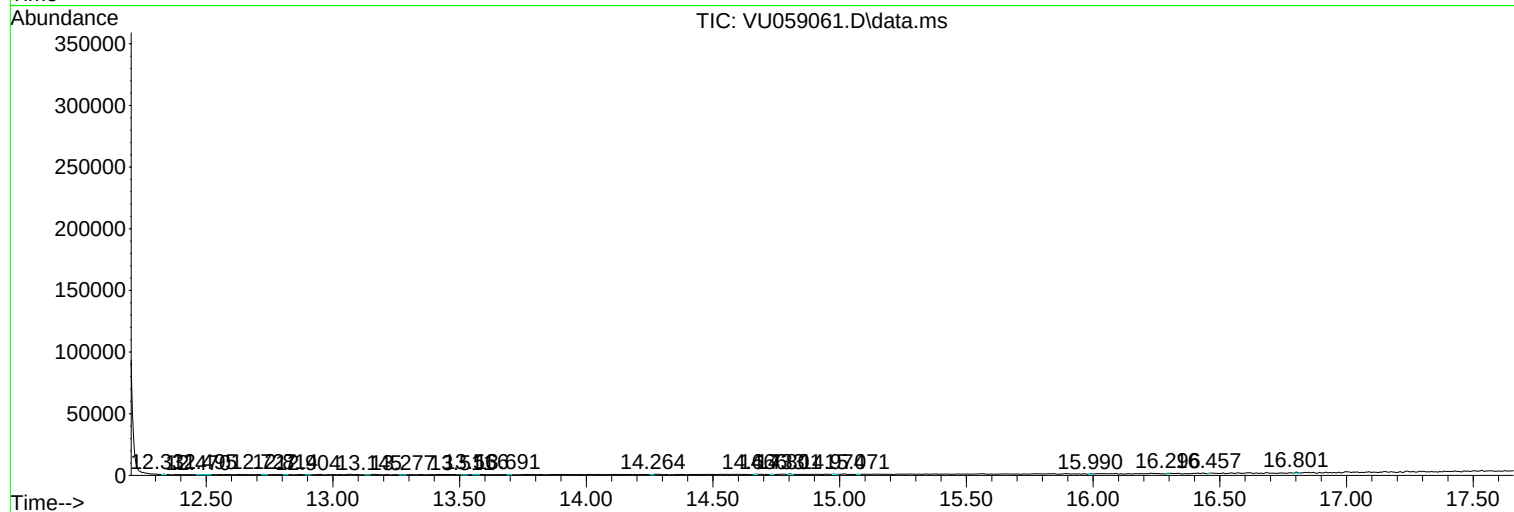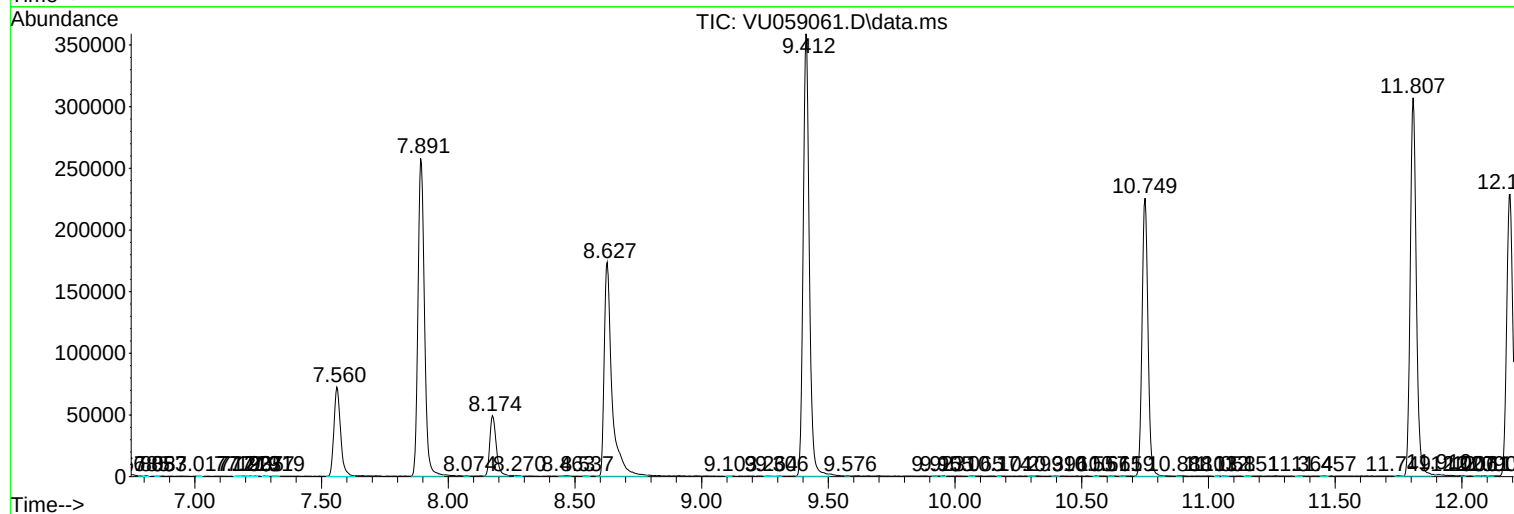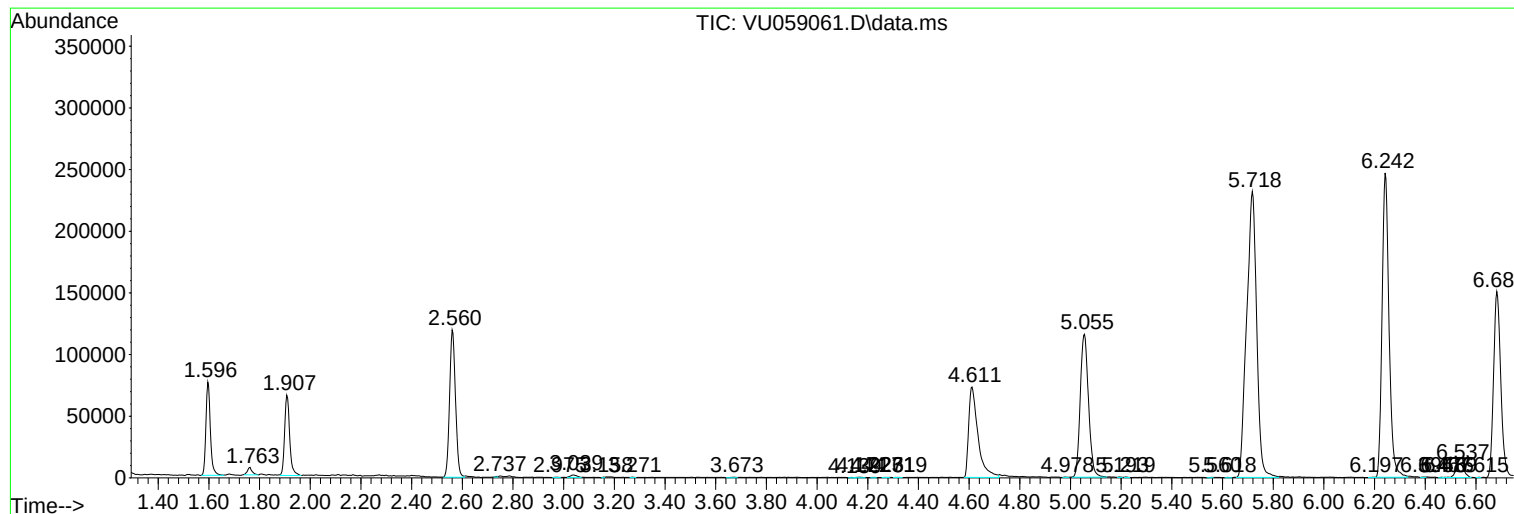

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059061.D
Acq On : 29 May 2024 19:09
Operator : MD/SY
Sample : P2591-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052924\
Data File : VU059061.D
Acq On : 29 May 2024 19:09
Operator : MD/SY
Sample : P2591-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------