


Data Path : W:\HPCHEM1\MSVOA U\Data\VU053018\
 Data File : VU024234.D
 Acq On : 30 May 2018 11:04
 Operator : MD/SY
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM052518WMA.M
 Title : VOC Analysis
 Last Update : Thu May 31 03:53:12 2018

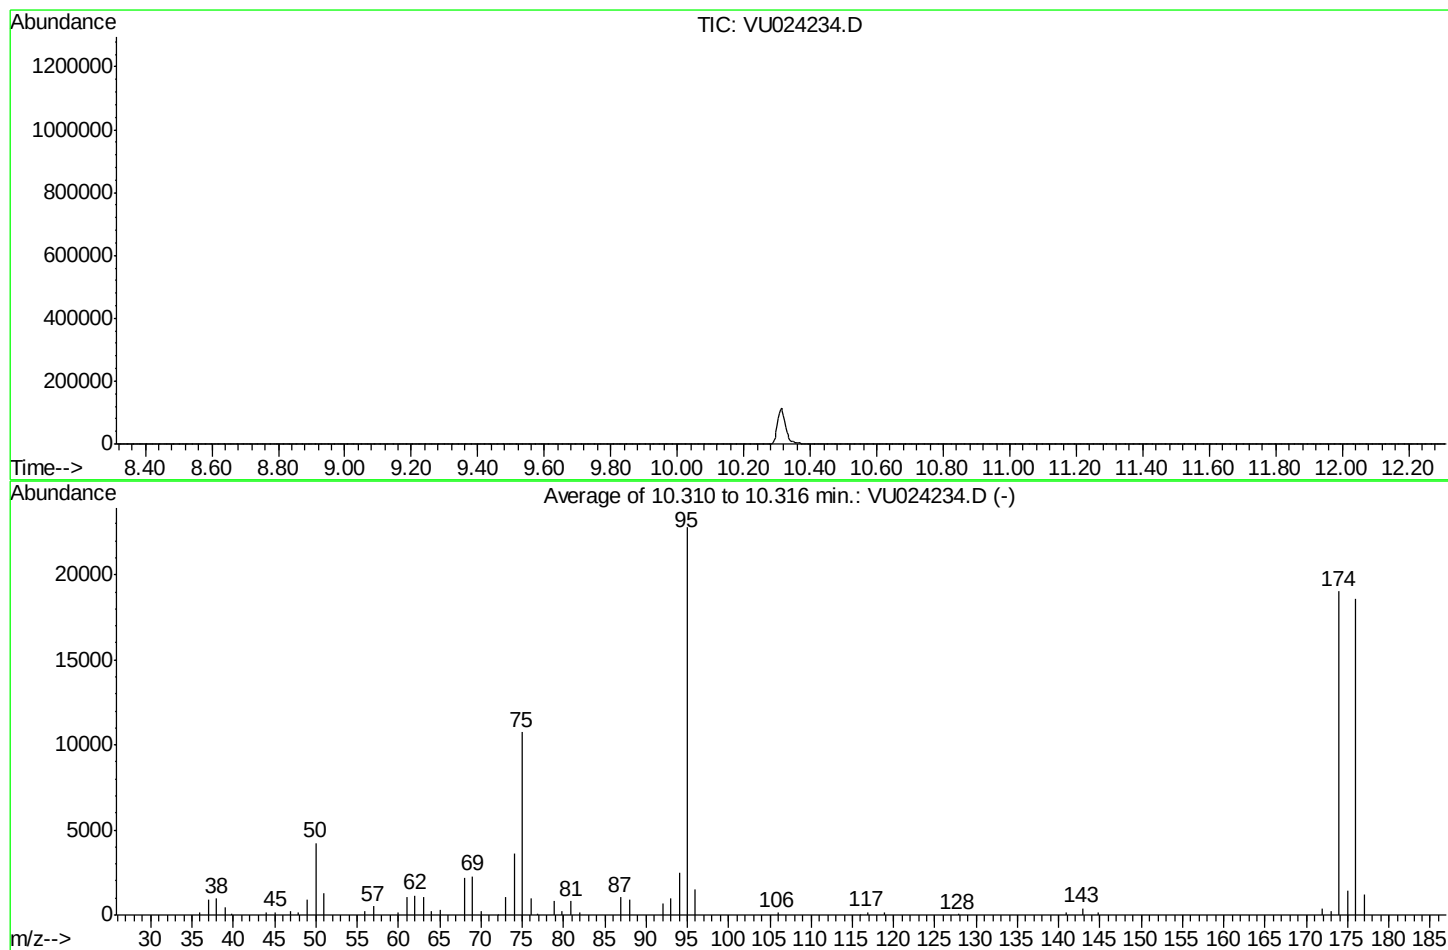

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	4254	PASS
75	95	30	80	47.2	10749	PASS
95	95	100	100	100.0	22794	PASS
96	95	5	9	6.6	1500	PASS
173	174	0.00	2	1.2	219	PASS
174	95	50	120	83.5	19026	PASS
175	174	5	9	7.6	1442	PASS
176	174	95	101	97.7	18592	PASS
177	176	5	9	6.3	1170	PASS

Scan 3012 (10.275 min): VU024234.D
BFB42

m/z	Abundance
44.00	462.0

m/z	Abundance
35.00	187.0
37.00	969.0
38.00	937.0
39.00	461.0
44.00	562.0
45.10	217.0
46.90	281.0
47.90	136.0
49.00	878.0
50.00	4137.0
51.00	1334.0
56.00	269.0
57.00	576.0
60.00	191.0
61.00	1147.0
62.00	1154.0
63.00	1095.0
64.00	273.0
65.00	363.0
68.00	2289.0
69.00	2262.0
70.00	203.0
72.00	108.0
73.00	1123.0
74.00	3567.0
75.00	10949.0
76.00	1041.0
76.80	148.0
78.90	805.0
79.80	213.0
80.90	805.0
82.00	141.0
86.90	1019.0
88.00	949.0
92.00	659.0
93.00	992.0
94.00	2493.0
95.00	23480.0
96.00	1645.0
106.00	109.0
115.90	104.0
116.90	166.0
118.80	130.0
141.00	192.0
142.90	404.0
144.80	135.0
172.00	331.0
173.00	219.0
173.90	18528.0
175.00	1413.0
175.90	18544.0
177.00	1204.0

m/z	Abundance
35.90	202.0
37.00	897.0
38.00	983.0
39.00	481.0
39.90	121.0
44.00	597.0
45.10	164.0
46.90	264.0
47.90	140.0
49.00	911.0
50.00	4383.0
51.00	1315.0
56.00	264.0
57.00	519.0
60.00	165.0
61.00	1086.0
62.00	1197.0
63.00	1138.0
64.00	241.0
65.00	335.0
68.00	2225.0
69.00	2358.0
70.00	230.0
73.00	1085.0
74.00	3720.0
75.00	11081.0
76.10	976.0
76.80	130.0
78.90	873.0
79.80	230.0
80.90	822.0
81.90	143.0
86.90	1058.0
88.00	920.0
92.00	717.0
93.00	1005.0
94.00	2513.0
95.00	23520.0
96.00	1539.0
106.00	136.0
116.90	158.0
118.90	145.0
127.80	104.0
141.00	145.0
142.90	386.0
144.80	140.0
172.00	359.0
173.10	234.0
174.00	19568.0
175.00	1497.0
176.00	19200.0
177.00	1207.0

m/z	Abundance
35.90	180.0
37.00	851.0
38.00	930.0
38.90	458.0
39.80	139.0
44.00	581.0
45.00	101.0
47.00	226.0
47.90	108.0
49.00	825.0
50.00	4244.0
51.00	1226.0
56.00	243.0
57.00	453.0
59.90	178.0
61.00	964.0
62.00	1057.0
63.00	1048.0
64.00	217.0
65.00	286.0
68.00	2059.0
69.00	2225.0
70.00	217.0
73.00	920.0
74.00	3547.0
75.00	10218.0
76.10	905.0
78.90	830.0
79.90	203.0
80.90	757.0
81.90	159.0
86.90	984.0
88.00	849.0
92.00	696.0
93.00	896.0
94.00	2423.0
95.00	21384.0
96.00	1317.0
105.90	129.0
116.80	150.0
118.90	142.0
127.80	110.0
140.90	157.0
142.90	386.0
144.80	135.0
171.90	356.0
173.00	204.0
174.00	18984.0
175.00	1416.0
176.00	18032.0
176.90	1100.0