

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053019\
 Data File : VU032387.D
 Acq On : 30 May 2019 17:22
 Operator : JC/SP
 Sample : K3017-20ME
 Misc : 3.39g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A51F1ME

Manual Integrations
 APPROVED

MMDadoda
 5/31/2019 10:29:13 AM

Quant Time: Jun 14 05:39:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 04:34:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	793583	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	813262	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	402404	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	226213	38.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.34%
7) Chloroethane-d5	1.64	69	145403	30.78	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	61.56%#
11) 1,1-Dichloroethene-d2	2.23	63	340950m	32.81	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.62%
21) 2-Butanone-d5	4.19	46	424524	110.28	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.28%
24) Chloroform-d	4.64	84	472171	46.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.24%
26) 1,2-Dichloroethane-d4	5.30	65	299761	49.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.96%
32) Benzene-d6	5.33	84	1002067	46.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.96%
36) 1,2-Dichloropropane-d6	6.32	67	312514	47.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.40%
41) Toluene-d8	7.56	98	915615	46.01	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.02%
43) trans-1,3-Dichloropropene-	7.85	79	141912	46.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.60%
47) 2-Hexanone-d5	8.32	63	378429	136.22	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	136.22%#
57) 1,1,2,2-Tetrachloroethane-	10.43	84	529924	52.38	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.76%
64) 1,2-Dichlorobenzene-d4	11.86	152	400627	48.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.64%

Target Compounds				Ovalue
15) Methyl Acetate	2.62	43	158145	27.277 ug/L 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU053019\
Data File : VU032387.D
Acq On : 30 May 2019 17:22
Operator : JC/SP
Sample : K3017-20ME
Misc : 3.39g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
A51F1ME

Manual Integrations
APPROVED

MMDadoda
5/31/2019 10:29:13 AM

Quant Time: Jun 14 05:39:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 04:34:14 2019
Response via : Initial Calibration

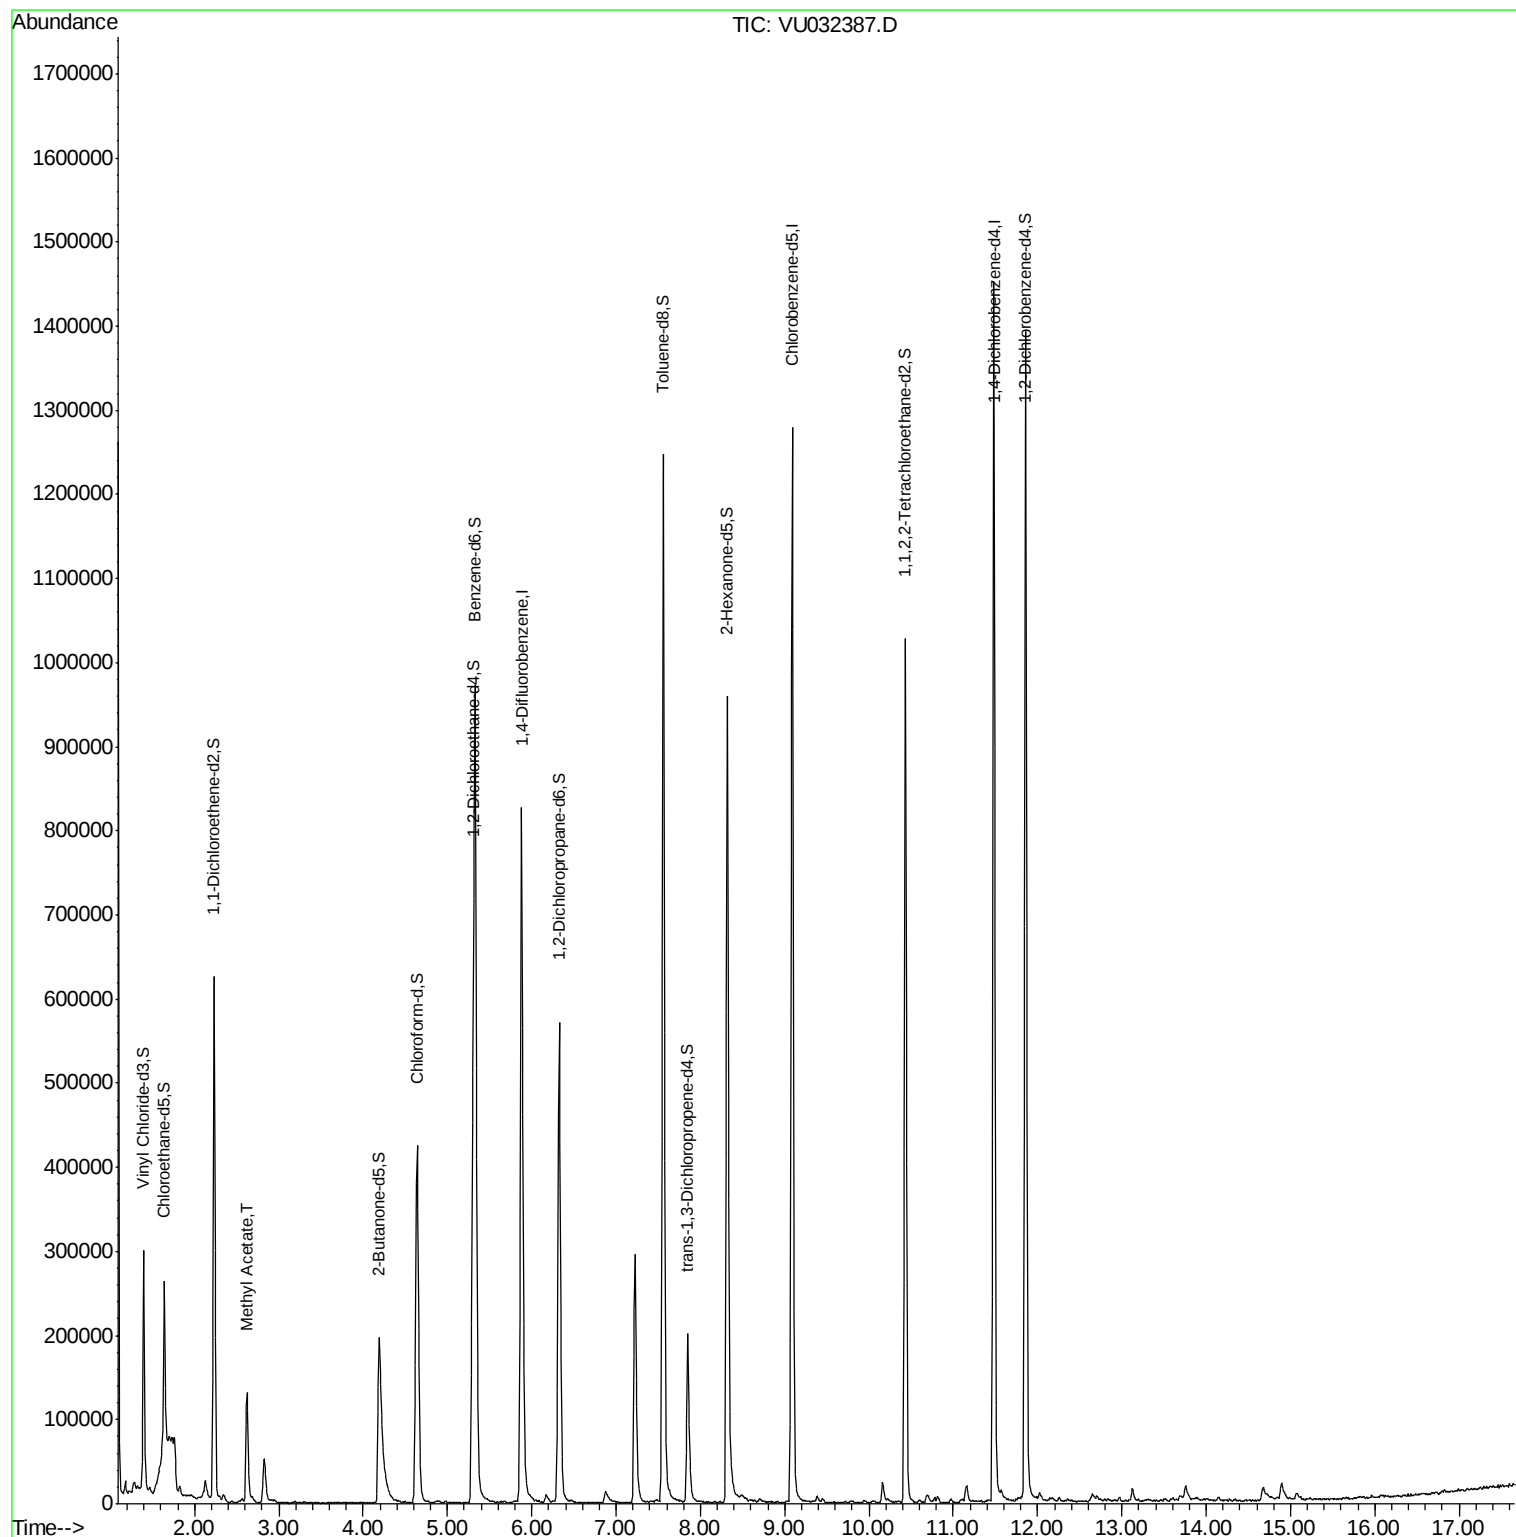

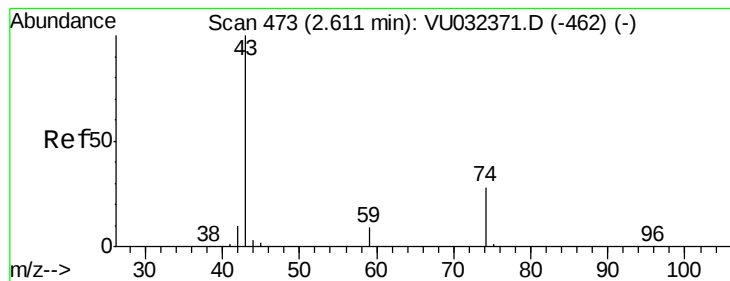

#15

Methyl Acetate

Concen: 27.277 ug/L

RT: 2.62 min Scan# 476

Delta R.T. 0.01 min

Lab File: VU032387.D

Acq: 30 May 2019 17:22

Tot Ion: 43 Resp: 158145

Ion Ratio Lower Upper

43 100

74 28.4 21.1 31.7

Instrument :

MSVOA_U

ClientSampleId :

A51F1ME

Manual Integrations

APPROVED

MMDadoda

5/31/2019 10:29:13 AM

